

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028410.D
 Acq On : 07 Oct 2022 16:24
 Operator : SY/MD
 Sample : N4893-09DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J06DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028410.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	205681	217517	11.95%	1.504%
2	1.564	157	163	177	rVB	180481	205060	11.26%	1.418%
3	2.101	322	330	343	rVB	352578	495320	27.20%	3.426%
4	2.892	573	576	580	rBV5	1112	1122	0.06%	0.008%
5	3.063	626	629	635	rBV7	970	899	0.05%	0.006%
6	3.114	642	645	647	rBV3	940	621	0.03%	0.004%
7	3.175	662	664	667	rBV3	957	496	0.03%	0.003%
8	3.384	726	729	735	rVB6	666	611	0.03%	0.004%
9	3.465	750	754	758	rBV4	1657	1159	0.06%	0.008%
10	3.651	810	812	815	rBV3	932	643	0.04%	0.004%
11	3.712	828	831	833	rBV3	818	580	0.03%	0.004%
12	3.741	836	840	842	rBV3	723	520	0.03%	0.004%
13	3.818	862	864	870	rVB4	866	619	0.03%	0.004%
14	3.847	872	873	876	rBV4	730	508	0.03%	0.004%
15	3.905	879	891	951	rVV	105359	542660	29.80%	3.753%
16	4.342	1014	1027	1052	rVB2	269162	672303	36.92%	4.650%
17	4.719	1141	1144	1145	rBV2	988	505	0.03%	0.003%
18	4.809	1169	1172	1174	rBV3	915	606	0.03%	0.004%
19	4.821	1174	1176	1178	rVB2	1010	469	0.03%	0.003%
20	4.831	1178	1179	1182	rBV2	678	464	0.03%	0.003%
21	4.924	1205	1208	1209	rBV2	1230	781	0.04%	0.005%
22	5.040	1228	1244	1278	rBV2	719410	1820767	100.00%	12.593%
23	5.419	1359	1362	1363	rBV3	1316	718	0.04%	0.005%
24	5.474	1376	1379	1381	rBV2	685	484	0.03%	0.003%
25	5.612	1410	1422	1453	rBV	527785	1067571	58.63%	7.383%
26	5.908	1503	1514	1530	rBV10	9904	25831	1.42%	0.179%
27	6.066	1550	1563	1593	rBV	409113	842607	46.28%	5.828%
28	6.429	1672	1676	1679	rBV5	903	642	0.04%	0.004%
29	6.474	1684	1690	1694	rBV8	944	1143	0.06%	0.008%
30	6.677	1750	1753	1756	rBV4	2122	1275	0.07%	0.009%
31	6.889	1815	1819	1822	rBV5	1128	752	0.04%	0.005%
32	6.918	1826	1828	1830	rBV2	1076	614	0.03%	0.004%
33	6.934	1830	1833	1835	rBV3	853	425	0.02%	0.003%
34	6.982	1837	1848	1870	rBV	250587	461488	25.35%	3.192%
35	7.243	1926	1929	1931	rBV3	1203	695	0.04%	0.005%
36	7.310	1939	1950	1980	rBV	843466	1454037	79.86%	10.056%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100722\
 Data File : VW028410.D
 Acq On : 07 Oct 2022 16:24
 Operator : SY/MD
 Sample : N4893-09DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J06DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.616	2036	2045	2069	rBV	168823	304077	16.70%	2.103%
38	7.921	2136	2140	2141	rBV2	948	565	0.03%	0.004%
39	7.969	2142	2155	2172	rBV	394063	655830	36.02%	4.536%
40	8.085	2182	2191	2222	rBV	562047	1073708	58.97%	7.426%
41	8.616	2355	2356	2360	rBV3	510	389	0.02%	0.003%
42	8.844	2416	2427	2458	rVV	737834	1232504	67.69%	8.524%
43	9.130	2513	2516	2518	rBV4	866	472	0.03%	0.003%
44	9.181	2528	2532	2534	rVB5	962	571	0.03%	0.004%
45	9.194	2534	2536	2543	rVB7	885	873	0.05%	0.006%
46	9.352	2580	2585	2587	rBV5	937	639	0.04%	0.004%
47	9.361	2587	2588	2594	rVV5	746	718	0.04%	0.005%
48	9.429	2607	2609	2615	rBV6	815	837	0.05%	0.006%
49	9.497	2627	2630	2633	rBV4	771	509	0.03%	0.004%
50	9.519	2633	2637	2638	rVV4	1093	676	0.04%	0.005%
51	9.545	2642	2645	2650	rVV6	884	887	0.05%	0.006%
52	9.567	2650	2652	2658	rVB5	662	637	0.03%	0.004%
53	9.664	2679	2682	2683	rBV2	881	454	0.02%	0.003%
54	9.738	2702	2705	2709	rVB4	1143	768	0.04%	0.005%
55	9.876	2743	2748	2749	rBV4	784	472	0.03%	0.003%
56	9.902	2753	2756	2757	rBV2	875	530	0.03%	0.004%
57	9.966	2773	2776	2779	rBV4	684	425	0.02%	0.003%
58	10.008	2786	2789	2795	rVB8	1035	1005	0.06%	0.007%
59	10.056	2801	2804	2806	rBV4	634	460	0.03%	0.003%
60	10.069	2806	2808	2811	rBV3	694	551	0.03%	0.004%
61	10.107	2817	2820	2821	rBV3	721	379	0.02%	0.003%
62	10.133	2825	2828	2830	rBV3	802	574	0.03%	0.004%
63	10.210	2839	2852	2882	rBV	554313	886020	48.66%	6.128%
64	10.374	2899	2903	2908	rBV6	1190	1268	0.07%	0.009%
65	10.461	2927	2930	2933	rBV5	1233	723	0.04%	0.005%
66	10.538	2950	2954	2957	rVV6	984	744	0.04%	0.005%
67	10.767	3020	3025	3028	rBV6	1106	912	0.05%	0.006%
68	10.812	3036	3039	3041	rBV4	892	513	0.03%	0.004%
69	10.956	3079	3084	3085	rBV5	938	748	0.04%	0.005%
70	11.181	3150	3154	3155	rBV3	751	491	0.03%	0.003%
71	11.239	3161	3172	3193	rBV	768443	1198574	65.83%	8.290%
72	11.615	3277	3289	3310	rBV	787609	1247292	68.50%	8.626%
73	11.776	3336	3339	3341	rBV3	892	647	0.04%	0.004%
74	11.863	3362	3366	3369	rVB3	910	700	0.04%	0.005%
75	11.879	3369	3371	3373	rBV3	760	405	0.02%	0.003%
76	11.956	3390	3395	3399	rVB6	830	799	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028410.D
 Acq On : 07 Oct 2022 16:24
 Operator : SY/MD
 Sample : N4893-09DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J06DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.979	3399	3402	3403	rBV3	721	428	0.02%	0.003%
78	12.037	3416	3420	3423	rBV5	1055	815	0.04%	0.006%
79	12.088	3433	3436	3438	rBV3	1008	615	0.03%	0.004%
80	12.143	3450	3453	3454	rBV3	685	396	0.02%	0.003%
81	12.233	3475	3481	3482	rBV5	1190	899	0.05%	0.006%
82	12.342	3512	3515	3520	rBV4	1033	690	0.04%	0.005%
83	12.368	3520	3523	3526	rVB4	1208	696	0.04%	0.005%
84	12.387	3526	3529	3530	rBV3	1092	584	0.03%	0.004%
85	12.525	3569	3572	3574	rBV3	551	386	0.02%	0.003%
86	12.593	3588	3593	3597	rBV6	1071	939	0.05%	0.006%
87	12.680	3617	3620	3623	rBV5	1079	1000	0.05%	0.007%
88	12.760	3641	3645	3647	rBV4	723	627	0.03%	0.004%
89	12.828	3662	3666	3670	rVB7	937	743	0.04%	0.005%
90	12.892	3683	3686	3687	rBV2	950	524	0.03%	0.004%
91	12.992	3713	3717	3719	rBV4	1028	798	0.04%	0.006%
92	13.085	3743	3746	3749	rBV4	598	467	0.03%	0.003%
93	13.136	3760	3762	3769	rVB7	1046	1178	0.06%	0.008%
94	13.175	3771	3774	3776	rBV4	870	492	0.03%	0.003%
95	13.207	3781	3784	3786	rBV4	786	564	0.03%	0.004%
96	13.246	3794	3796	3799	rBV3	722	447	0.02%	0.003%
97	13.310	3813	3816	3820	rBV7	814	535	0.03%	0.004%
98	14.101	4060	4062	4070	rVB5	1285	1035	0.06%	0.007%
99	14.451	4168	4171	4174	rBV5	1100	859	0.05%	0.006%
100	14.683	4239	4243	4247	rBV7	1227	1345	0.07%	0.009%




Sum of corrected areas: 14458920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028410.D
Acq On : 07 Oct 2022 16:24
Operator : SY/MD
Sample : N4893-09DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J06DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

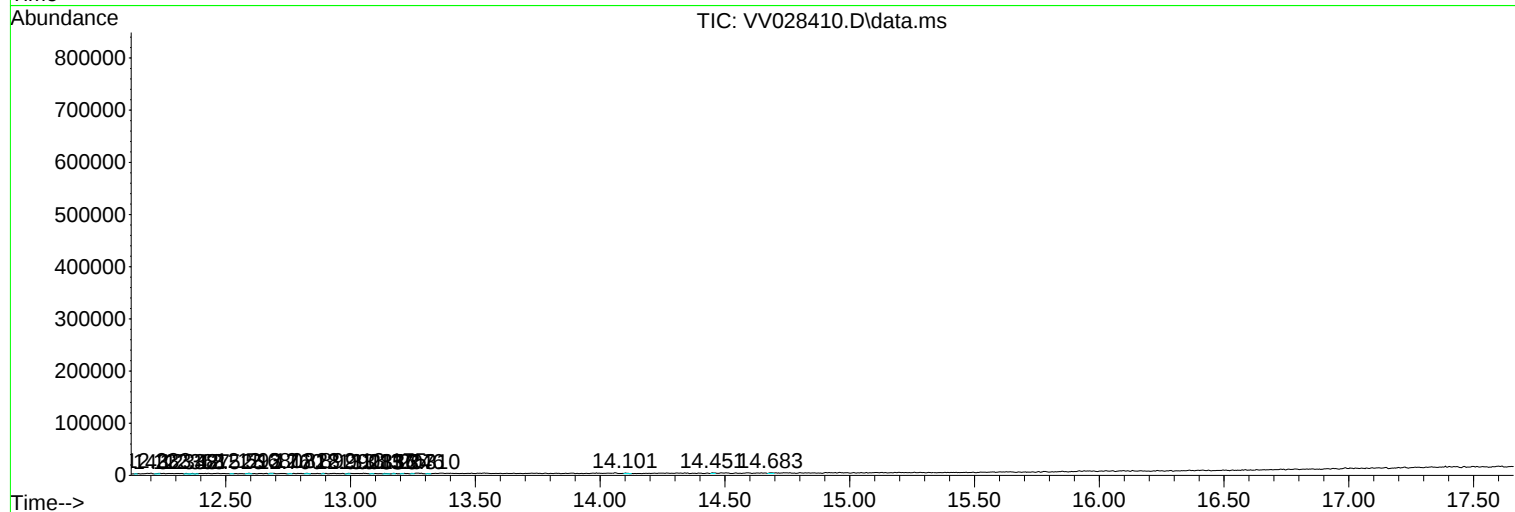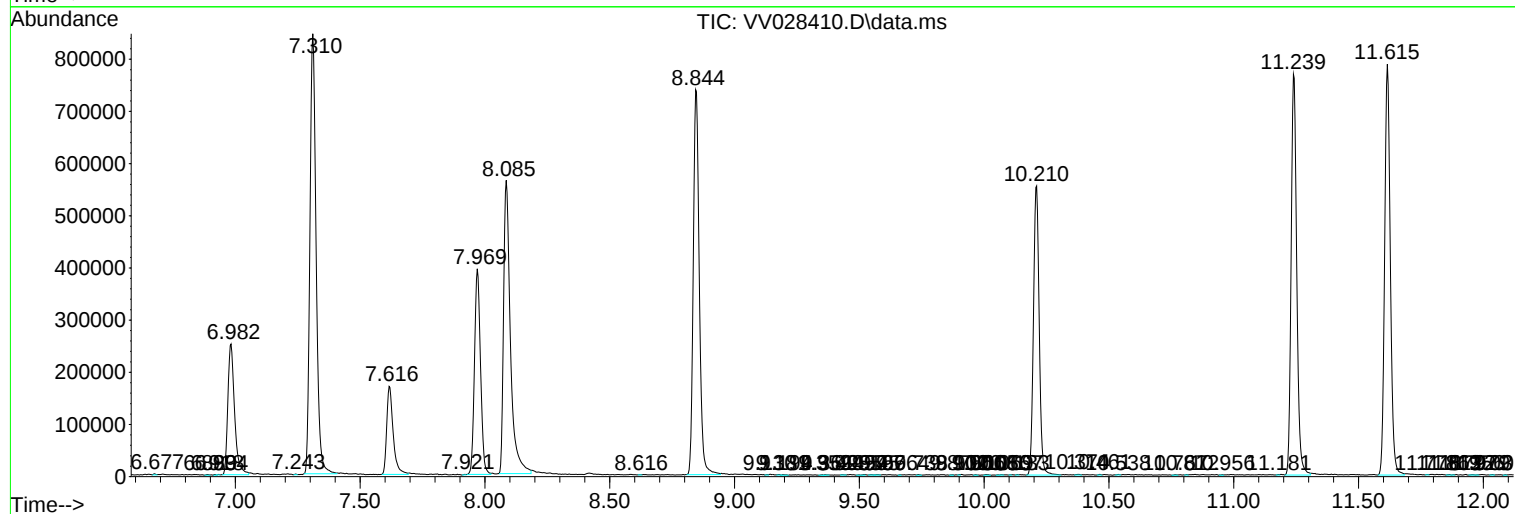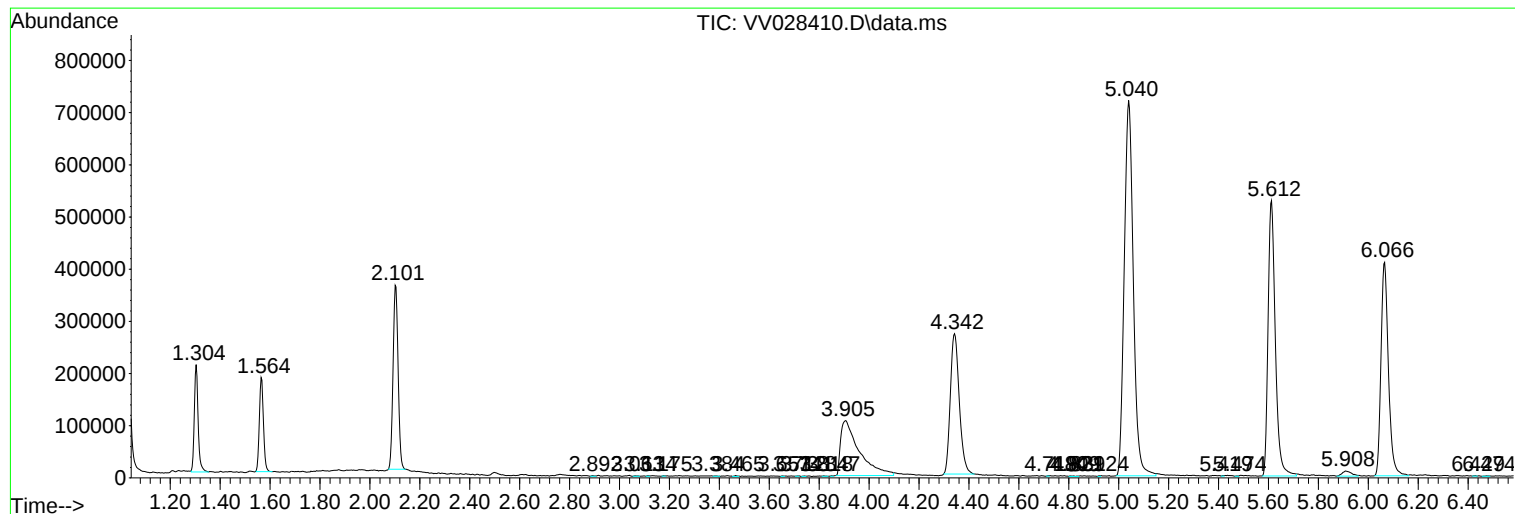

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028410.D
Acq On : 07 Oct 2022 16:24
Operator : SY/MD
Sample : N4893-09DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J06DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028410.D
Acq On : 07 Oct 2022 16:24
Operator : SY/MD
Sample : N4893-09DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J06DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc