

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028413.D
 Acq On : 07 Oct 2022 17:37
 Operator : SY/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028413.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	196748	200136	6.33%	1.271%
2	1.564	156	163	175	rVB	160322	182651	5.78%	1.160%
3	2.101	322	330	347	rVB	316501	454818	14.38%	2.889%
4	2.719	520	522	523	rBV2	786	309	0.01%	0.002%
5	2.912	578	582	584	rVB3	872	659	0.02%	0.004%
6	2.924	584	586	587	rBV3	706	258	0.01%	0.002%
7	3.301	698	703	708	rBV5	1090	1308	0.04%	0.008%
8	3.359	717	721	725	rBV6	1551	1339	0.04%	0.009%
9	3.487	758	761	762	rBV2	686	439	0.01%	0.003%
10	3.513	767	769	772	rVV4	760	532	0.02%	0.003%
11	3.545	777	779	784	rVB4	1203	705	0.02%	0.004%
12	3.574	785	788	790	rBV2	778	433	0.01%	0.003%
13	3.641	806	809	812	rVB3	861	422	0.01%	0.003%
14	3.674	812	819	821	rBV5	830	811	0.03%	0.005%
15	3.712	829	831	833	rVB3	732	215	0.01%	0.001%
16	3.738	836	839	843	rBV5	890	545	0.02%	0.003%
17	3.760	844	846	849	rVB3	705	293	0.01%	0.002%
18	3.783	850	853	856	rVB3	977	650	0.02%	0.004%
19	3.805	856	860	862	rBV5	603	466	0.01%	0.003%
20	3.902	878	890	947	rBV	93742	449611	14.22%	2.856%
21	4.342	1011	1027	1055	rBV	252633	634013	20.05%	4.028%
22	4.690	1133	1135	1137	rBV	590	332	0.01%	0.002%
23	4.815	1172	1174	1176	rBV3	811	339	0.01%	0.002%
24	4.950	1214	1216	1220	rBV5	817	500	0.02%	0.003%
25	5.040	1227	1244	1276	rBV2	645702	1662241	52.56%	10.560%
26	5.612	1410	1422	1448	rBV	480952	974505	30.81%	6.191%
27	5.915	1507	1516	1537	rVB7	15598	39866	1.26%	0.253%
28	6.066	1549	1563	1592	rBV	366892	767954	24.28%	4.879%
29	6.551	1711	1714	1716	rBV3	474	368	0.01%	0.002%
30	6.606	1728	1731	1733	rVB2	1470	725	0.02%	0.005%
31	6.622	1733	1736	1739	rBV4	1248	1150	0.04%	0.007%
32	6.821	1793	1798	1800	rBV6	992	847	0.03%	0.005%
33	6.982	1832	1848	1873	rBV	230640	431517	13.64%	2.741%
34	7.262	1932	1935	1937	rBV3	1087	646	0.02%	0.004%
35	7.310	1939	1950	1979	rVV	759195	1331284	42.09%	8.458%
36	7.616	2035	2045	2070	rBV	153785	278842	8.82%	1.772%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028413.D
 Acq On : 07 Oct 2022 17:37
 Operator : SY/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.969	2142	2155	2181	rBV	1906222	3162699	100.00%	20.093%
38	8.085	2182	2191	2232	rVV	497295	951955	30.10%	6.048%
39	8.616	2352	2356	2358	rBV3	1329	858	0.03%	0.005%
40	8.644	2363	2365	2368	rBV3	755	440	0.01%	0.003%
41	8.767	2401	2403	2406	rVV4	531	384	0.01%	0.002%
42	8.847	2416	2428	2453	rBV	685681	1141273	36.09%	7.251%
43	9.136	2516	2518	2522	rVB5	713	524	0.02%	0.003%
44	9.162	2522	2526	2529	rBV3	1065	1014	0.03%	0.006%
45	9.204	2536	2539	2541	rBV4	875	613	0.02%	0.004%
46	9.268	2553	2559	2563	rBV7	1176	1354	0.04%	0.009%
47	9.291	2563	2566	2570	rVV4	444	389	0.01%	0.002%
48	9.333	2577	2579	2582	rVB3	1189	616	0.02%	0.004%
49	9.432	2607	2610	2614	rVB5	1152	938	0.03%	0.006%
50	9.455	2614	2617	2620	rBV4	815	520	0.02%	0.003%
51	9.493	2625	2629	2631	rBV4	584	412	0.01%	0.003%
52	9.509	2631	2634	2637	rBV5	951	701	0.02%	0.004%
53	9.664	2679	2682	2685	rBV4	497	395	0.01%	0.003%
54	9.696	2688	2692	2694	rBV3	706	496	0.02%	0.003%
55	9.773	2712	2716	2718	rBV4	1115	651	0.02%	0.004%
56	9.796	2722	2723	2725	rBV2	466	217	0.01%	0.001%
57	9.902	2752	2756	2758	rBV5	599	558	0.02%	0.004%
58	9.931	2763	2765	2769	rVV3	529	301	0.01%	0.002%
59	9.963	2772	2775	2779	rVB4	487	362	0.01%	0.002%
60	9.988	2779	2783	2787	rBV5	1136	1001	0.03%	0.006%
61	10.033	2794	2797	2802	rBV4	828	734	0.02%	0.005%
62	10.053	2802	2803	2805	rBV2	642	273	0.01%	0.002%
63	10.085	2810	2813	2818	rVB5	561	406	0.01%	0.003%
64	10.162	2836	2837	2838	rVV	785	217	0.01%	0.001%
65	10.207	2839	2851	2875	rVV	502678	803175	25.40%	5.103%
66	10.384	2899	2906	2914	rVB10	3860	5537	0.18%	0.035%
67	10.423	2914	2918	2920	rBV3	1310	856	0.03%	0.005%
68	10.529	2949	2951	2953	rBV2	972	477	0.02%	0.003%
69	10.554	2957	2959	2963	rBV3	652	392	0.01%	0.002%
70	10.583	2963	2968	2971	rBV5	1348	1151	0.04%	0.007%
71	10.612	2975	2977	2980	rBV4	873	565	0.02%	0.004%
72	10.747	3016	3019	3024	rBV5	454	354	0.01%	0.002%
73	10.773	3024	3027	3029	rBV5	501	340	0.01%	0.002%
74	10.815	3037	3040	3042	rBV3	650	425	0.01%	0.003%
75	11.085	3120	3124	3129	rVB7	1067	1161	0.04%	0.007%
76	11.120	3129	3135	3136	rBV4	939	1000	0.03%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028413.D
 Acq On : 07 Oct 2022 17:37
 Operator : SY/MD
 Sample : N4893-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.188	3154	3156	3158	rBV4	636	384	0.01%	0.002%
78	11.239	3162	3172	3197	rVV	688910	1093281	34.57%	6.946%
79	11.500	3251	3253	3256	rBV3	784	417	0.01%	0.003%
80	11.615	3276	3289	3309	rBV	701056	1126826	35.63%	7.159%
81	11.828	3352	3355	3358	rBV3	591	391	0.01%	0.002%
82	11.879	3368	3371	3373	rBV2	694	593	0.02%	0.004%
83	11.950	3391	3393	3397	rVB5	1466	726	0.02%	0.005%
84	11.976	3397	3401	3402	rBV3	598	341	0.01%	0.002%
85	12.156	3455	3457	3460	rBV3	530	360	0.01%	0.002%
86	12.236	3478	3482	3483	rBV3	709	522	0.02%	0.003%
87	12.432	3541	3543	3548	rVB5	1120	565	0.02%	0.004%
88	12.455	3548	3550	3552	rBV	481	233	0.01%	0.001%
89	12.493	3558	3562	3563	rBV4	965	553	0.02%	0.004%
90	12.570	3584	3586	3591	rVB3	581	396	0.01%	0.003%
91	12.628	3602	3604	3607	rBV4	482	284	0.01%	0.002%
92	12.770	3644	3648	3649	rBV3	732	518	0.02%	0.003%
93	12.808	3657	3660	3662	rBV4	699	383	0.01%	0.002%
94	13.201	3778	3782	3784	rBV5	969	640	0.02%	0.004%
95	13.255	3793	3799	3802	rBV5	1178	1332	0.04%	0.008%
96	13.599	3904	3906	3909	rBV3	775	547	0.02%	0.003%
97	13.683	3929	3932	3938	rBV6	1560	1452	0.05%	0.009%
98	13.850	3982	3984	3987	rBV4	667	316	0.01%	0.002%
99	13.985	4024	4026	4030	rVB4	1118	637	0.02%	0.004%
100	14.265	4108	4113	4115	rBV4	1414	1257	0.04%	0.008%




Sum of corrected areas: 15740417

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028413.D
Acq On : 07 Oct 2022 17:37
Operator : SY/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

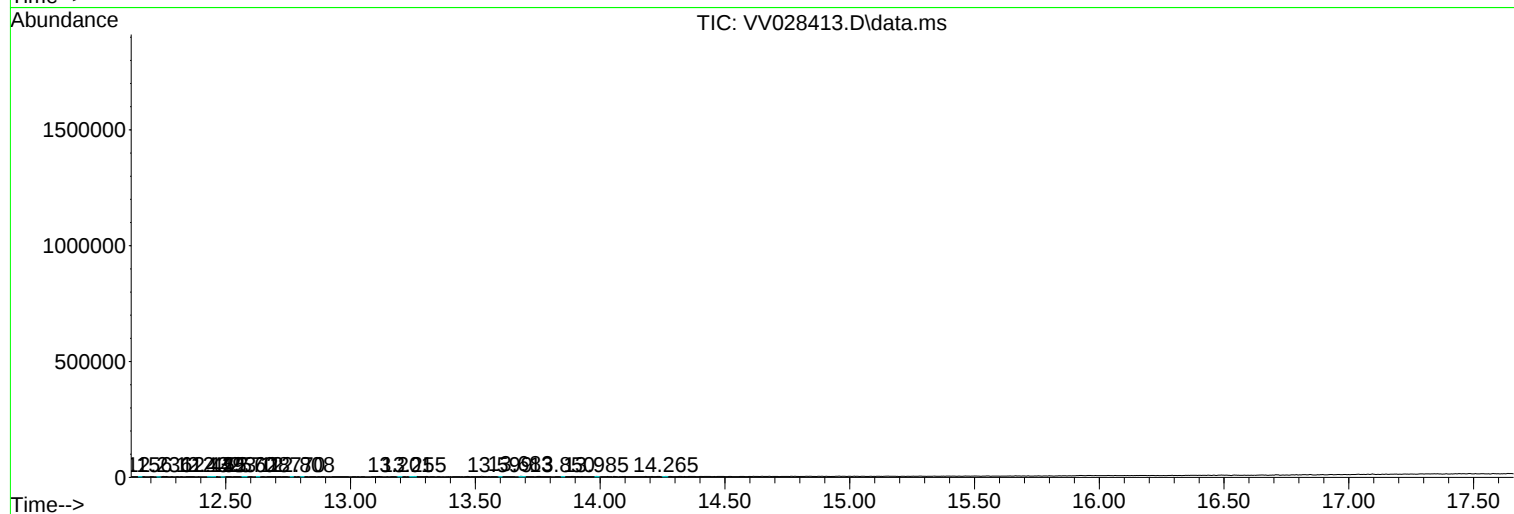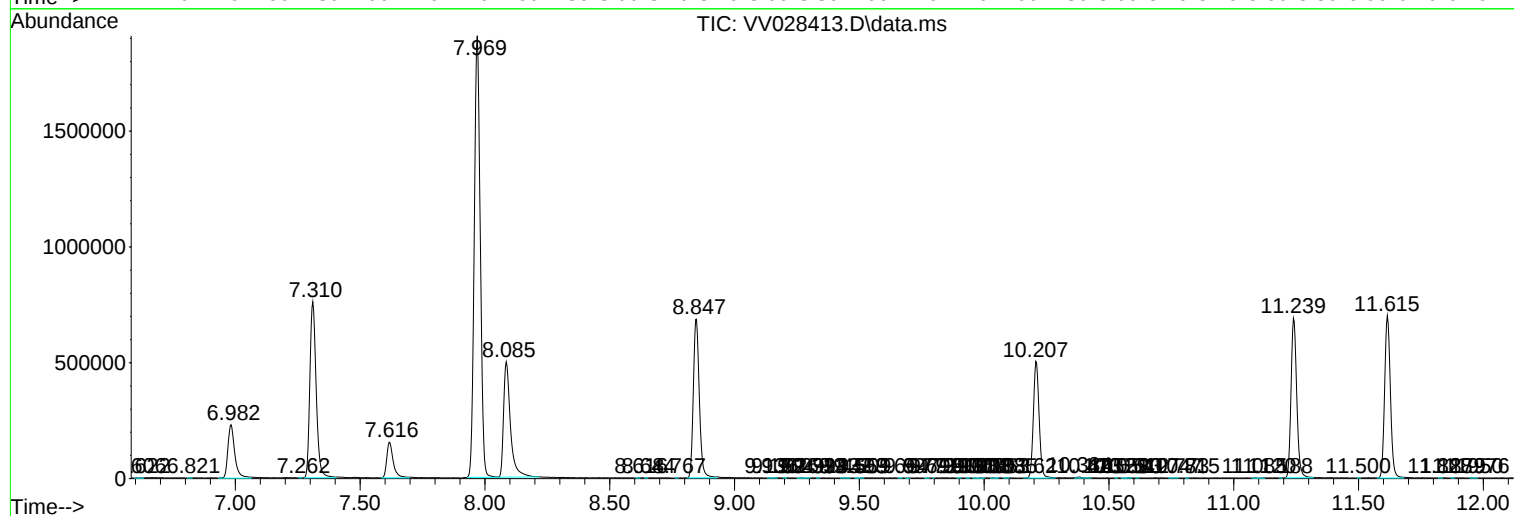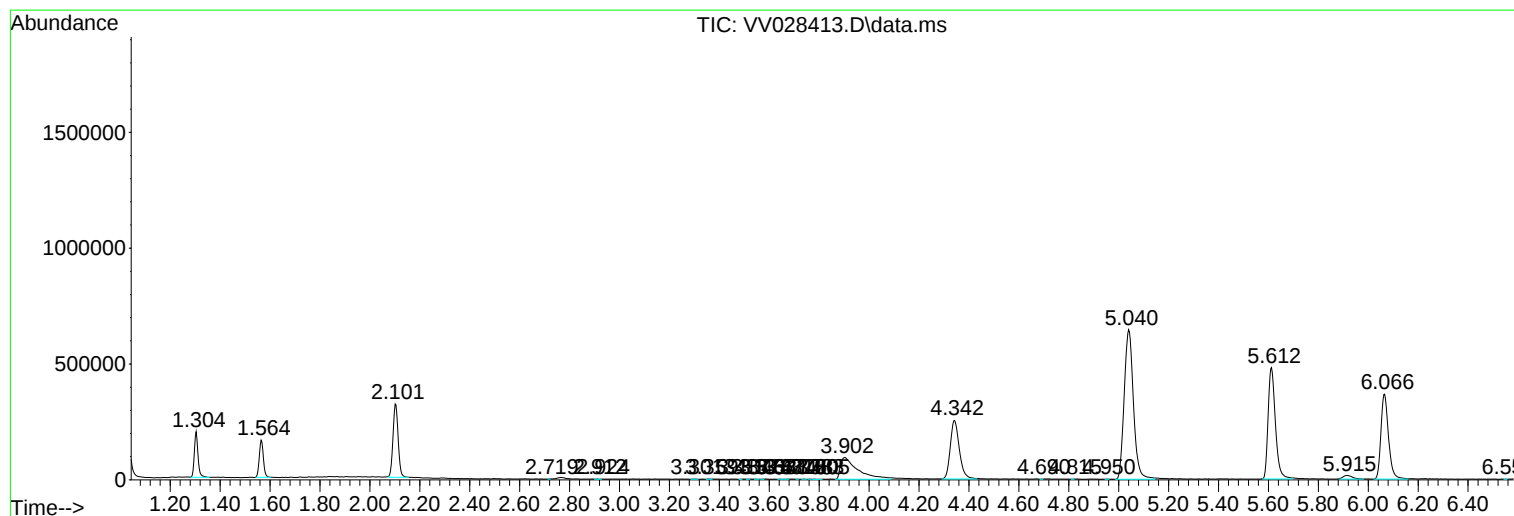

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028413.D
Acq On : 07 Oct 2022 17:37
Operator : SY/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028413.D
Acq On : 07 Oct 2022 17:37
Operator : SY/MD
Sample : N4893-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc