

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028414.D
 Acq On : 07 Oct 2022 17:59
 Operator : SY/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028414.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	187205	191701	9.10%	1.318%
2	1.564	157	163	177	rVB	157881	183275	8.70%	1.260%
3	2.105	322	331	346	rVB	313185	450030	21.37%	3.094%
4	2.928	582	587	589	rBV6	1365	1024	0.05%	0.007%
5	3.224	676	679	680	rBV	839	516	0.02%	0.004%
6	3.326	709	711	712	rBV2	677	295	0.01%	0.002%
7	3.494	761	763	766	rBV4	1060	748	0.04%	0.005%
8	3.635	804	807	813	rBV6	1141	833	0.04%	0.006%
9	3.683	820	822	825	rVB2	552	214	0.01%	0.001%
10	3.744	839	841	844	rBV3	643	342	0.02%	0.002%
11	3.773	845	850	853	rBV5	871	807	0.04%	0.006%
12	3.905	878	891	943	rBV	88558	442417	21.01%	3.041%
13	4.343	1013	1027	1055	rBV	245725	618424	29.37%	4.251%
14	4.928	1205	1209	1211	rBV5	541	386	0.02%	0.003%
15	5.043	1228	1245	1279	rBV2	634825	1650775	78.40%	11.348%
16	5.561	1404	1406	1409	rBV3	722	433	0.02%	0.003%
17	5.613	1411	1422	1451	rVV	472813	962047	45.69%	6.613%
18	5.918	1504	1517	1537	rBV8	22357	57601	2.74%	0.396%
19	6.066	1551	1563	1591	rBV	365506	751818	35.70%	5.168%
20	6.384	1660	1662	1668	rVB5	1267	1170	0.06%	0.008%
21	6.416	1668	1672	1676	rBV5	1017	890	0.04%	0.006%
22	6.474	1686	1690	1695	rVB7	1413	1300	0.06%	0.009%
23	6.497	1695	1697	1704	rBV5	642	819	0.04%	0.006%
24	6.567	1718	1719	1721	rBV	741	375	0.02%	0.003%
25	6.908	1822	1825	1826	rBV	706	431	0.02%	0.003%
26	6.982	1837	1848	1872	rBV	224916	419817	19.94%	2.886%
27	7.310	1938	1950	1980	rBV	756147	1327703	63.05%	9.127%
28	7.619	2036	2046	2070	rBV	153927	278035	13.20%	1.911%
29	7.905	2131	2135	2137	rBV4	954	753	0.04%	0.005%
30	7.969	2143	2155	2178	rBV	1261996	2105701	100.00%	14.475%
31	8.088	2182	2192	2230	rBV	491932	948429	45.04%	6.520%
32	8.542	2329	2333	2334	rBV2	618	484	0.02%	0.003%
33	8.712	2385	2386	2388	rBV2	471	243	0.01%	0.002%
34	8.847	2417	2428	2453	rBV	681104	1115471	52.97%	7.668%
35	9.120	2510	2513	2515	rBV3	1051	649	0.03%	0.004%
36	9.153	2521	2523	2525	rBV2	865	449	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028414.D
 Acq On : 07 Oct 2022 17:59
 Operator : SY/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	9.175	2529	2530	2533	rVB3	691	281	0.01%	0.002%
38	9.204	2537	2539	2541	rBV2	544	350	0.02%	0.002%
39	9.313	2570	2573	2575	rBV3	1100	722	0.03%	0.005%
40	9.381	2590	2594	2596	rBV5	965	608	0.03%	0.004%
41	9.471	2621	2622	2624	rVB	984	331	0.02%	0.002%
42	9.487	2624	2627	2632	rBV6	886	1066	0.05%	0.007%
43	9.564	2649	2651	2654	rBV3	692	391	0.02%	0.003%
44	9.603	2661	2663	2666	rVB3	793	438	0.02%	0.003%
45	9.622	2666	2669	2672	rBV4	859	761	0.04%	0.005%
46	9.683	2686	2688	2689	rBV2	565	238	0.01%	0.002%
47	9.831	2730	2734	2737	rBV5	739	547	0.03%	0.004%
48	9.847	2737	2739	2742	rBV4	571	371	0.02%	0.003%
49	9.892	2751	2753	2756	rVB4	874	501	0.02%	0.003%
50	10.011	2789	2790	2795	rVB5	723	479	0.02%	0.003%
51	10.050	2799	2802	2804	rBV3	880	418	0.02%	0.003%
52	10.095	2814	2816	2817	rBV2	421	173	0.01%	0.001%
53	10.108	2818	2820	2823	rVV4	800	460	0.02%	0.003%
54	10.140	2828	2830	2833	rVV3	512	286	0.01%	0.002%
55	10.207	2840	2851	2877	rBV	497309	790890	37.56%	5.437%
56	10.378	2897	2904	2914	rVB5	3654	5339	0.25%	0.037%
57	10.448	2922	2926	2927	rBV3	516	402	0.02%	0.003%
58	10.506	2941	2944	2945	rBV2	712	410	0.02%	0.003%
59	10.535	2950	2953	2956	rBV4	779	653	0.03%	0.004%
60	10.670	2990	2995	2997	rBV3	927	983	0.05%	0.007%
61	10.725	3008	3012	3016	rBV6	669	743	0.04%	0.005%
62	10.792	3032	3033	3036	rVB2	695	186	0.01%	0.001%
63	10.805	3036	3037	3039	rVB2	645	225	0.01%	0.002%
64	10.825	3039	3043	3044	rBV4	984	773	0.04%	0.005%
65	10.992	3093	3095	3098	rBV3	507	312	0.01%	0.002%
66	11.037	3107	3109	3111	rBV2	515	346	0.02%	0.002%
67	11.066	3116	3118	3120	rVV3	616	240	0.01%	0.002%
68	11.162	3145	3148	3150	rBV3	854	565	0.03%	0.004%
69	11.175	3150	3152	3153	rBV	675	289	0.01%	0.002%
70	11.239	3160	3172	3194	rBV	677480	1079437	51.26%	7.420%
71	11.458	3238	3240	3242	rBV3	900	597	0.03%	0.004%
72	11.558	3268	3271	3275	rVB5	826	655	0.03%	0.005%
73	11.616	3277	3289	3309	rBV	698302	1124982	53.43%	7.733%
74	11.995	3404	3407	3412	rVB5	933	934	0.04%	0.006%
75	12.014	3412	3413	3417	rBV4	771	496	0.02%	0.003%
76	12.037	3417	3420	3426	rVB6	870	761	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028414.D
 Acq On : 07 Oct 2022 17:59
 Operator : SY/MD
 Sample : N4893-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.069	3426	3430	3431	rBV3	511	335	0.02%	0.002%
78	12.104	3439	3441	3444	rVB3	1207	617	0.03%	0.004%
79	12.127	3444	3448	3449	rBV2	668	491	0.02%	0.003%
80	12.185	3464	3466	3470	rBV3	527	418	0.02%	0.003%
81	12.226	3474	3479	3480	rBV4	1489	1122	0.05%	0.008%
82	12.300	3500	3502	3503	rBV2	493	244	0.01%	0.002%
83	12.406	3533	3535	3538	rVB5	966	449	0.02%	0.003%
84	12.435	3541	3544	3547	rBV5	1064	661	0.03%	0.005%
85	12.487	3558	3560	3563	rVB3	1147	511	0.02%	0.004%
86	12.599	3593	3595	3596	rBV	811	337	0.02%	0.002%
87	12.641	3606	3608	3610	rBV3	474	190	0.01%	0.001%
88	12.686	3618	3622	3623	rBV3	578	379	0.02%	0.003%
89	12.731	3634	3636	3638	rBV3	708	400	0.02%	0.003%
90	12.802	3656	3658	3660	rBV3	824	345	0.02%	0.002%
91	13.178	3771	3775	3777	rBV4	1217	877	0.04%	0.006%
92	13.201	3780	3782	3784	rBV3	369	189	0.01%	0.001%
93	13.255	3797	3799	3802	rBV4	655	477	0.02%	0.003%
94	13.403	3842	3845	3846	rBV3	1262	687	0.03%	0.005%
95	13.455	3858	3861	3864	rBV4	621	380	0.02%	0.003%
96	13.490	3868	3872	3876	rBV5	920	732	0.03%	0.005%
97	13.779	3960	3962	3963	rVV2	614	160	0.01%	0.001%
98	13.847	3979	3983	3986	rBV5	1115	883	0.04%	0.006%
99	13.924	4003	4007	4009	rBV6	882	689	0.03%	0.005%
100	14.242	4103	4106	4108	rVB3	1056	557	0.03%	0.004%




Sum of corrected areas: 14547174

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028414.D
Acq On : 07 Oct 2022 17:59
Operator : SY/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

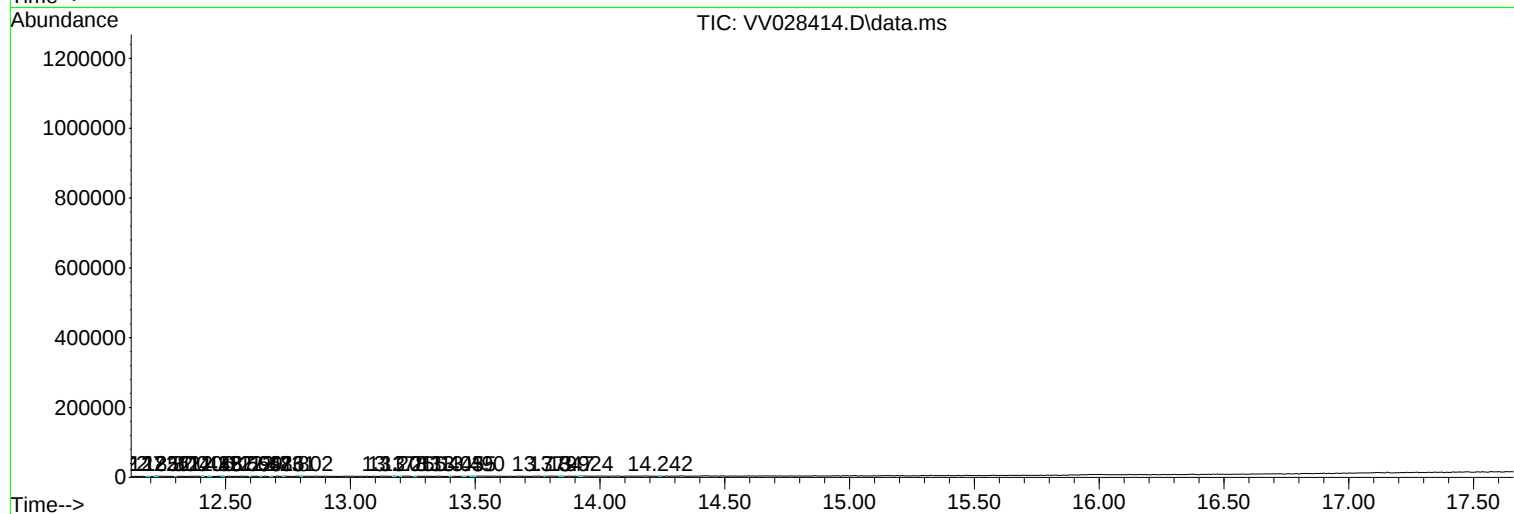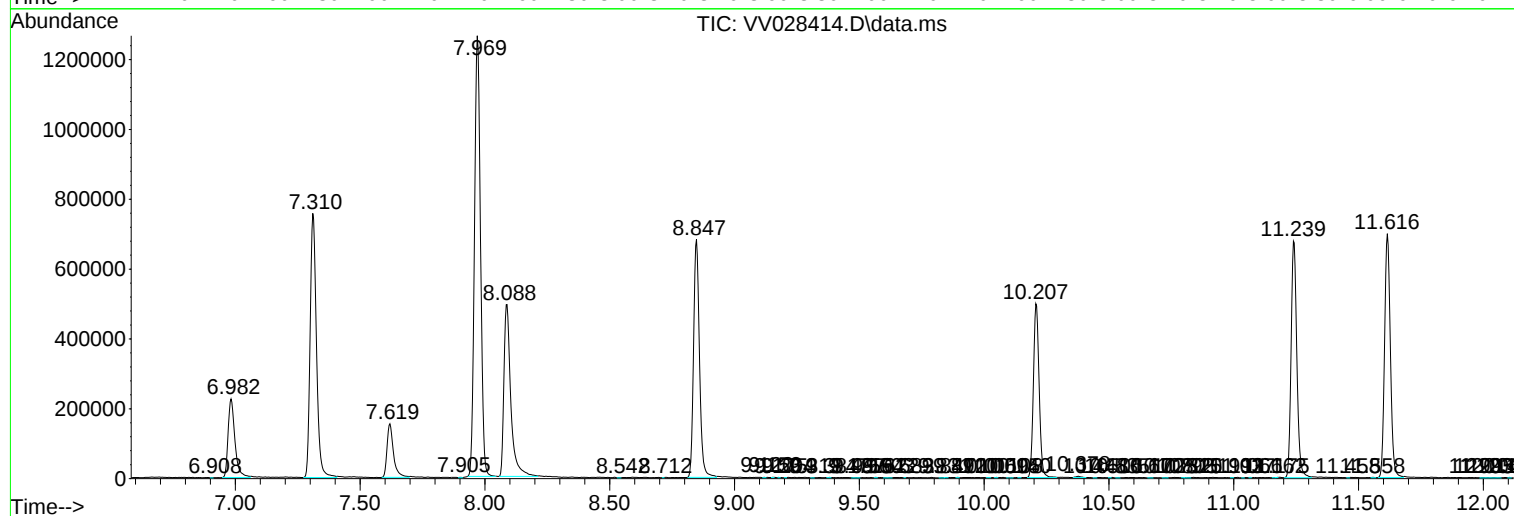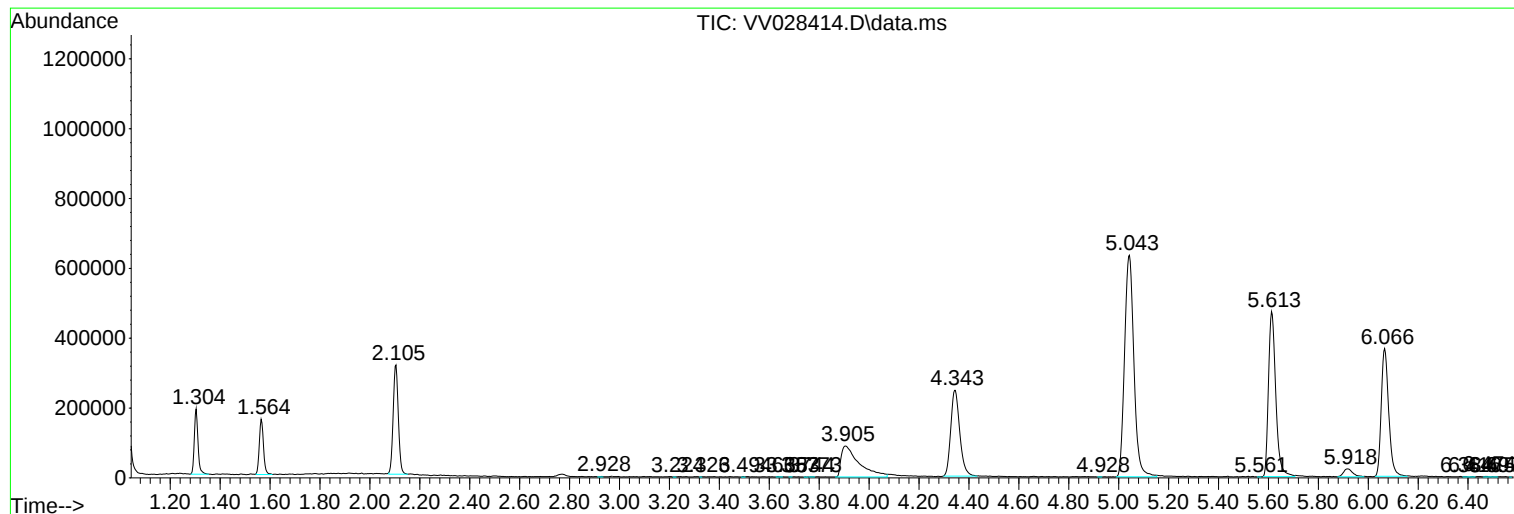

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028414.D
Acq On : 07 Oct 2022 17:59
Operator : SY/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028414.D
Acq On : 07 Oct 2022 17:59
Operator : SY/MD
Sample : N4893-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc