

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028415.D
 Acq On : 07 Oct 2022 18:23
 Operator : SY/MD
 Sample : N4893-14DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028415.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	189705	196677	11.70%	1.449%
2	1.565	156	163	175	rBV	165273	187616	11.16%	1.383%
3	2.102	322	330	345	rVB	318826	458679	27.29%	3.380%
4	3.294	697	701	706	rVB5	697	699	0.04%	0.005%
5	3.330	711	712	714	rBV2	615	345	0.02%	0.003%
6	3.507	765	767	772	rVB3	614	369	0.02%	0.003%
7	3.548	778	780	783	rBV4	702	317	0.02%	0.002%
8	3.568	783	786	787	rVV2	736	365	0.02%	0.003%
9	3.735	835	838	839	rBV2	868	458	0.03%	0.003%
10	3.773	843	850	854	rBV8	1219	1198	0.07%	0.009%
11	3.905	879	891	932	rBV3	99146	499067	29.69%	3.678%
12	4.343	1013	1027	1058	rVB	255026	636241	37.85%	4.688%
13	4.680	1129	1132	1134	rBV4	707	460	0.03%	0.003%
14	4.883	1193	1195	1199	rVB5	813	421	0.03%	0.003%
15	4.963	1217	1220	1221	rBV2	696	398	0.02%	0.003%
16	5.040	1227	1244	1279	rBV2	653778	1680807	100.00%	12.386%
17	5.445	1368	1370	1373	rBV4	719	378	0.02%	0.003%
18	5.613	1410	1422	1450	rBV	468223	956079	56.88%	7.045%
19	5.915	1505	1516	1538	rVB6	18529	45335	2.70%	0.334%
20	6.063	1550	1562	1586	rBV	374518	771477	45.90%	5.685%
21	6.381	1659	1661	1667	rVB5	972	925	0.06%	0.007%
22	6.413	1668	1671	1674	rBV4	643	514	0.03%	0.004%
23	6.461	1684	1686	1688	rBV3	871	409	0.02%	0.003%
24	6.506	1698	1700	1702	rBV2	622	368	0.02%	0.003%
25	6.632	1736	1739	1741	rBV4	753	526	0.03%	0.004%
26	6.732	1768	1770	1771	rBV2	674	323	0.02%	0.002%
27	6.928	1826	1831	1834	rVB4	915	810	0.05%	0.006%
28	6.982	1834	1848	1875	rBV	229578	433529	25.79%	3.195%
29	7.310	1939	1950	1976	rBV	780436	1347088	80.15%	9.927%
30	7.616	2035	2045	2076	rBV	157890	287515	17.11%	2.119%
31	7.969	2142	2155	2174	rBV	536247	890785	53.00%	6.564%
32	8.085	2182	2191	2229	rBV	495994	975401	58.03%	7.188%
33	8.580	2343	2345	2348	rBV5	957	566	0.03%	0.004%
34	8.664	2367	2371	2373	rBV4	1218	816	0.05%	0.006%
35	8.693	2376	2380	2383	rBV3	1153	628	0.04%	0.005%
36	8.847	2414	2428	2453	rBV	668804	1121860	66.75%	8.267%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028415.D
 Acq On : 07 Oct 2022 18:23
 Operator : SY/MD
 Sample : N4893-14DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	9.307	2570	2571	2573	rBV	716	342	0.02%	0.003%
38	9.333	2576	2579	2584	rVB6	746	708	0.04%	0.005%
39	9.362	2586	2588	2591	rVV2	584	346	0.02%	0.003%
40	9.387	2594	2596	2599	rVB2	773	357	0.02%	0.003%
41	9.484	2622	2626	2628	rBV4	1004	820	0.05%	0.006%
42	9.651	2676	2678	2682	rBV3	1032	521	0.03%	0.004%
43	9.699	2691	2693	2696	rVB4	920	561	0.03%	0.004%
44	9.719	2696	2699	2700	rBV2	683	306	0.02%	0.002%
45	9.783	2715	2719	2720	rBV4	927	503	0.03%	0.004%
46	9.831	2731	2734	2737	rBV3	734	568	0.03%	0.004%
47	9.931	2763	2765	2769	rVB4	716	485	0.03%	0.004%
48	9.957	2770	2773	2775	rBV4	453	323	0.02%	0.002%
49	9.969	2775	2777	2781	rVV5	955	641	0.04%	0.005%
50	10.085	2811	2813	2816	rBV4	755	547	0.03%	0.004%
51	10.207	2837	2851	2869	rBV	504134	806070	47.96%	5.940%
52	10.371	2899	2902	2907	rBV6	1135	977	0.06%	0.007%
53	10.420	2914	2917	2921	rBV4	903	784	0.05%	0.006%
54	10.477	2931	2935	2937	rBV3	859	566	0.03%	0.004%
55	10.542	2953	2955	2957	rVB2	1173	513	0.03%	0.004%
56	10.561	2957	2961	2962	rBV4	480	395	0.02%	0.003%
57	10.571	2962	2964	2968	rVV3	1267	877	0.05%	0.006%
58	10.593	2968	2971	2974	rVB4	661	402	0.02%	0.003%
59	10.609	2974	2976	2980	rBV5	610	491	0.03%	0.004%
60	10.629	2980	2982	2988	rVB6	1102	886	0.05%	0.007%
61	10.657	2988	2991	2993	rBV3	903	626	0.04%	0.005%
62	10.686	2997	3000	3003	rVV4	824	584	0.03%	0.004%
63	10.722	3007	3011	3013	rBV3	603	461	0.03%	0.003%
64	10.821	3040	3042	3045	rVB4	1199	581	0.03%	0.004%
65	10.985	3091	3093	3100	rVB7	819	615	0.04%	0.005%
66	11.014	3100	3102	3105	rBV4	536	510	0.03%	0.004%
67	11.082	3121	3123	3127	rVB3	893	520	0.03%	0.004%
68	11.133	3137	3139	3141	rBV3	725	459	0.03%	0.003%
69	11.175	3148	3152	3155	rBV5	803	749	0.04%	0.006%
70	11.239	3161	3172	3196	rBV	677884	1081356	64.34%	7.968%
71	11.519	3256	3259	3261	rBV3	1225	582	0.03%	0.004%
72	11.616	3277	3289	3312	rBV	712731	1148198	68.31%	8.461%
73	11.799	3344	3346	3349	rVB2	813	398	0.02%	0.003%
74	11.854	3360	3363	3367	rBV4	453	466	0.03%	0.003%
75	11.886	3371	3373	3375	rBV3	923	454	0.03%	0.003%
76	12.101	3436	3440	3444	rBV5	906	994	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028415.D
 Acq On : 07 Oct 2022 18:23
 Operator : SY/MD
 Sample : N4893-14DL 4X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J15DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.127	3444	3448	3450	rVV3	946	603	0.04%	0.004%
78	12.185	3463	3466	3470	rBV3	1163	916	0.05%	0.007%
79	12.371	3521	3524	3525	rBV3	722	399	0.02%	0.003%
80	12.416	3536	3538	3542	rBV5	1198	911	0.05%	0.007%
81	12.477	3555	3557	3562	rVB5	1348	796	0.05%	0.006%
82	12.509	3562	3567	3568	rBV4	728	553	0.03%	0.004%
83	12.628	3600	3604	3607	rBV4	817	612	0.04%	0.005%
84	12.670	3616	3617	3621	rBV4	681	396	0.02%	0.003%
85	12.873	3677	3680	3683	rVB4	813	548	0.03%	0.004%
86	12.915	3691	3693	3697	rVB3	794	486	0.03%	0.004%
87	12.966	3707	3709	3712	rBV3	766	513	0.03%	0.004%
88	13.069	3737	3741	3742	rBV3	914	661	0.04%	0.005%
89	13.111	3752	3754	3757	rBV3	878	620	0.04%	0.005%
90	13.220	3786	3788	3791	rBV4	729	511	0.03%	0.004%
91	13.410	3845	3847	3850	rBV2	1016	774	0.05%	0.006%
92	13.513	3877	3879	3881	rBV3	773	434	0.03%	0.003%
93	13.632	3913	3916	3920	rVB5	1523	1063	0.06%	0.008%
94	13.654	3921	3923	3926	rBV3	755	373	0.02%	0.003%
95	13.808	3969	3971	3974	rBV3	878	355	0.02%	0.003%
96	14.107	4062	4064	4066	rBV2	868	472	0.03%	0.003%
97	14.178	4084	4086	4090	rBV3	821	688	0.04%	0.005%
98	14.281	4116	4118	4121	rBV2	825	417	0.02%	0.003%
99	14.596	4215	4216	4223	rBV6	1218	920	0.05%	0.007%
100	14.869	4299	4301	4303	rBV3	1110	532	0.03%	0.004%




Sum of corrected areas: 13570544

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028415.D
Acq On : 07 Oct 2022 18:23
Operator : SY/MD
Sample : N4893-14DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

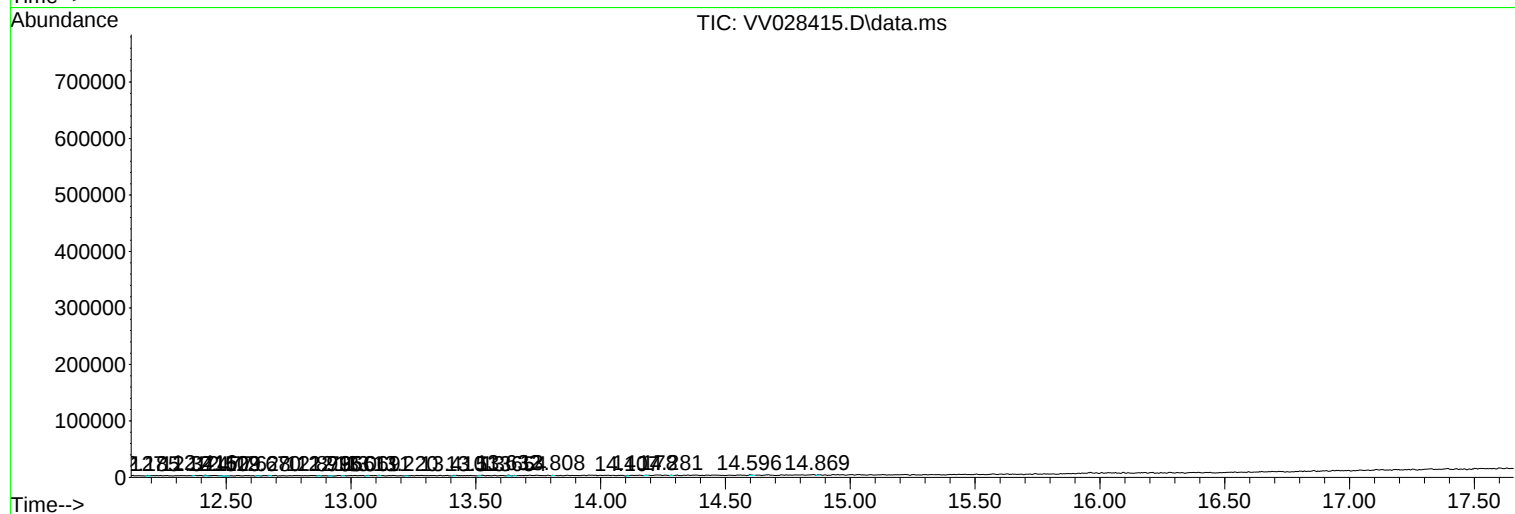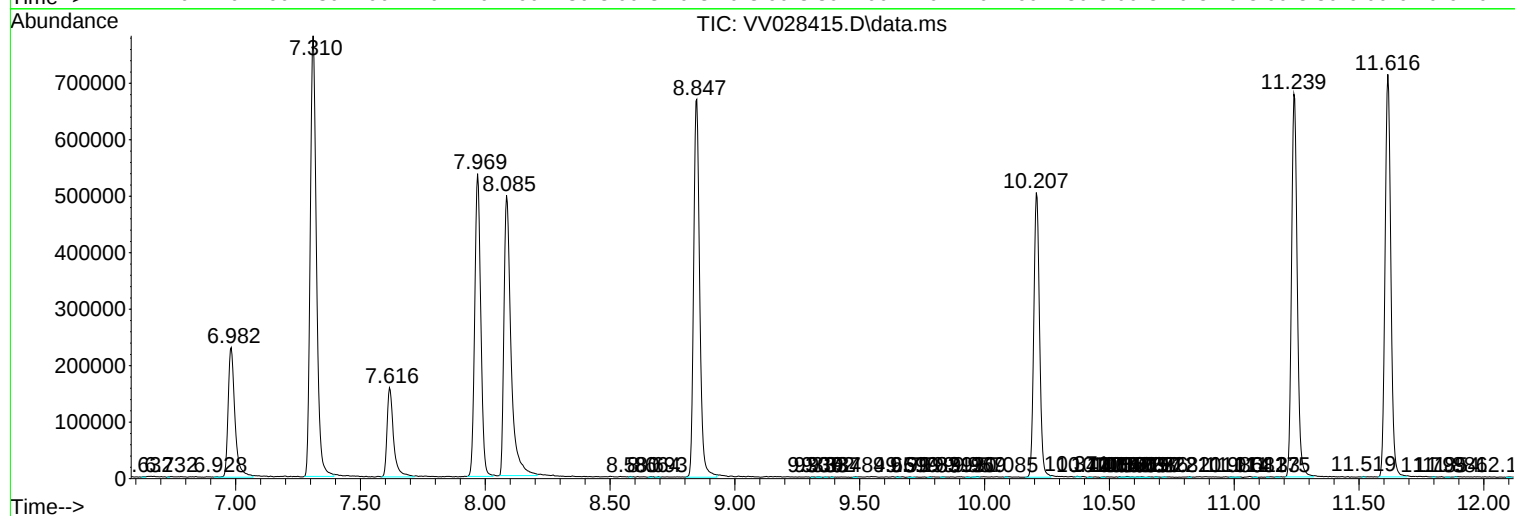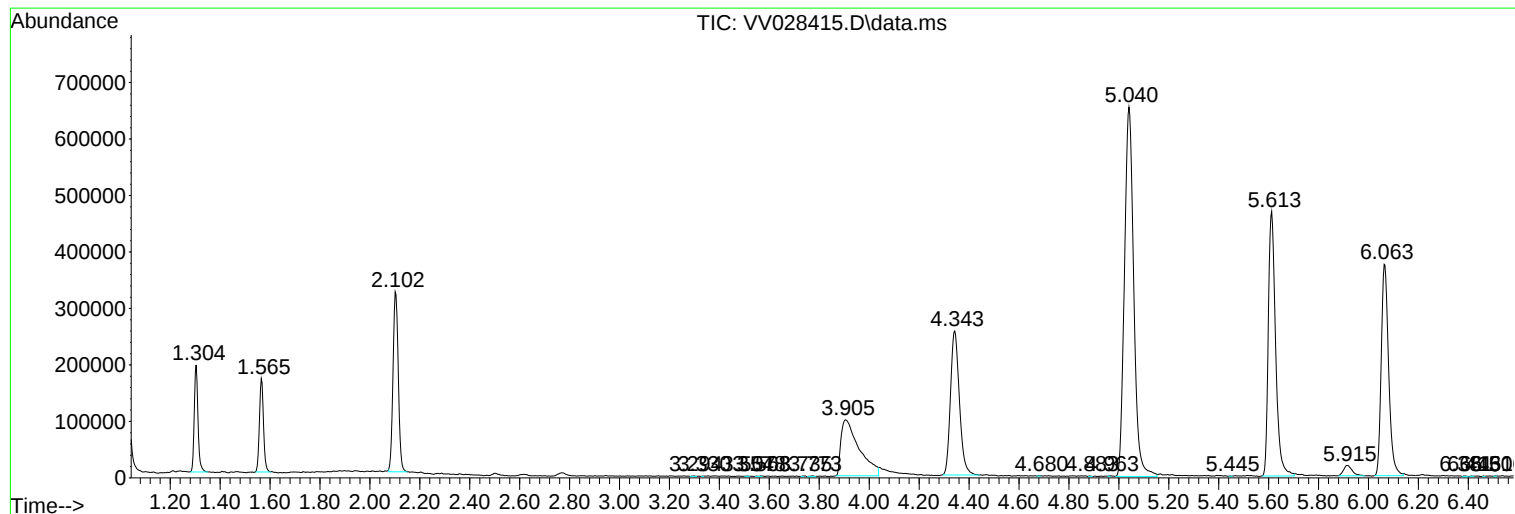

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028415.D
Acq On : 07 Oct 2022 18:23
Operator : SY/MD
Sample : N4893-14DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028415.D
Acq On : 07 Oct 2022 18:23
Operator : SY/MD
Sample : N4893-14DL 4X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J15DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc