

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028416.D
 Acq On : 07 Oct 2022 18:48
 Operator : SY/MD
 Sample : N4893-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028416.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	100	rVB	187067	192568	11.77%	1.423%
2	1.564	156	163	177	rBV	159437	183096	11.19%	1.353%
3	2.101	322	330	348	rVB	313755	444320	27.16%	3.283%
4	2.905	577	580	581	rBV2	874	532	0.03%	0.004%
5	2.944	589	592	595	rBV5	1248	896	0.05%	0.007%
6	3.031	616	619	622	rBV4	904	585	0.04%	0.004%
7	3.050	622	625	627	rBV4	844	659	0.04%	0.005%
8	3.217	675	677	680	rVB4	774	323	0.02%	0.002%
9	3.349	714	718	719	rBV4	893	549	0.03%	0.004%
10	3.397	729	733	737	rVB6	976	723	0.04%	0.005%
11	3.773	847	850	852	rBV	633	384	0.02%	0.003%
12	3.793	854	856	862	rVB4	719	446	0.03%	0.003%
13	3.902	879	890	953	rBV	96912	487147	29.78%	3.599%
14	4.342	1013	1027	1058	rVB	246328	624152	38.15%	4.612%
15	4.638	1117	1119	1122	rBV4	1124	774	0.05%	0.006%
16	4.670	1127	1129	1131	rBV3	557	281	0.02%	0.002%
17	4.834	1178	1180	1183	rBV3	795	465	0.03%	0.003%
18	4.857	1183	1187	1188	rBV3	760	507	0.03%	0.004%
19	5.040	1228	1244	1272	rBV2	635916	1635925	100.00%	12.088%
20	5.484	1380	1382	1385	rBV3	965	513	0.03%	0.004%
21	5.612	1409	1422	1450	rBV	496793	1006853	61.55%	7.440%
22	5.841	1491	1493	1495	rBV3	1242	754	0.05%	0.006%
23	6.011	1542	1546	1549	rBV5	1438	1328	0.08%	0.010%
24	6.066	1549	1563	1585	rVV	368712	756812	46.26%	5.592%
25	6.587	1723	1725	1729	rBV5	797	475	0.03%	0.004%
26	6.635	1734	1740	1742	rBV4	1605	1532	0.09%	0.011%
27	6.767	1779	1781	1784	rBV3	684	377	0.02%	0.003%
28	6.786	1784	1787	1791	rBV4	757	586	0.04%	0.004%
29	6.892	1819	1820	1823	rBV	836	433	0.03%	0.003%
30	6.915	1826	1827	1829	rVB	564	144	0.01%	0.001%
31	6.931	1830	1832	1833	rBV2	418	176	0.01%	0.001%
32	6.982	1837	1848	1874	rBV	225154	416710	25.47%	3.079%
33	7.310	1938	1950	1972	rBV	760047	1319159	80.64%	9.747%
34	7.548	2022	2024	2028	rVB4	1487	916	0.06%	0.007%
35	7.616	2036	2045	2068	rBV	149910	268351	16.40%	1.983%
36	7.902	2130	2134	2138	rVB4	1018	720	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028416.D
 Acq On : 07 Oct 2022 18:48
 Operator : SY/MD
 Sample : N4893-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.921	2138	2140	2142	rBV2	1059	552	0.03%	0.004%
38	7.969	2142	2155	2175	rBV	611032	1014239	62.00%	7.494%
39	8.085	2182	2191	2233	rBV	497927	950984	58.13%	7.027%
40	8.432	2297	2299	2301	rBV3	720	204	0.01%	0.002%
41	8.847	2416	2428	2452	rBV	705024	1160860	70.96%	8.577%
42	9.120	2512	2513	2514	rVB	651	126	0.01%	0.001%
43	9.149	2519	2522	2523	rBV	1019	532	0.03%	0.004%
44	9.255	2552	2555	2558	rVB3	917	549	0.03%	0.004%
45	9.323	2574	2576	2578	rBV2	677	411	0.03%	0.003%
46	9.345	2581	2583	2584	rBV2	569	312	0.02%	0.002%
47	9.365	2587	2589	2591	rVV4	607	202	0.01%	0.001%
48	9.432	2606	2610	2613	rBV5	699	557	0.03%	0.004%
49	9.448	2613	2615	2620	rBV6	481	337	0.02%	0.002%
50	9.474	2620	2623	2626	rBV3	988	519	0.03%	0.004%
51	9.500	2627	2631	2634	rBV6	671	602	0.04%	0.004%
52	9.535	2641	2642	2644	rBV	722	269	0.02%	0.002%
53	9.632	2669	2672	2678	rBV5	787	782	0.05%	0.006%
54	9.706	2693	2695	2696	rBV2	485	164	0.01%	0.001%
55	9.725	2696	2701	2706	rVB5	663	817	0.05%	0.006%
56	9.747	2706	2708	2710	rVB3	451	173	0.01%	0.001%
57	9.767	2710	2714	2716	rBV3	949	771	0.05%	0.006%
58	9.802	2722	2725	2726	rBV2	285	198	0.01%	0.001%
59	9.815	2726	2729	2734	rVV6	915	869	0.05%	0.006%
60	9.895	2752	2754	2758	rVB5	616	363	0.02%	0.003%
61	9.911	2758	2759	2761	rBV	309	92	0.01%	0.001%
62	9.934	2761	2766	2770	rBV6	1085	1126	0.07%	0.008%
63	9.969	2773	2777	2779	rBV4	458	337	0.02%	0.002%
64	10.050	2798	2802	2806	rBV6	1227	1484	0.09%	0.011%
65	10.104	2817	2819	2823	rBV7	1339	1039	0.06%	0.008%
66	10.207	2840	2851	2871	rBV	494541	785385	48.01%	5.803%
67	10.323	2885	2887	2890	rVB3	1158	466	0.03%	0.003%
68	10.455	2924	2928	2930	rBV2	811	708	0.04%	0.005%
69	10.516	2945	2947	2948	rBV	455	225	0.01%	0.002%
70	10.525	2948	2950	2951	rBV2	635	277	0.02%	0.002%
71	10.567	2959	2963	2964	rBV2	665	429	0.03%	0.003%
72	10.760	3020	3023	3024	rBV2	825	450	0.03%	0.003%
73	10.905	3064	3068	3070	rBV4	827	675	0.04%	0.005%
74	11.101	3127	3129	3131	rBV2	768	405	0.02%	0.003%
75	11.133	3136	3139	3142	rBV4	1042	563	0.03%	0.004%
76	11.178	3150	3153	3155	rBV3	1445	927	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028416.D
 Acq On : 07 Oct 2022 18:48
 Operator : SY/MD
 Sample : N4893-16DL 10X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J21DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.239	3161	3172	3197	rBV	706019	1122655	68.63%	8.295%
78	11.529	3260	3262	3264	rBV2	590	212	0.01%	0.002%
79	11.615	3278	3289	3311	rBV	707260	1119625	68.44%	8.273%
80	11.776	3337	3339	3343	rBV4	920	593	0.04%	0.004%
81	11.866	3366	3367	3369	rBV2	512	175	0.01%	0.001%
82	11.972	3397	3400	3403	rBV3	1054	909	0.06%	0.007%
83	11.988	3403	3405	3411	rVB6	1190	919	0.06%	0.007%
84	12.140	3450	3452	3456	rBV5	933	643	0.04%	0.005%
85	12.188	3464	3467	3468	rBV2	820	383	0.02%	0.003%
86	12.471	3553	3555	3556	rBV2	605	177	0.01%	0.001%
87	12.484	3556	3559	3560	rBV3	690	369	0.02%	0.003%
88	12.532	3573	3574	3577	rVB3	610	229	0.01%	0.002%
89	12.561	3577	3583	3584	rBV4	717	719	0.04%	0.005%
90	12.779	3648	3651	3652	rBV3	890	444	0.03%	0.003%
91	12.866	3675	3678	3680	rBV2	1009	603	0.04%	0.004%
92	13.085	3743	3746	3747	rBV2	636	355	0.02%	0.003%
93	13.246	3794	3796	3797	rVB2	672	190	0.01%	0.001%
94	13.281	3805	3807	3808	rBV2	778	275	0.02%	0.002%
95	13.416	3846	3849	3850	rBV2	808	487	0.03%	0.004%
96	13.635	3915	3917	3922	rVB5	1285	1006	0.06%	0.007%
97	13.670	3924	3928	3931	rBV5	1325	888	0.05%	0.007%
98	13.686	3931	3933	3938	rBV6	846	782	0.05%	0.006%
99	14.271	4111	4115	4118	rBV6	1096	995	0.06%	0.007%




Sum of corrected areas: 13533784

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028416.D
Acq On : 07 Oct 2022 18:48
Operator : SY/MD
Sample : N4893-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

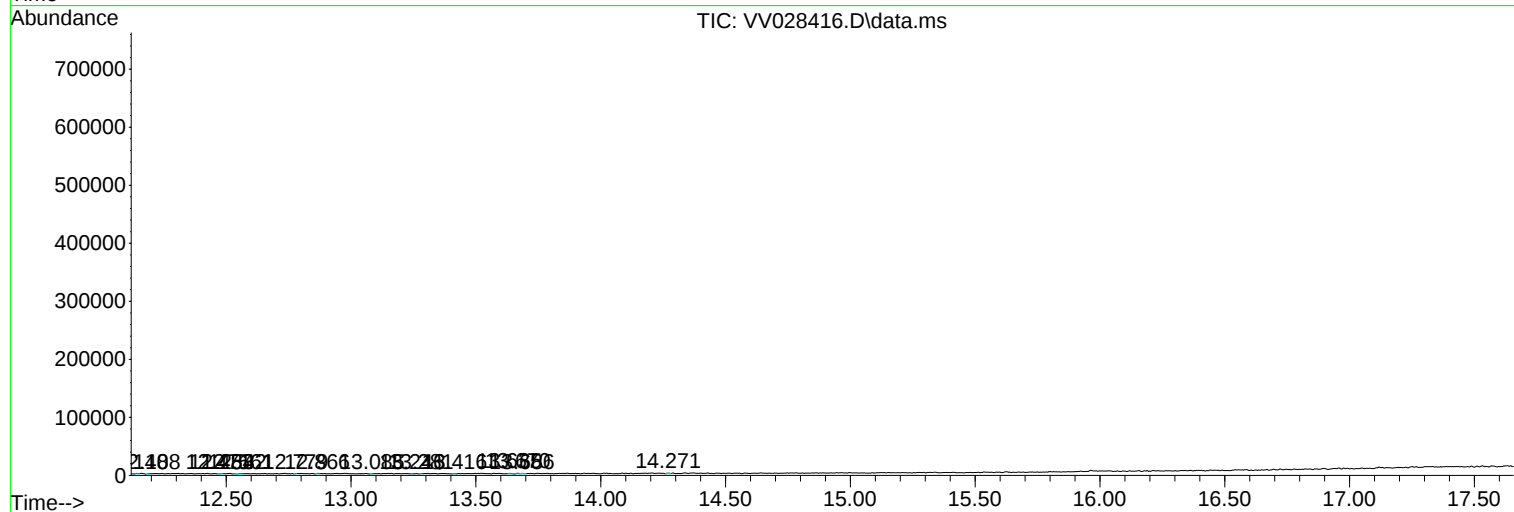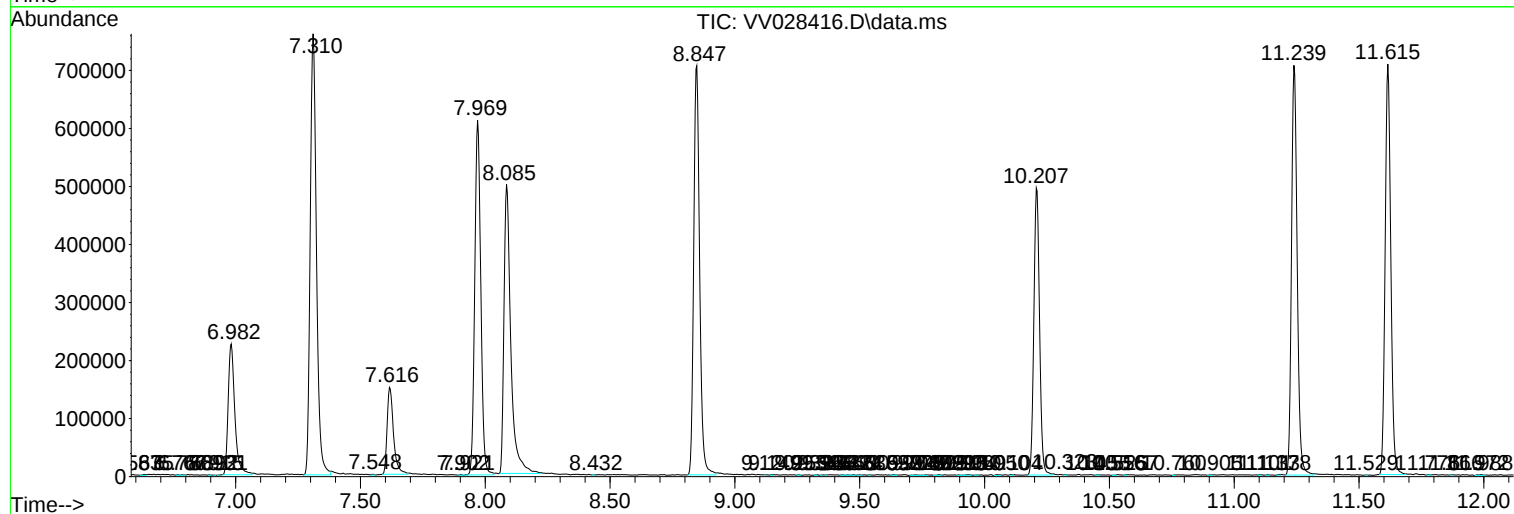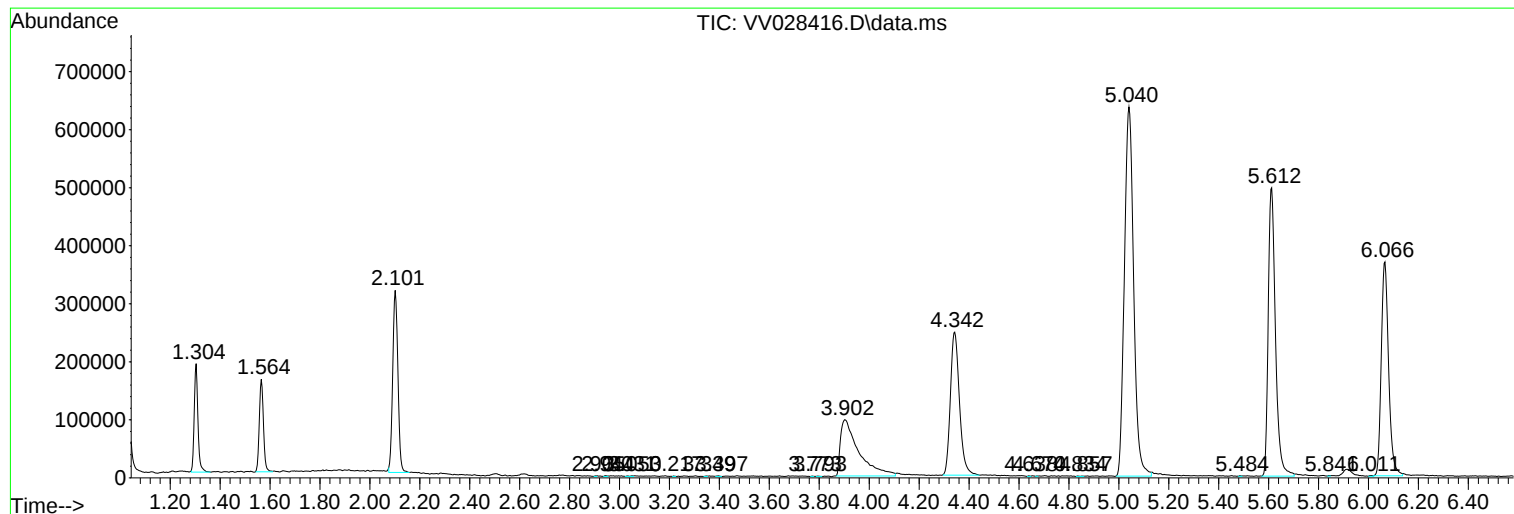

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028416.D
Acq On : 07 Oct 2022 18:48
Operator : SY/MD
Sample : N4893-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028416.D
Acq On : 07 Oct 2022 18:48
Operator : SY/MD
Sample : N4893-16DL 10X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J21DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------