

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028417.D
 Acq On : 07 Oct 2022 19:12
 Operator : SY/MD
 Sample : N4893-17DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028417.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	180715	188587	11.72%	1.455%
2	1.564	157	163	178	rVB	155531	179678	11.17%	1.386%
3	2.104	322	331	349	rVB	310280	445897	27.72%	3.440%
4	2.728	522	525	527	rBV4	1270	774	0.05%	0.006%
5	3.172	659	663	664	rBV3	823	383	0.02%	0.003%
6	3.368	723	724	727	rBV2	531	283	0.02%	0.002%
7	3.477	756	758	762	rBV4	914	752	0.05%	0.006%
8	3.500	763	765	767	rBV3	728	356	0.02%	0.003%
9	3.532	773	775	778	rBV4	853	508	0.03%	0.004%
10	3.664	814	816	818	rBV2	927	492	0.03%	0.004%
11	3.680	818	821	825	rVV4	796	615	0.04%	0.005%
12	3.760	843	846	848	rVB4	648	369	0.02%	0.003%
13	3.799	851	858	862	rBV7	1040	1191	0.07%	0.009%
14	3.902	879	890	926	rBV	89347	427091	26.55%	3.295%
15	4.342	1012	1027	1054	rBV	240501	612236	38.06%	4.724%
16	4.760	1155	1157	1160	rVB5	585	330	0.02%	0.003%
17	4.847	1181	1184	1187	rBV5	935	675	0.04%	0.005%
18	4.866	1187	1190	1191	rBV3	828	453	0.03%	0.003%
19	4.937	1210	1212	1214	rVB3	926	431	0.03%	0.003%
20	4.953	1214	1217	1221	rBV4	1101	1078	0.07%	0.008%
21	5.040	1228	1244	1280	rBV2	627077	1608436	100.00%	12.410%
22	5.326	1331	1333	1337	rBV5	1320	842	0.05%	0.006%
23	5.526	1393	1395	1401	rVB4	748	456	0.03%	0.004%
24	5.551	1401	1403	1406	rVB4	687	331	0.02%	0.003%
25	5.612	1410	1422	1456	rBV	480473	987298	61.38%	7.618%
26	5.911	1503	1515	1526	rBV	8555	19837	1.23%	0.153%
27	6.066	1550	1563	1590	rBV	357116	739881	46.00%	5.709%
28	6.355	1651	1653	1655	rBV3	773	445	0.03%	0.003%
29	6.413	1669	1671	1674	rVB3	798	421	0.03%	0.003%
30	6.432	1675	1677	1680	rVB4	910	371	0.02%	0.003%
31	6.461	1683	1686	1687	rBV4	651	352	0.02%	0.003%
32	6.506	1698	1700	1704	rVB4	694	446	0.03%	0.003%
33	6.558	1713	1716	1722	rBV4	566	601	0.04%	0.005%
34	6.599	1725	1729	1733	rBV4	955	889	0.06%	0.007%
35	6.632	1737	1739	1741	rBV3	699	353	0.02%	0.003%
36	6.886	1817	1818	1821	rBV	678	339	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028417.D
 Acq On : 07 Oct 2022 19:12
 Operator : SY/MD
 Sample : N4893-17DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.982	1835	1848	1876	rBV	219963	412771	25.66%	3.185%
38	7.310	1939	1950	1981	rBV	737247	1297872	80.69%	10.014%
39	7.619	2036	2046	2065	rBV	149340	266992	16.60%	2.060%
40	7.796	2099	2101	2104	rVB3	1082	450	0.03%	0.003%
41	7.841	2111	2115	2118	rBV5	1069	1052	0.07%	0.008%
42	7.879	2124	2127	2128	rBV3	845	498	0.03%	0.004%
43	7.969	2143	2155	2181	rBV	386421	651428	40.50%	5.026%
44	8.085	2182	2191	2229	rBV	481344	940617	58.48%	7.258%
45	8.657	2365	2369	2370	rBV3	849	583	0.04%	0.004%
46	8.693	2377	2380	2382	rBV2	852	530	0.03%	0.004%
47	8.725	2386	2390	2393	rBV6	786	694	0.04%	0.005%
48	8.783	2401	2408	2412	rBV6	1373	1472	0.09%	0.011%
49	8.847	2416	2428	2451	rBV	687787	1137722	70.73%	8.778%
50	9.136	2516	2518	2520	rBV2	880	383	0.02%	0.003%
51	9.226	2544	2546	2549	rBV3	646	427	0.03%	0.003%
52	9.242	2549	2551	2553	rVB3	1017	448	0.03%	0.003%
53	9.310	2569	2572	2573	rBV2	598	366	0.02%	0.003%
54	9.416	2603	2605	2608	rVB4	683	358	0.02%	0.003%
55	9.545	2638	2645	2646	rBV6	638	749	0.05%	0.006%
56	9.667	2682	2683	2688	rBV5	639	492	0.03%	0.004%
57	9.860	2738	2743	2744	rBV4	645	591	0.04%	0.005%
58	9.988	2780	2783	2784	rBV3	641	311	0.02%	0.002%
59	10.005	2786	2788	2792	rVB3	1407	748	0.05%	0.006%
60	10.156	2832	2835	2836	rBV3	896	528	0.03%	0.004%
61	10.210	2839	2852	2873	rVV	482720	773608	48.10%	5.969%
62	10.384	2898	2906	2913	rVB8	1312	2045	0.13%	0.016%
63	10.422	2914	2918	2920	rBV3	886	625	0.04%	0.005%
64	10.570	2960	2964	2968	rBV5	779	876	0.05%	0.007%
65	10.693	2998	3002	3008	rBV6	895	1220	0.08%	0.009%
66	10.728	3010	3013	3015	rBV4	662	409	0.03%	0.003%
67	10.792	3031	3033	3036	rBV4	898	571	0.04%	0.004%
68	10.808	3036	3038	3043	rVB5	799	717	0.04%	0.006%
69	10.918	3069	3072	3076	rBV4	984	910	0.06%	0.007%
70	10.998	3094	3097	3100	rBV4	630	486	0.03%	0.004%
71	11.017	3100	3103	3105	rBV5	559	295	0.02%	0.002%
72	11.075	3119	3121	3124	rBV2	693	418	0.03%	0.003%
73	11.239	3159	3172	3195	rBV	703323	1109146	68.96%	8.558%
74	11.426	3227	3230	3232	rBV4	875	585	0.04%	0.005%
75	11.519	3257	3259	3260	rBV2	672	281	0.02%	0.002%
76	11.615	3278	3289	3308	rBV	708938	1112849	69.19%	8.586%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028417.D
 Acq On : 07 Oct 2022 19:12
 Operator : SY/MD
 Sample : N4893-17DL 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J50DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.799	3343	3346	3349	rBV4	885	515	0.03%	0.004%
78	11.815	3349	3351	3354	rVB3	797	374	0.02%	0.003%
79	11.837	3355	3358	3360	rBV4	816	483	0.03%	0.004%
80	11.869	3366	3368	3371	rVB3	1092	593	0.04%	0.005%
81	12.008	3409	3411	3414	rVV2	1052	588	0.04%	0.005%
82	12.027	3414	3417	3422	rVB5	1056	773	0.05%	0.006%
83	12.104	3436	3441	3444	rBV6	1096	1146	0.07%	0.009%
84	12.136	3449	3451	3456	rVB4	719	572	0.04%	0.004%
85	12.336	3510	3513	3514	rBV2	509	295	0.02%	0.002%
86	12.403	3532	3534	3538	rBV3	700	346	0.02%	0.003%
87	12.500	3562	3564	3567	rBV4	715	460	0.03%	0.004%
88	12.654	3608	3612	3614	rBV4	719	483	0.03%	0.004%
89	12.773	3646	3649	3650	rBV2	732	370	0.02%	0.003%
90	12.844	3668	3671	3673	rBV2	822	484	0.03%	0.004%
91	12.963	3706	3708	3714	rVB5	750	368	0.02%	0.003%
92	13.020	3724	3726	3729	rBV4	686	438	0.03%	0.003%
93	13.303	3812	3814	3816	rBV2	709	360	0.02%	0.003%
94	13.548	3888	3890	3895	rVB3	1296	810	0.05%	0.006%
95	13.577	3895	3899	3903	rBV5	1096	1009	0.06%	0.008%
96	13.599	3903	3906	3909	rVV5	1228	822	0.05%	0.006%
97	13.625	3912	3914	3917	rVV4	780	399	0.02%	0.003%
98	13.689	3932	3934	3940	rVB6	1089	571	0.04%	0.004%
99	13.718	3940	3943	3946	rVB4	1020	581	0.04%	0.004%
100	14.432	4161	4165	4169	rVB5	1266	1080	0.07%	0.008%




Sum of corrected areas: 12960520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028417.D
Acq On : 07 Oct 2022 19:12
Operator : SY/MD
Sample : N4893-17DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

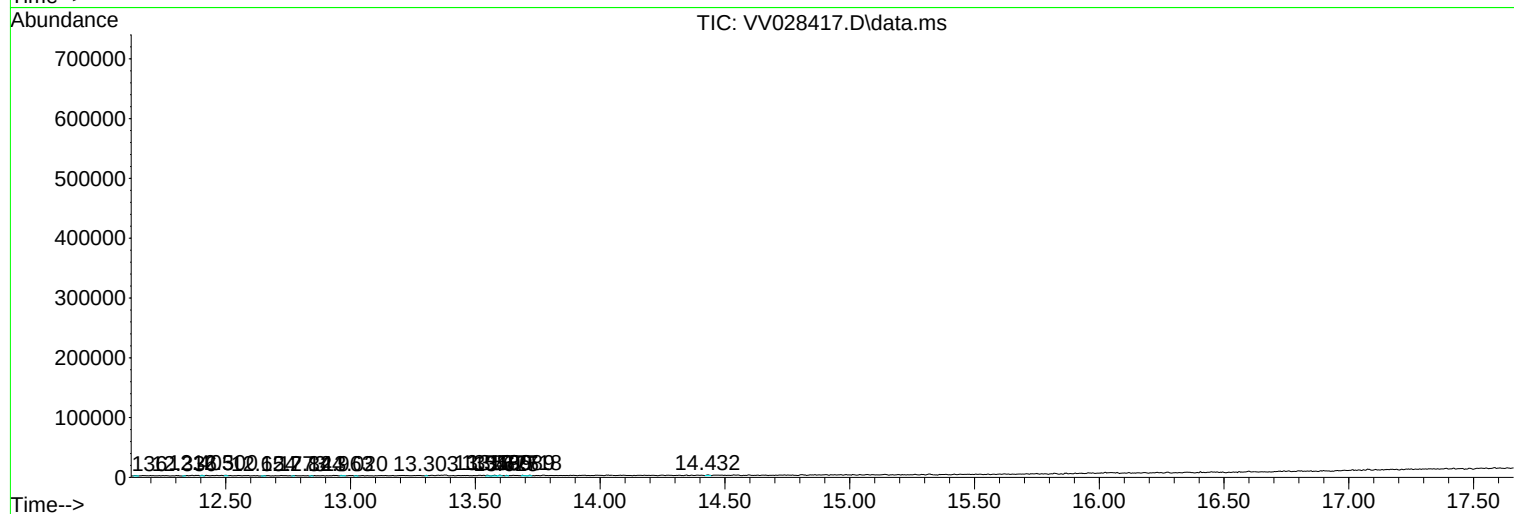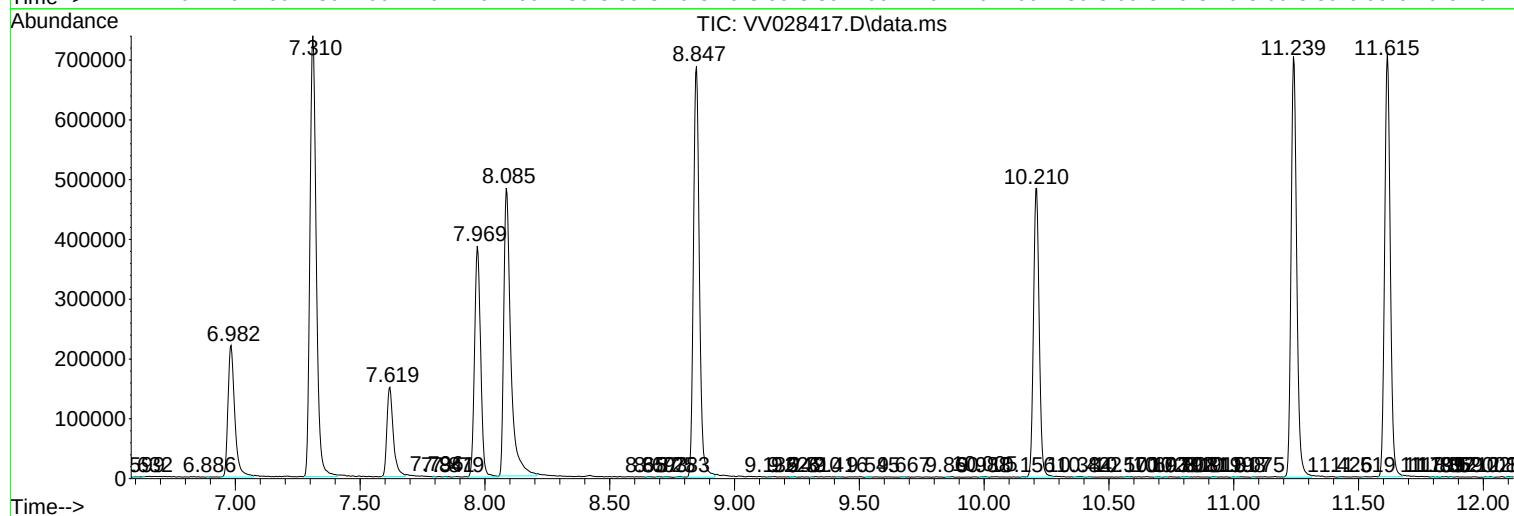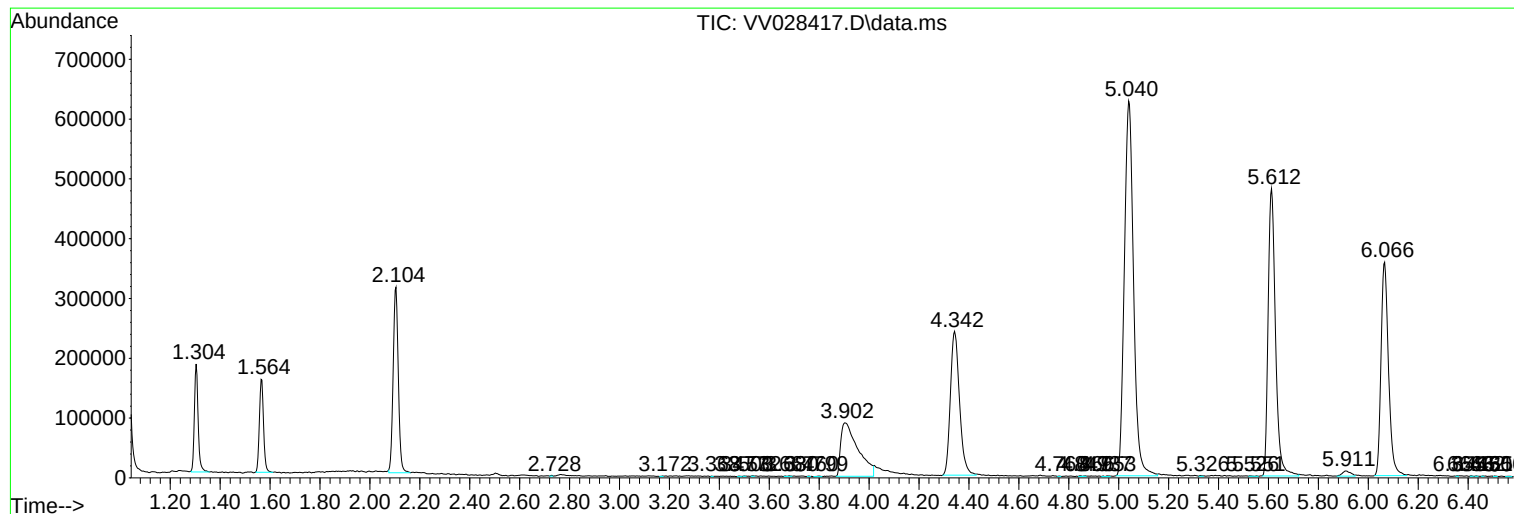

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028417.D
Acq On : 07 Oct 2022 19:12
Operator : SY/MD
Sample : N4893-17DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028417.D
Acq On : 07 Oct 2022 19:12
Operator : SY/MD
Sample : N4893-17DL 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J50DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc