

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028419.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.207	48	52	64	rBV	35954	32474	2.02%	0.266%
2	1.304	76	82	99	rVB	179218	184929	11.50%	1.514%
3	1.564	157	163	176	rVB	155543	180601	11.23%	1.479%
4	2.101	322	330	344	rVB	305979	430987	26.80%	3.529%
5	2.818	551	553	557	rBV5	1054	725	0.05%	0.006%
6	3.040	620	622	624	rBV4	595	385	0.02%	0.003%
7	3.124	645	648	651	rBV4	750	456	0.03%	0.004%
8	3.140	651	653	656	rBV3	552	378	0.02%	0.003%
9	3.204	670	673	676	rBV4	602	478	0.03%	0.004%
10	3.252	685	688	690	rBV3	503	300	0.02%	0.002%
11	3.272	693	694	696	rBV	709	360	0.02%	0.003%
12	3.362	719	722	724	rBV3	672	469	0.03%	0.004%
13	3.407	733	736	740	rVB4	561	407	0.03%	0.003%
14	3.465	752	754	757	rBV3	646	420	0.03%	0.003%
15	3.529	772	774	777	rBV2	648	351	0.02%	0.003%
16	3.693	822	825	826	rBV3	550	308	0.02%	0.003%
17	3.815	861	863	871	rVB5	704	704	0.04%	0.006%
18	3.895	873	888	928	rBV	93060	407545	25.34%	3.337%
19	4.342	1013	1027	1064	rVB	247164	635852	39.54%	5.207%
20	4.751	1150	1154	1157	rBV5	1256	1029	0.06%	0.008%
21	4.786	1163	1165	1170	rBV5	446	377	0.02%	0.003%
22	4.825	1175	1177	1179	rVV3	633	275	0.02%	0.002%
23	5.040	1228	1244	1273	rBV2	621296	1608158	100.00%	13.168%
24	5.612	1410	1422	1446	rBV	463693	939488	58.42%	7.693%
25	6.063	1549	1562	1594	rBV	359870	749433	46.60%	6.137%
26	6.371	1656	1658	1660	rBV3	888	483	0.03%	0.004%
27	6.452	1679	1683	1684	rBV3	745	522	0.03%	0.004%
28	6.513	1699	1702	1707	rVB6	1281	1182	0.07%	0.010%
29	6.538	1707	1710	1712	rBV3	1101	519	0.03%	0.004%
30	6.555	1712	1715	1717	rBV4	422	286	0.02%	0.002%
31	6.638	1737	1741	1743	rBV4	1275	991	0.06%	0.008%
32	6.828	1798	1800	1801	rBV2	676	294	0.02%	0.002%
33	6.854	1805	1808	1811	rVV3	855	688	0.04%	0.006%
34	6.882	1815	1817	1820	rBV2	722	383	0.02%	0.003%
35	6.982	1836	1848	1867	rBV	219020	403536	25.09%	3.304%
36	7.310	1939	1950	1978	rBV	746550	1297440	80.68%	10.624%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.616	2036	2045	2070	rBV	157106	288142	17.92%	2.359%
38	7.889	2127	2130	2132	rBV2	974	594	0.04%	0.005%
39	7.905	2132	2135	2136	rBV3	781	440	0.03%	0.004%
40	8.085	2181	2191	2228	rBV	448468	917800	57.07%	7.515%
41	8.461	2304	2308	2310	rBV4	1067	809	0.05%	0.007%
42	8.657	2366	2369	2372	rBV5	579	353	0.02%	0.003%
43	8.776	2403	2406	2407	rBV3	554	317	0.02%	0.003%
44	8.847	2415	2428	2451	rBV	659098	1102394	68.55%	9.027%
45	9.207	2538	2540	2543	rVB4	795	406	0.03%	0.003%
46	9.239	2543	2550	2553	rBV6	1277	1454	0.09%	0.012%
47	9.297	2564	2568	2569	rVV3	713	488	0.03%	0.004%
48	9.310	2569	2572	2574	rVV4	1283	769	0.05%	0.006%
49	9.416	2601	2605	2608	rBV4	723	584	0.04%	0.005%
50	9.477	2622	2624	2627	rVB3	786	355	0.02%	0.003%
51	9.493	2627	2629	2630	rBV2	554	304	0.02%	0.002%
52	9.699	2690	2693	2694	rBV3	653	297	0.02%	0.002%
53	9.905	2751	2757	2758	rBV6	861	780	0.05%	0.006%
54	9.956	2772	2773	2777	rBV4	612	347	0.02%	0.003%
55	9.998	2783	2786	2787	rBV2	495	321	0.02%	0.003%
56	10.024	2790	2794	2795	rBV3	1082	777	0.05%	0.006%
57	10.107	2818	2820	2824	rVB5	733	360	0.02%	0.003%
58	10.207	2839	2851	2871	rBV	477862	767441	47.72%	6.284%
59	10.632	2980	2983	2984	rBV3	573	350	0.02%	0.003%
60	10.686	2993	3000	3004	rBV6	904	1001	0.06%	0.008%
61	10.750	3017	3020	3022	rBV2	756	527	0.03%	0.004%
62	10.789	3029	3032	3034	rVB4	951	479	0.03%	0.004%
63	10.808	3037	3038	3040	rBV3	547	282	0.02%	0.002%
64	10.841	3043	3048	3052	rBV6	1166	1547	0.10%	0.013%
65	11.239	3161	3172	3192	rBV	683321	1066276	66.30%	8.731%
66	11.480	3243	3247	3251	rBV5	862	710	0.04%	0.006%
67	11.529	3251	3262	3274	rBV3	17845	35076	2.18%	0.287%
68	11.615	3278	3289	3318	rVB	711854	1117795	69.51%	9.153%
69	11.921	3382	3384	3389	rVB4	1040	702	0.04%	0.006%
70	11.947	3389	3392	3395	rBV3	906	605	0.04%	0.005%
71	12.149	3451	3455	3460	rVB7	1036	1049	0.07%	0.009%
72	12.175	3460	3463	3465	rBV4	739	422	0.03%	0.003%
73	12.426	3538	3541	3543	rVB2	880	412	0.03%	0.003%
74	12.442	3543	3546	3548	rBV4	587	356	0.02%	0.003%
75	12.545	3575	3578	3579	rBV3	680	383	0.02%	0.003%
76	12.660	3610	3614	3617	rVB4	871	787	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028419.D
 Acq On : 07 Oct 2022 20:00
 Operator : SY/MD
 Sample : N4893-19
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 F5J63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.766	3645	3647	3650	rVB2	1051	537	0.03%	0.004%
78	12.799	3655	3657	3660	rVV4	572	335	0.02%	0.003%
79	12.818	3660	3663	3665	rBV4	663	350	0.02%	0.003%
80	12.879	3679	3682	3684	rVB2	1074	497	0.03%	0.004%
81	12.895	3684	3687	3693	rBV6	1177	1052	0.07%	0.009%
82	12.950	3701	3704	3707	rBV5	774	386	0.02%	0.003%
83	12.998	3715	3719	3724	rBV5	1225	952	0.06%	0.008%
84	13.020	3724	3726	3727	rBV	647	299	0.02%	0.002%
85	13.056	3735	3737	3743	rVB5	693	452	0.03%	0.004%
86	13.197	3779	3781	3784	rBV3	627	399	0.02%	0.003%
87	13.246	3794	3796	3799	rBV2	911	692	0.04%	0.006%
88	13.438	3853	3856	3860	rVB4	1519	1002	0.06%	0.008%
89	13.593	3900	3904	3905	rBV2	911	627	0.04%	0.005%
90	13.609	3907	3909	3911	rVV3	946	439	0.03%	0.004%
91	13.680	3927	3931	3934	rBV5	1313	869	0.05%	0.007%
92	13.792	3963	3966	3968	rBV3	842	432	0.03%	0.004%
93	13.802	3968	3969	3973	rBV4	799	608	0.04%	0.005%
94	13.863	3984	3988	3990	rBV3	1355	1121	0.07%	0.009%
95	13.953	4014	4016	4020	rVB4	1038	611	0.04%	0.005%
96	14.049	4044	4046	4048	rBV2	712	294	0.02%	0.002%
97	14.152	4076	4078	4081	rBV3	923	607	0.04%	0.005%
98	14.188	4086	4089	4092	rBV3	742	642	0.04%	0.005%
99	14.429	4162	4164	4167	rBV4	885	513	0.03%	0.004%
100	15.053	4356	4358	4361	rBV3	1394	1071	0.07%	0.009%




Sum of corrected areas: 12212291

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028419.D
Acq On : 07 Oct 2022 20:00
Operator : SY/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

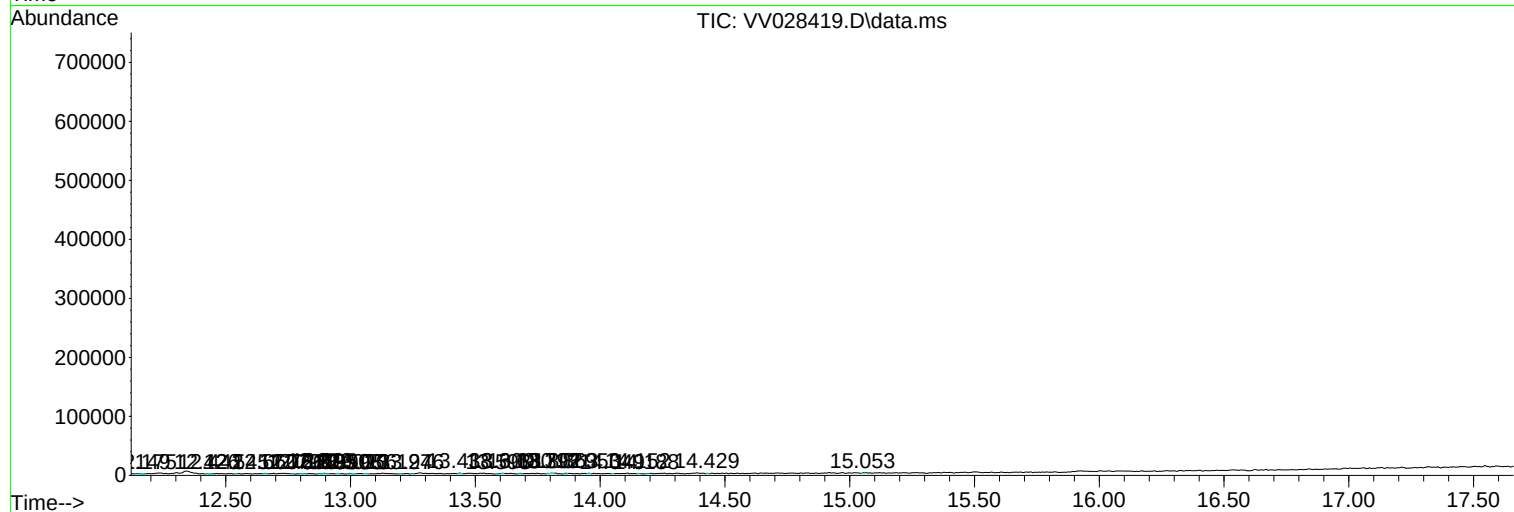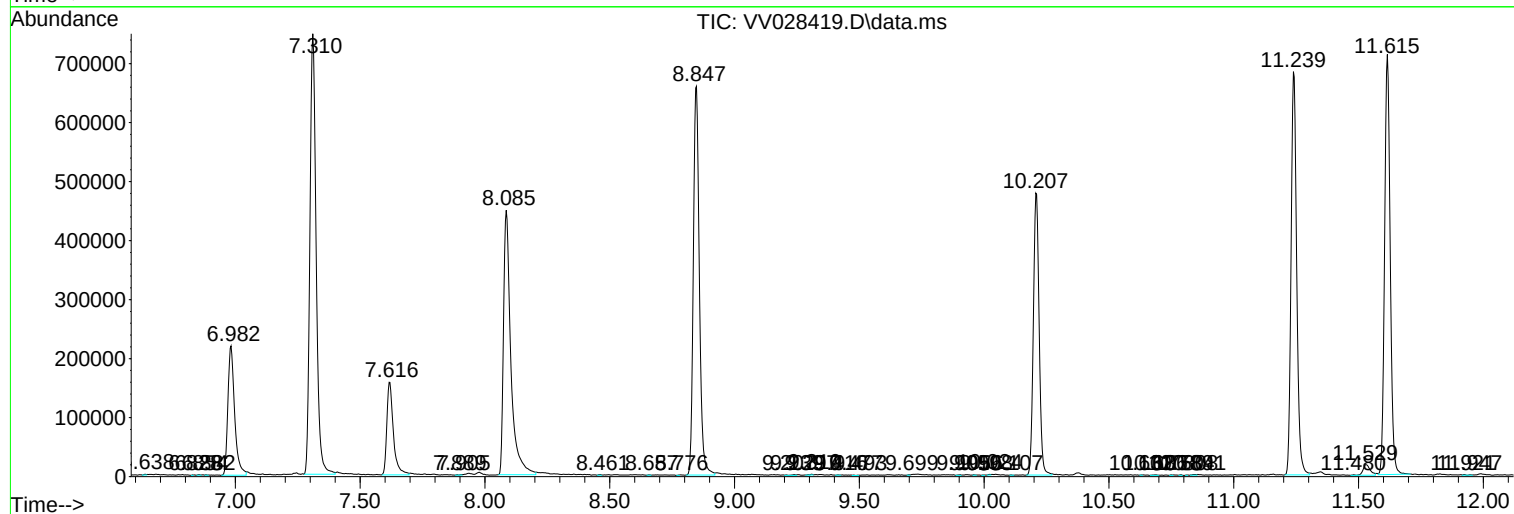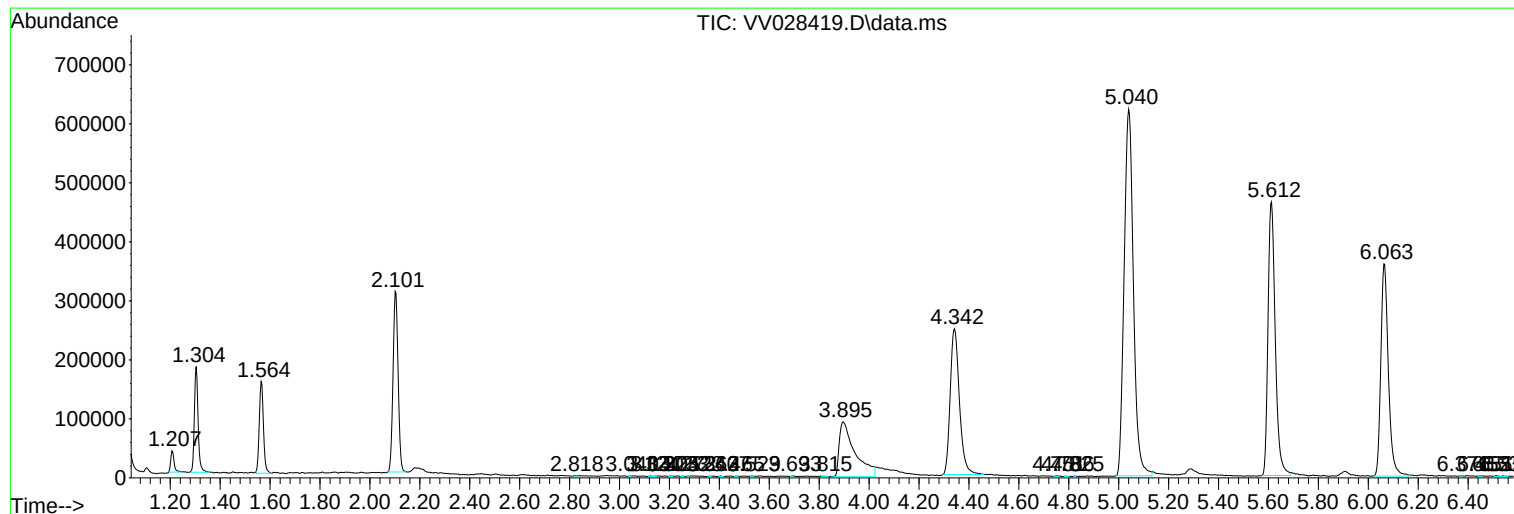

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028419.D
Acq On : 07 Oct 2022 20:00
Operator : SY/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028419.D
Acq On : 07 Oct 2022 20:00
Operator : SY/MD
Sample : N4893-19
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
F5J63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc