

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028421.D
 Acq On : 07 Oct 2022 20:48
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028421.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	189127	190053	11.96%	1.596%
2	1.564	156	163	173	rBV	154564	174758	10.99%	1.468%
3	2.105	322	331	345	rVB	297260	424719	26.72%	3.567%
4	2.455	437	440	442	rBV3	1159	683	0.04%	0.006%
5	2.593	481	483	486	rBV2	657	455	0.03%	0.004%
6	2.693	510	514	517	rBV2	946	979	0.06%	0.008%
7	2.764	535	536	540	rVB2	988	458	0.03%	0.004%
8	2.896	574	577	578	rBV3	900	530	0.03%	0.004%
9	3.018	611	615	617	rBV4	1234	805	0.05%	0.007%
10	3.082	632	635	639	rBV4	538	397	0.02%	0.003%
11	3.179	663	665	668	rBV3	1043	740	0.05%	0.006%
12	3.191	668	669	675	rVB3	1634	695	0.04%	0.006%
13	3.333	704	713	716	rBV6	1008	1141	0.07%	0.010%
14	3.375	724	726	731	rVB3	912	576	0.04%	0.005%
15	3.661	811	815	817	rBV4	437	408	0.03%	0.003%
16	3.780	848	852	855	rBV4	820	471	0.03%	0.004%
17	3.841	869	871	874	rBV4	538	382	0.02%	0.003%
18	3.908	880	892	937	rBV	78542	411298	25.87%	3.455%
19	4.342	1014	1027	1057	rVB	234914	591717	37.22%	4.970%
20	4.629	1114	1116	1121	rVB5	1187	684	0.04%	0.006%
21	4.793	1164	1167	1171	rVB4	925	673	0.04%	0.006%
22	4.960	1216	1219	1222	rVB5	806	499	0.03%	0.004%
23	5.040	1222	1244	1285	rBV2	613191	1589593	100.00%	13.352%
24	5.436	1364	1367	1369	rBV4	711	433	0.03%	0.004%
25	5.487	1380	1383	1384	rBV3	633	369	0.02%	0.003%
26	5.558	1402	1405	1408	rBV4	747	505	0.03%	0.004%
27	5.613	1410	1422	1451	rVV	452906	926346	58.28%	7.781%
28	5.825	1486	1488	1492	rBV4	1033	478	0.03%	0.004%
29	5.908	1504	1514	1532	rBV7	6094	13122	0.83%	0.110%
30	6.066	1550	1563	1589	rBV	344647	719051	45.23%	6.040%
31	6.330	1642	1645	1647	rBV3	1144	712	0.04%	0.006%
32	6.358	1652	1654	1656	rBV3	608	293	0.02%	0.002%
33	6.490	1691	1695	1701	rVB7	909	1141	0.07%	0.010%
34	6.522	1701	1705	1707	rBV2	497	352	0.02%	0.003%
35	6.580	1721	1723	1727	rBV5	661	451	0.03%	0.004%
36	6.638	1738	1741	1742	rBV2	722	369	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028421.D
 Acq On : 07 Oct 2022 20:48
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.834	1797	1802	1805	rBV5	982	718	0.05%	0.006%
38	6.863	1809	1811	1814	rBV3	597	336	0.02%	0.003%
39	6.982	1835	1848	1872	rBV	213033	399627	25.14%	3.357%
40	7.310	1934	1950	1973	rBV	724555	1271089	79.96%	10.676%
41	7.616	2036	2045	2075	rBV2	141790	259483	16.32%	2.180%
42	7.921	2137	2140	2142	rBV3	1143	661	0.04%	0.006%
43	7.973	2153	2156	2159	rBV5	1099	913	0.06%	0.008%
44	8.008	2164	2167	2170	rBV4	570	376	0.02%	0.003%
45	8.085	2181	2191	2233	rBV	460702	941066	59.20%	7.904%
46	8.603	2351	2352	2358	rVB4	702	532	0.03%	0.004%
47	8.632	2358	2361	2364	rBV4	675	523	0.03%	0.004%
48	8.686	2375	2378	2382	rBV3	773	526	0.03%	0.004%
49	8.847	2414	2428	2456	rBV	645421	1081530	68.04%	9.084%
50	9.153	2518	2523	2526	rVB4	1500	1270	0.08%	0.011%
51	9.181	2526	2532	2534	rBV5	866	899	0.06%	0.008%
52	9.275	2557	2561	2562	rBV4	464	302	0.02%	0.003%
53	9.297	2565	2568	2573	rVB5	1127	1110	0.07%	0.009%
54	9.394	2595	2598	2600	rBV2	734	436	0.03%	0.004%
55	9.455	2611	2617	2619	rBV5	1106	952	0.06%	0.008%
56	9.509	2631	2634	2636	rVB2	659	303	0.02%	0.003%
57	9.571	2651	2653	2656	rVB3	682	307	0.02%	0.003%
58	9.596	2656	2661	2664	rBV6	591	569	0.04%	0.005%
59	9.686	2684	2689	2693	rBV5	605	630	0.04%	0.005%
60	9.818	2726	2730	2733	rBV3	457	448	0.03%	0.004%
61	9.931	2758	2765	2769	rVB8	875	979	0.06%	0.008%
62	9.953	2769	2772	2775	rBV4	755	604	0.04%	0.005%
63	9.992	2781	2784	2786	rBV4	662	426	0.03%	0.004%
64	10.034	2792	2797	2799	rBV3	708	585	0.04%	0.005%
65	10.165	2835	2838	2839	rVV2	525	319	0.02%	0.003%
66	10.207	2839	2851	2873	rVV	476823	758951	47.74%	6.375%
67	10.345	2892	2894	2896	rBV3	717	454	0.03%	0.004%
68	10.452	2923	2927	2930	rBV4	682	499	0.03%	0.004%
69	10.516	2943	2947	2948	rBV3	612	406	0.03%	0.003%
70	10.599	2970	2973	2976	rBV3	569	326	0.02%	0.003%
71	10.635	2982	2984	2987	rVB4	750	376	0.02%	0.003%
72	10.680	2996	2998	3001	rVB4	765	407	0.03%	0.003%
73	10.792	3029	3033	3037	rVB6	1044	911	0.06%	0.008%
74	10.818	3037	3041	3043	rBV4	784	546	0.03%	0.005%
75	10.844	3047	3049	3053	rVV3	418	292	0.02%	0.002%
76	10.908	3067	3069	3071	rBV3	658	285	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028421.D
 Acq On : 07 Oct 2022 20:48
 Operator : SY/MD
 Sample : N4893-20
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.162	3146	3148	3151	rBV3	586	378	0.02%	0.003%
78	11.239	3161	3172	3193	rBV	654836	1031531	64.89%	8.664%
79	11.615	3277	3289	3309	rBV	666276	1074303	67.58%	9.024%
80	11.911	3378	3381	3384	rBV2	748	567	0.04%	0.005%
81	11.972	3396	3400	3401	rBV3	524	356	0.02%	0.003%
82	12.062	3421	3428	3431	rBV4	515	758	0.05%	0.006%
83	12.156	3454	3457	3460	rBV3	612	389	0.02%	0.003%
84	12.516	3565	3569	3575	rBV6	945	898	0.06%	0.008%
85	12.570	3582	3586	3589	rBV3	875	897	0.06%	0.008%
86	12.593	3591	3593	3594	rBV2	743	305	0.02%	0.003%
87	12.664	3612	3615	3617	rBV3	721	420	0.03%	0.004%
88	12.821	3661	3664	3666	rBV3	590	348	0.02%	0.003%
89	12.927	3695	3697	3698	rBV	696	365	0.02%	0.003%
90	12.953	3703	3705	3708	rVV4	805	388	0.02%	0.003%
91	13.011	3721	3723	3725	rBV3	507	280	0.02%	0.002%
92	13.197	3779	3781	3784	rBV2	466	281	0.02%	0.002%
93	13.513	3877	3879	3882	rBV4	663	504	0.03%	0.004%
94	13.558	3891	3893	3896	rBV2	475	297	0.02%	0.002%
95	13.783	3958	3963	3966	rBV5	1098	1085	0.07%	0.009%
96	13.799	3966	3968	3970	rBV2	714	514	0.03%	0.004%
97	13.837	3977	3980	3981	rBV	1095	684	0.04%	0.006%
98	13.902	3992	4000	4002	rBV8	1224	1506	0.09%	0.013%
99	14.345	4136	4138	4140	rBV2	724	404	0.03%	0.003%
100	14.477	4177	4179	4183	rBV5	981	827	0.05%	0.007%




Sum of corrected areas: 11905593

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028421.D
Acq On : 07 Oct 2022 20:48
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

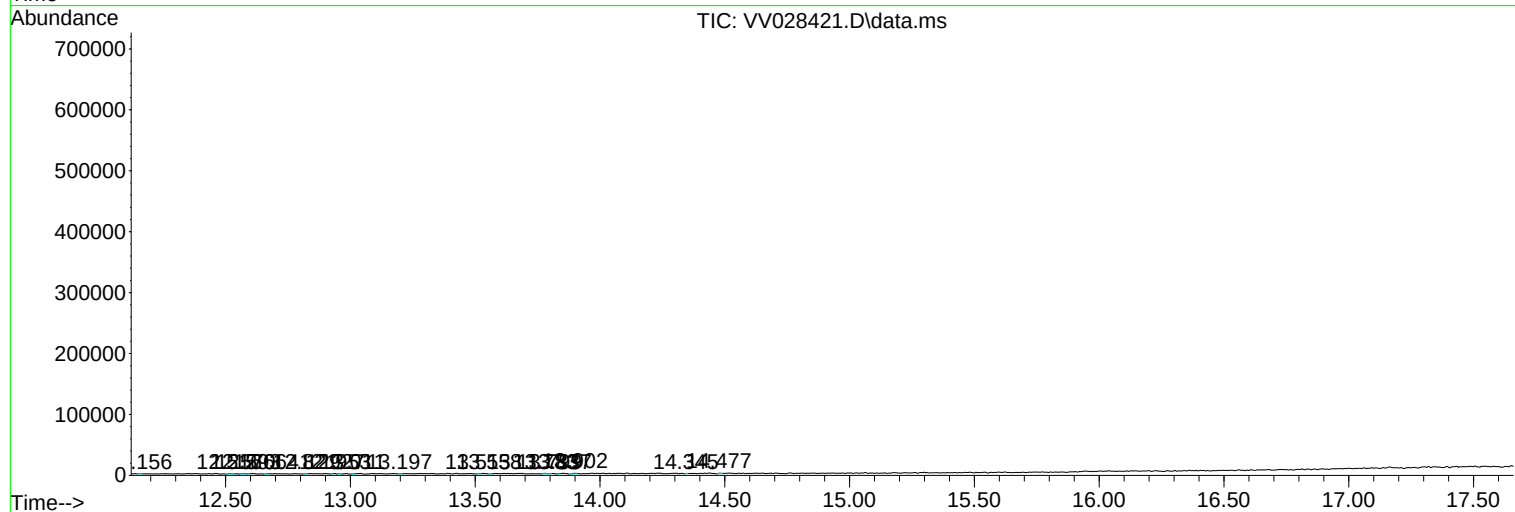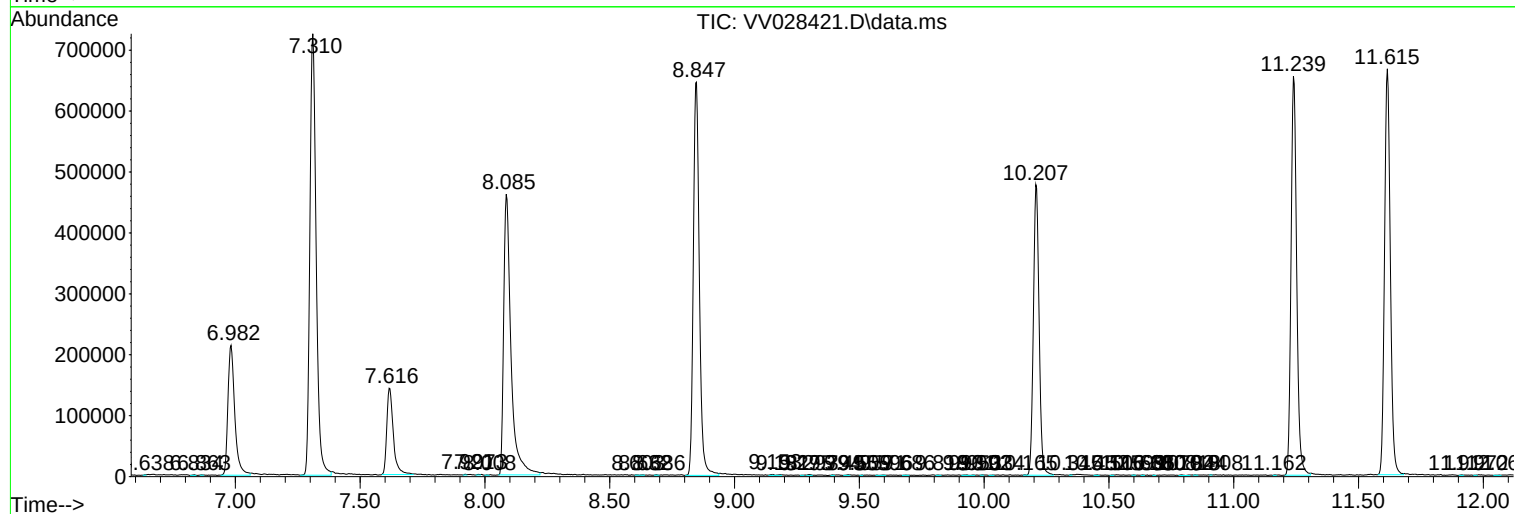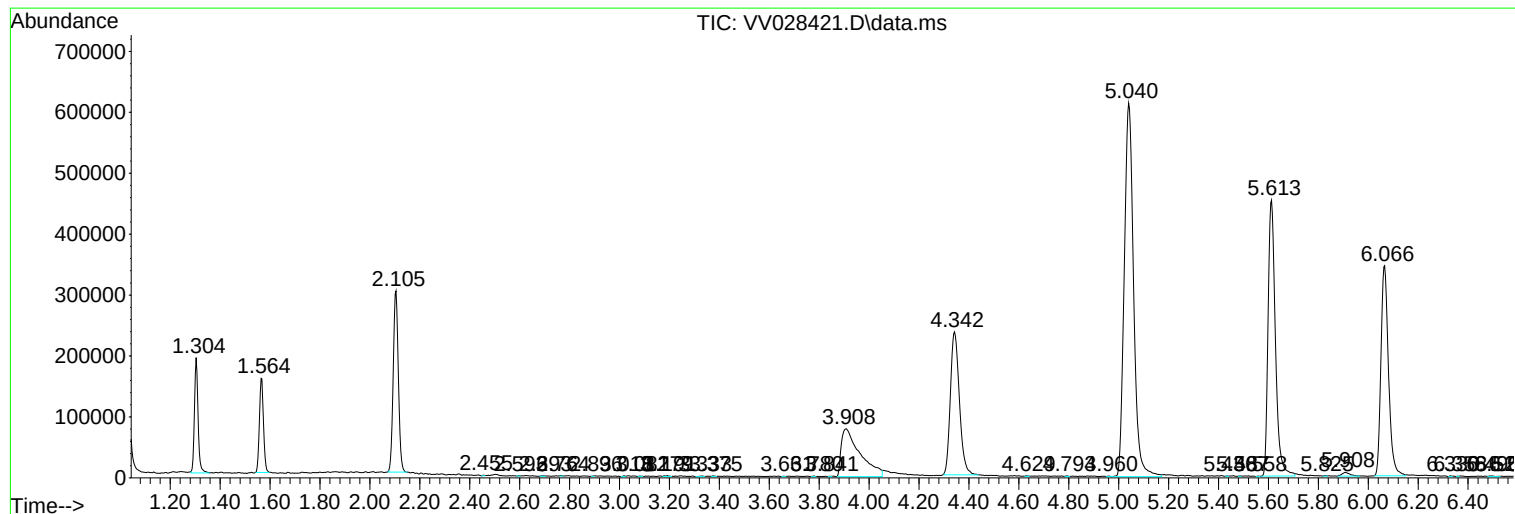

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028421.D
Acq On : 07 Oct 2022 20:48
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028421.D
Acq On : 07 Oct 2022 20:48
Operator : SY/MD
Sample : N4893-20
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------