

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028422.D
 Acq On : 07 Oct 2022 21:12
 Operator : SY/MD
 Sample : N4889-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028422.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	99	rVB	170270	179154	11.11%	1.302%
2	1.564	156	163	175	rVB	151942	174299	10.81%	1.267%
3	2.101	321	330	349	rVB	286947	417978	25.93%	3.038%
4	2.715	518	521	527	rBV5	1087	1397	0.09%	0.010%
5	2.908	577	581	585	rVB5	947	856	0.05%	0.006%
6	3.137	650	652	655	rVV2	675	404	0.03%	0.003%
7	3.256	688	689	692	rBV2	545	323	0.02%	0.002%
8	3.275	692	695	698	rVB3	589	318	0.02%	0.002%
9	3.461	751	753	756	rBV4	660	484	0.03%	0.004%
10	3.584	789	791	794	rBV3	830	522	0.03%	0.004%
11	3.664	814	816	819	rVB3	848	418	0.03%	0.003%
12	3.683	819	822	824	rBV3	601	388	0.02%	0.003%
13	3.748	840	842	844	rBV2	704	330	0.02%	0.002%
14	3.841	866	871	874	rVB4	821	898	0.06%	0.007%
15	3.905	874	891	936	rBV3	100424	506070	31.39%	3.678%
16	4.342	1014	1027	1050	rVB	241933	589663	36.58%	4.285%
17	4.577	1097	1100	1101	rBV2	752	423	0.03%	0.003%
18	4.651	1121	1123	1125	rBV3	1193	659	0.04%	0.005%
19	4.825	1174	1177	1179	rBV4	691	418	0.03%	0.003%
20	5.040	1227	1244	1284	rBV2	615957	1611968	100.00%	11.715%
21	5.484	1380	1382	1384	rBV3	944	495	0.03%	0.004%
22	5.612	1410	1422	1448	rBV	447520	910800	56.50%	6.619%
23	5.831	1488	1490	1493	rBV2	1158	543	0.03%	0.004%
24	6.066	1546	1563	1590	rBV2	356357	759294	47.10%	5.518%
25	6.619	1732	1735	1736	rBV3	869	463	0.03%	0.003%
26	6.982	1837	1848	1875	rBV	216647	404979	25.12%	2.943%
27	7.172	1903	1907	1909	rBV3	1077	872	0.05%	0.006%
28	7.310	1939	1950	1974	rBV	727119	1249091	77.49%	9.078%
29	7.513	2010	2013	2015	rBV3	1144	661	0.04%	0.005%
30	7.616	2036	2045	2067	rBV	147403	269726	16.73%	1.960%
31	7.876	2123	2126	2132	rBV7	1090	1014	0.06%	0.007%
32	7.969	2153	2155	2157	rBV3	1089	641	0.04%	0.005%
33	8.024	2170	2172	2175	rBV4	848	536	0.03%	0.004%
34	8.085	2179	2191	2223	rBV	491807	964157	59.81%	7.007%
35	8.799	2408	2413	2414	rBV4	901	599	0.04%	0.004%
36	8.844	2417	2427	2448	rBV	623580	1037322	64.35%	7.539%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028422.D
 Acq On : 07 Oct 2022 21:12
 Operator : SY/MD
 Sample : N4889-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	9.011	2470	2479	2494	rBV	33695	56089	3.48%	0.408%
38	9.130	2504	2516	2550	rVB	955972	1539842	95.53%	11.191%
39	9.384	2592	2595	2598	rBV5	795	552	0.03%	0.004%
40	9.445	2610	2614	2617	rBV4	657	572	0.04%	0.004%
41	9.471	2617	2622	2623	rBV3	1200	867	0.05%	0.006%
42	9.583	2653	2657	2658	rBV3	627	426	0.03%	0.003%
43	9.696	2689	2692	2696	rVB4	1200	556	0.03%	0.004%
44	9.718	2696	2699	2702	rBV3	658	428	0.03%	0.003%
45	9.760	2710	2712	2715	rVB4	761	444	0.03%	0.003%
46	9.796	2719	2723	2727	rBV4	1098	879	0.05%	0.006%
47	9.831	2730	2734	2735	rBV4	489	327	0.02%	0.002%
48	9.927	2755	2764	2773	rBV2	10170	16546	1.03%	0.120%
49	10.066	2804	2807	2808	rBV2	662	380	0.02%	0.003%
50	10.165	2830	2838	2840	rBV8	849	1030	0.06%	0.007%
51	10.207	2840	2851	2867	rBV	490835	782735	48.56%	5.689%
52	10.349	2883	2895	2904	rBV	8540	15702	0.97%	0.114%
53	10.445	2915	2925	2941	rBV	17501	33232	2.06%	0.242%
54	10.535	2945	2953	2965	rVV2	13947	21853	1.36%	0.159%
55	10.606	2973	2975	2979	rBV5	601	442	0.03%	0.003%
56	10.734	3004	3015	3022	rBV2	10323	16784	1.04%	0.122%
57	10.818	3040	3041	3046	rVB3	1161	707	0.04%	0.005%
58	10.911	3061	3070	3083	rBV	37403	59526	3.69%	0.433%
59	11.001	3095	3098	3100	rBV3	737	356	0.02%	0.003%
60	11.037	3105	3109	3110	rBV3	999	591	0.04%	0.004%
61	11.140	3140	3141	3144	rBV3	462	319	0.02%	0.002%
62	11.181	3149	3154	3155	rBV4	2600	1795	0.11%	0.013%
63	11.239	3161	3172	3192	rBV	638198	999501	62.01%	7.264%
64	11.429	3228	3231	3232	rBV2	1041	577	0.04%	0.004%
65	11.615	3278	3289	3312	rVB	683014	1079972	67.00%	7.849%
66	11.815	3345	3351	3359	rVB5	2200	3099	0.19%	0.023%
67	11.979	3398	3402	3403	rBV3	1291	656	0.04%	0.005%
68	12.088	3433	3436	3437	rBV3	937	480	0.03%	0.003%
69	12.217	3473	3476	3480	rVB5	572	385	0.02%	0.003%
70	12.275	3492	3494	3496	rBV2	1022	471	0.03%	0.003%
71	12.458	3544	3551	3560	rVB8	2874	4697	0.29%	0.034%
72	12.516	3567	3569	3576	rVB5	769	627	0.04%	0.005%
73	12.558	3579	3582	3586	rVB3	992	557	0.03%	0.004%
74	12.583	3586	3590	3592	rBV3	638	454	0.03%	0.003%
75	12.631	3603	3605	3608	rBV3	757	448	0.03%	0.003%
76	12.693	3621	3624	3627	rBV4	914	603	0.04%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028422.D
 Acq On : 07 Oct 2022 21:12
 Operator : SY/MD
 Sample : N4889-01 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ59

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.876	3673	3681	3691	rVB9	6396	10280	0.64%	0.075%
78	12.937	3699	3700	3704	rVB2	902	332	0.02%	0.002%
79	12.959	3704	3707	3709	rBV2	738	474	0.03%	0.003%
80	12.985	3709	3715	3720	rBV7	935	1074	0.07%	0.008%
81	13.008	3720	3722	3725	rBV3	615	481	0.03%	0.003%
82	13.033	3725	3730	3731	rBV4	2451	1844	0.11%	0.013%
83	13.085	3743	3746	3747	rBV3	757	342	0.02%	0.002%
84	13.149	3764	3766	3767	rBV	806	374	0.02%	0.003%
85	13.197	3777	3781	3783	rBV3	626	406	0.03%	0.003%
86	13.239	3790	3794	3796	rBV2	1022	674	0.04%	0.005%
87	13.313	3812	3817	3819	rBV5	809	732	0.05%	0.005%
88	13.365	3830	3833	3834	rBV4	843	471	0.03%	0.003%
89	13.413	3845	3848	3850	rBV3	1271	811	0.05%	0.006%
90	13.451	3855	3860	3863	rBV7	890	958	0.06%	0.007%
91	13.509	3871	3878	3881	rBV7	1824	2287	0.14%	0.017%
92	13.583	3898	3901	3902	rBV3	882	483	0.03%	0.004%
93	13.680	3928	3931	3932	rBV3	561	326	0.02%	0.002%
94	13.712	3937	3941	3944	rVB6	827	661	0.04%	0.005%
95	13.728	3944	3946	3948	rBV3	717	372	0.02%	0.003%
96	13.869	3987	3990	3991	rBV3	989	378	0.02%	0.003%
97	14.165	4080	4082	4086	rBV3	591	460	0.03%	0.003%
98	14.303	4124	4125	4128	rBV2	847	450	0.03%	0.003%
99	14.554	4201	4203	4206	rBV5	969	730	0.05%	0.005%
100	14.837	4289	4291	4293	rBV4	1036	502	0.03%	0.004%


Sum of corrected areas: 13759572

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028422.D
Acq On : 07 Oct 2022 21:12
Operator : SY/MD
Sample : N4889-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

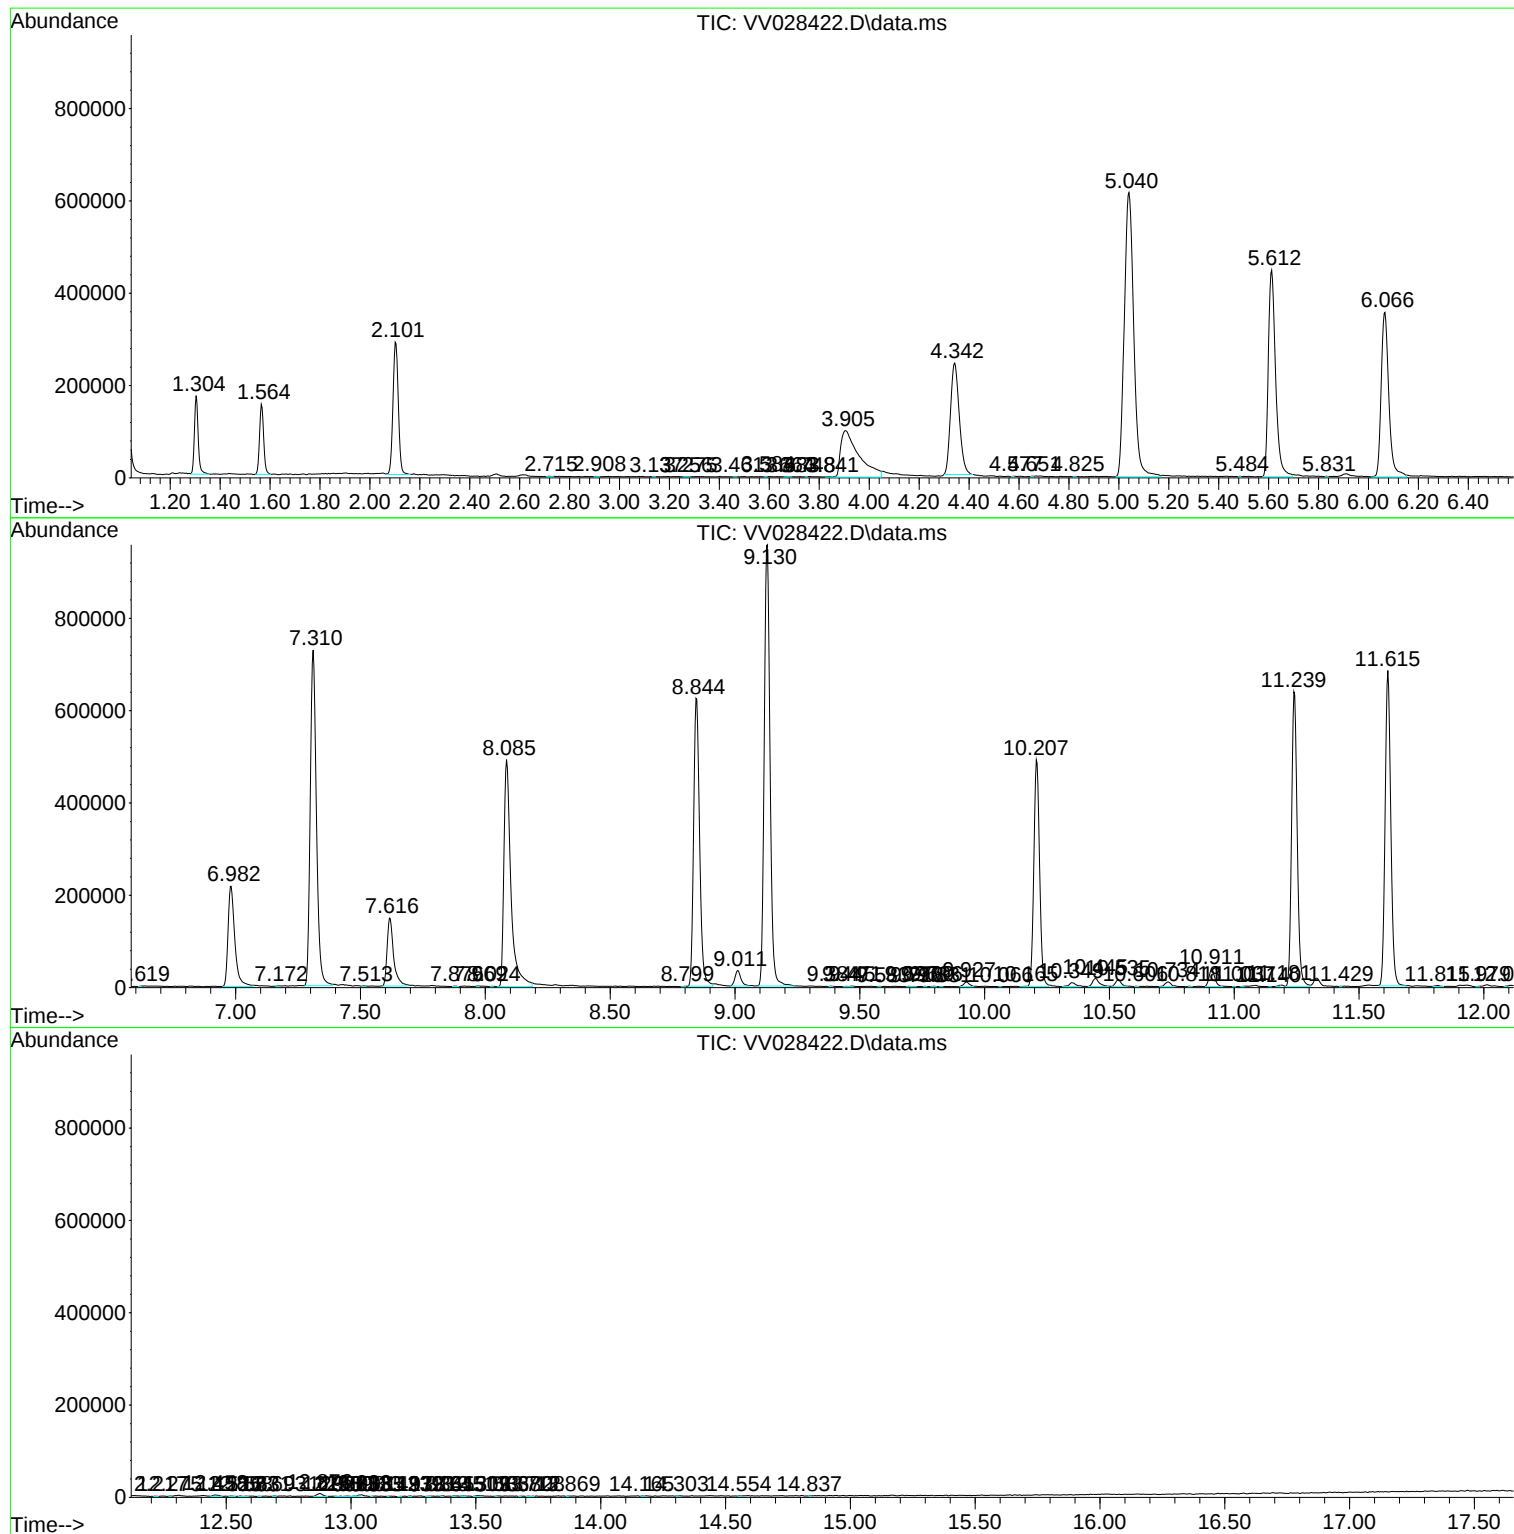

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028422.D
Acq On : 07 Oct 2022 21:12
Operator : SY/MD
Sample : N4889-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028422.D
Acq On : 07 Oct 2022 21:12
Operator : SY/MD
Sample : N4889-01 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ59

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc