

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028424.D
 Acq On : 07 Oct 2022 22:01
 Operator : SY/MD
 Sample : N4889-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028424.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	164855	170521	10.96%	1.227%
2	1.565	156	163	178	rVB	145434	168508	10.83%	1.212%
3	2.105	322	331	349	rVB	276939	406838	26.15%	2.927%
4	2.693	509	514	518	rBV5	833	765	0.05%	0.006%
5	2.712	518	520	524	rBV4	995	741	0.05%	0.005%
6	2.847	559	562	565	rBV4	649	531	0.03%	0.004%
7	2.889	570	575	579	rBV5	795	754	0.05%	0.005%
8	3.063	627	629	630	rBV	588	237	0.02%	0.002%
9	3.269	691	693	694	rBV2	517	243	0.02%	0.002%
10	3.401	731	734	740	rBV4	1098	1308	0.08%	0.009%
11	3.423	740	741	743	rBV2	444	222	0.01%	0.002%
12	3.487	758	761	763	rBV3	570	330	0.02%	0.002%
13	3.564	782	785	788	rBV2	991	718	0.05%	0.005%
14	3.581	788	790	792	rBV2	558	292	0.02%	0.002%
15	3.642	807	809	811	rVB3	788	289	0.02%	0.002%
16	3.677	818	820	821	rBV2	540	215	0.01%	0.002%
17	3.687	821	823	825	rBV4	515	185	0.01%	0.001%
18	3.728	834	836	838	rBV2	598	325	0.02%	0.002%
19	3.745	838	841	843	rVV4	1265	764	0.05%	0.005%
20	3.777	848	851	853	rBV	507	267	0.02%	0.002%
21	3.825	863	866	868	rBV4	563	384	0.02%	0.003%
22	3.905	876	891	935	rBV	88491	447374	28.75%	3.219%
23	4.343	1012	1027	1058	rBV	233057	586723	37.71%	4.221%
24	4.629	1112	1116	1118	rBV3	860	614	0.04%	0.004%
25	4.899	1198	1200	1203	rBV4	952	663	0.04%	0.005%
26	4.957	1216	1218	1221	rVB5	557	347	0.02%	0.002%
27	5.040	1225	1244	1280	rBV2	600470	1555876	100.00%	11.193%
28	5.519	1389	1393	1401	rBV9	1255	2008	0.13%	0.014%
29	5.613	1410	1422	1450	rBV	457787	921412	59.22%	6.629%
30	5.902	1505	1512	1514	rBV5	5387	5451	0.35%	0.039%
31	6.002	1539	1543	1545	rBV4	975	709	0.05%	0.005%
32	6.063	1549	1562	1594	rBV	347830	748007	48.08%	5.381%
33	6.568	1718	1719	1722	rBV2	739	531	0.03%	0.004%
34	6.796	1787	1790	1797	rBV4	1000	851	0.05%	0.006%
35	6.841	1803	1804	1806	rBV2	365	155	0.01%	0.001%
36	6.854	1806	1808	1811	rVV	656	324	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028424.D
 Acq On : 07 Oct 2022 22:01
 Operator : SY/MD
 Sample : N4889-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.870	1811	1813	1815	rVB3	425	163	0.01%	0.001%
38	6.912	1823	1826	1829	rBV5	763	607	0.04%	0.004%
39	6.982	1838	1848	1872	rBV	207961	379755	24.41%	2.732%
40	7.310	1939	1950	1963	rBV	722869	1229426	79.02%	8.845%
41	7.384	1965	1973	1993	rVB	307596	537057	34.52%	3.864%
42	7.616	2036	2045	2066	rBV	143393	259289	16.67%	1.865%
43	7.973	2152	2156	2157	rBV3	794	576	0.04%	0.004%
44	8.027	2170	2173	2175	rBV3	690	409	0.03%	0.003%
45	8.085	2178	2191	2224	rBV	467388	923873	59.38%	6.647%
46	8.555	2335	2337	2340	rVB4	628	254	0.02%	0.002%
47	8.635	2359	2362	2367	rVB5	820	683	0.04%	0.005%
48	8.715	2385	2387	2389	rBV3	802	378	0.02%	0.003%
49	8.844	2416	2427	2449	rBV	648481	1067050	68.58%	7.677%
50	9.008	2468	2478	2491	rBV	283000	452952	29.11%	3.259%
51	9.130	2505	2516	2538	rBV	571896	923323	59.34%	6.643%
52	9.542	2636	2644	2659	rVB2	22805	36677	2.36%	0.264%
53	9.651	2674	2678	2680	rBV5	1188	987	0.06%	0.007%
54	9.751	2706	2709	2712	rBV4	544	408	0.03%	0.003%
55	9.789	2716	2721	2722	rBV4	1549	1234	0.08%	0.009%
56	9.866	2742	2745	2750	rVB5	968	747	0.05%	0.005%
57	9.889	2750	2752	2753	rBV	520	153	0.01%	0.001%
58	9.928	2755	2764	2777	rVV	25787	42787	2.75%	0.308%
59	10.056	2802	2804	2806	rBV3	541	217	0.01%	0.002%
60	10.069	2806	2808	2813	rVV4	582	332	0.02%	0.002%
61	10.207	2838	2851	2871	rBV	471506	753972	48.46%	5.424%
62	10.349	2889	2895	2910	rVB	17112	27594	1.77%	0.199%
63	10.911	3064	3070	3080	rVB2	9271	13219	0.85%	0.095%
64	11.018	3097	3103	3109	rBV8	2381	3278	0.21%	0.024%
65	11.140	3139	3141	3143	rBV2	560	281	0.02%	0.002%
66	11.156	3143	3146	3148	rVV3	873	688	0.04%	0.005%
67	11.239	3161	3172	3191	rBV	673161	1053756	67.73%	7.581%
68	11.616	3277	3289	3313	rBV	676339	1082157	69.55%	7.785%
69	11.886	3370	3373	3377	rBV5	721	549	0.04%	0.004%
70	12.014	3406	3413	3430	rVB4	7559	16414	1.05%	0.118%
71	12.111	3430	3443	3450	rBV5	5459	10351	0.67%	0.074%
72	12.175	3461	3463	3465	rVB3	960	424	0.03%	0.003%
73	12.198	3465	3470	3472	rBV5	674	589	0.04%	0.004%
74	12.239	3481	3483	3484	rBV2	556	200	0.01%	0.001%
75	12.310	3495	3505	3514	rBV6	4736	8066	0.52%	0.058%
76	12.345	3514	3516	3518	rBV3	645	301	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028424.D
 Acq On : 07 Oct 2022 22:01
 Operator : SY/MD
 Sample : N4889-03 100X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ61

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.410	3530	3536	3544	rVB5	3236	4586	0.29%	0.033%
78	12.487	3558	3560	3563	rBV3	549	250	0.02%	0.002%
79	12.632	3598	3605	3607	rBV6	824	848	0.05%	0.006%
80	12.673	3612	3618	3619	rBV3	777	883	0.06%	0.006%
81	12.728	3629	3635	3639	rVB6	1172	1185	0.08%	0.009%
82	12.770	3646	3648	3651	rBV3	669	401	0.03%	0.003%
83	12.786	3651	3653	3655	rBV3	721	350	0.02%	0.003%
84	12.873	3673	3680	3690	rVB3	12164	18362	1.18%	0.132%
85	12.915	3691	3693	3698	rVB5	815	579	0.04%	0.004%
86	13.037	3723	3731	3740	rBV8	4578	7500	0.48%	0.054%
87	13.117	3753	3756	3757	rBV2	734	303	0.02%	0.002%
88	13.153	3764	3767	3768	rBV3	564	325	0.02%	0.002%
89	13.320	3815	3819	3822	rBV3	831	734	0.05%	0.005%
90	13.577	3893	3899	3904	rBV5	1287	1665	0.11%	0.012%
91	13.616	3909	3911	3914	rVB4	964	439	0.03%	0.003%
92	13.632	3914	3916	3919	rBV3	912	617	0.04%	0.004%
93	13.776	3959	3961	3965	rVB3	785	398	0.03%	0.003%
94	13.844	3980	3982	3984	rBV3	831	543	0.03%	0.004%
95	13.953	4013	4016	4020	rBV6	832	553	0.04%	0.004%
96	13.989	4025	4027	4029	rBV3	482	274	0.02%	0.002%
97	14.011	4032	4034	4035	rBV2	478	178	0.01%	0.001%
98	14.027	4037	4039	4043	rVV4	833	582	0.04%	0.004%
99	14.059	4046	4049	4055	rVB4	1120	785	0.05%	0.006%
100	14.709	4247	4251	4254	rBV5	1106	973	0.06%	0.007%




Sum of corrected areas: 13899971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028424.D
Acq On : 07 Oct 2022 22:01
Operator : SY/MD
Sample : N4889-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

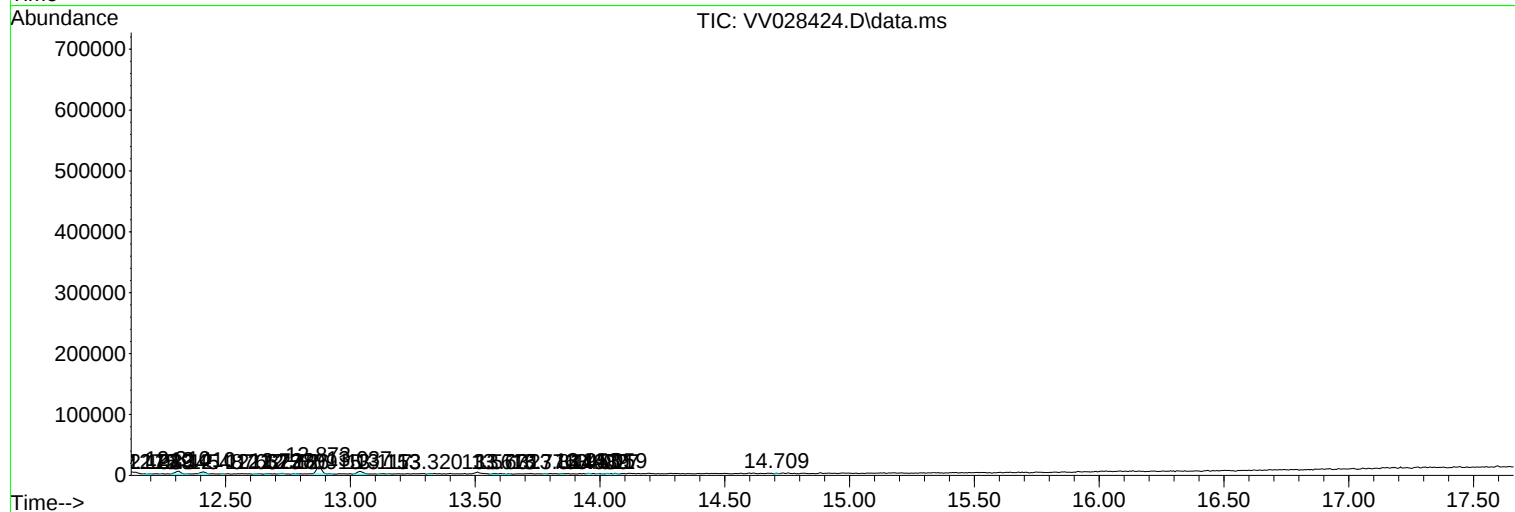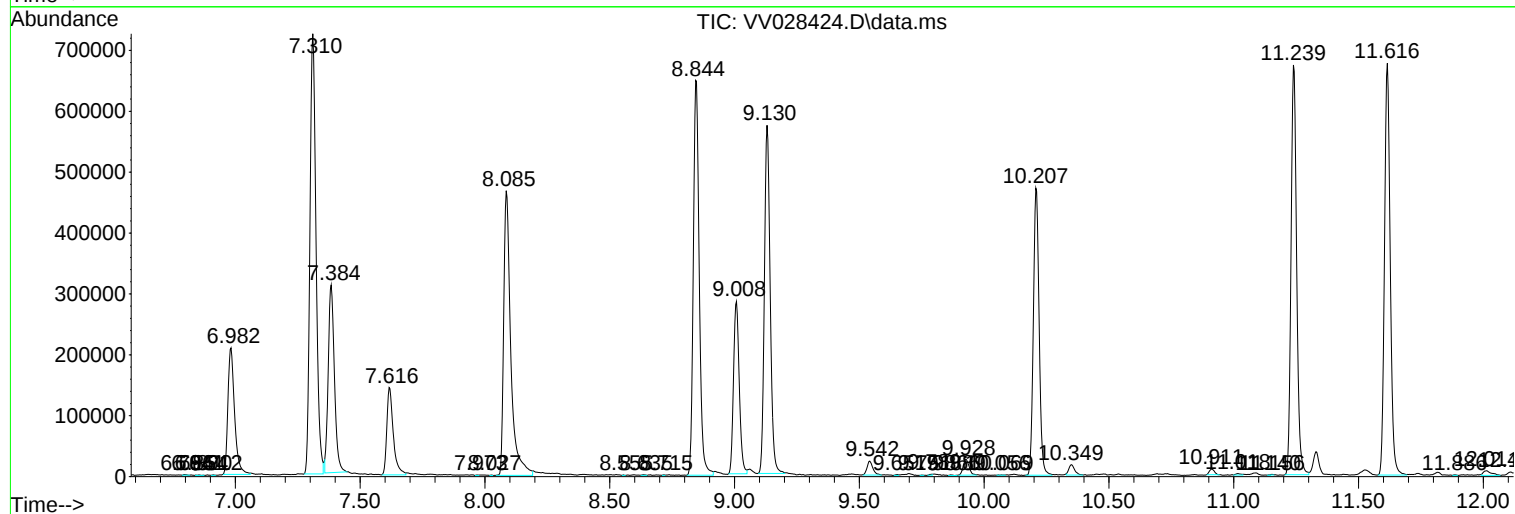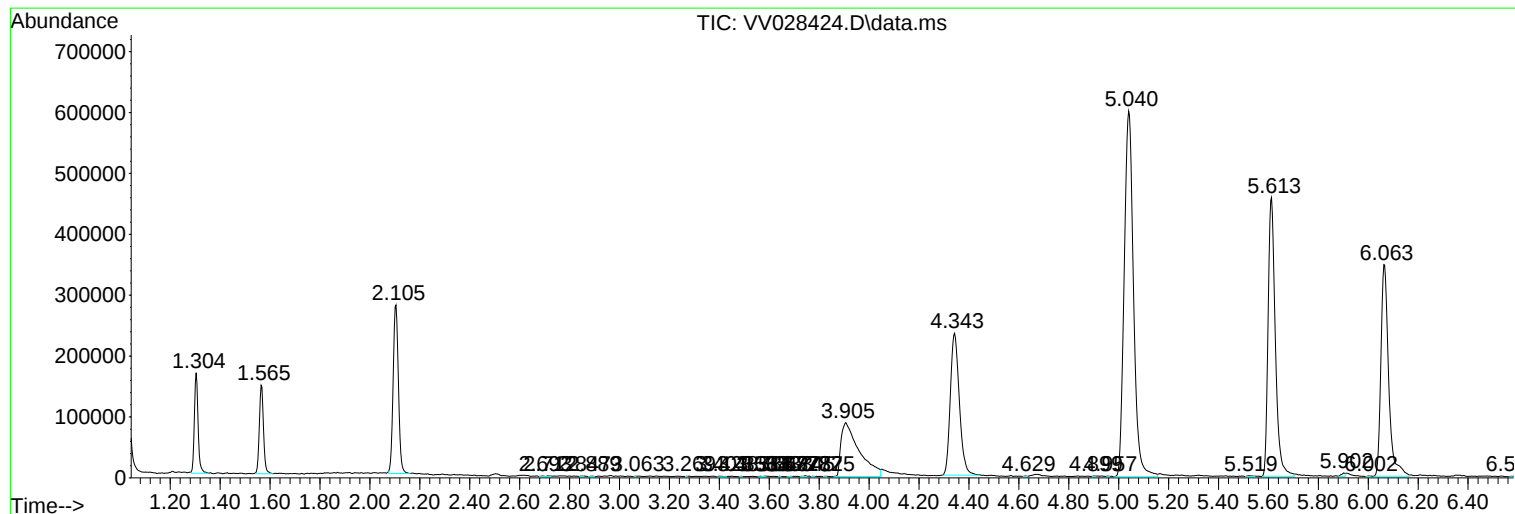

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028424.D
Acq On : 07 Oct 2022 22:01
Operator : SY/MD
Sample : N4889-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028424.D
Acq On : 07 Oct 2022 22:01
Operator : SY/MD
Sample : N4889-03 100X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ61

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------