

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028425.D
 Acq On : 07 Oct 2022 22:25
 Operator : SY/MD
 Sample : N4889-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028425.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	166666	173646	1.64%	0.767%
2	1.565	157	163	175	rVB	148145	169423	1.60%	0.749%
3	2.105	322	331	348	rVB	285359	412631	3.89%	1.824%
4	2.732	523	526	528	rBV4	908	589	0.01%	0.003%
5	3.333	711	713	715	rBV2	582	320	0.00%	0.001%
6	3.375	724	726	729	rVB2	1028	475	0.00%	0.002%
7	3.394	729	732	734	rBV4	804	442	0.00%	0.002%
8	3.426	739	742	744	rBV4	759	409	0.00%	0.002%
9	3.458	750	752	755	rBV4	622	376	0.00%	0.002%
10	3.548	778	780	781	rBV	733	309	0.00%	0.001%
11	3.571	785	787	790	rBV4	624	396	0.00%	0.002%
12	3.667	815	817	822	rBV4	740	680	0.01%	0.003%
13	3.725	831	835	836	rBV3	763	504	0.00%	0.002%
14	3.764	844	847	848	rBV2	592	313	0.00%	0.001%
15	3.902	879	890	939	rBV2	83683	435376	4.11%	1.924%
16	4.343	1013	1027	1053	rVB	232225	581499	5.49%	2.570%
17	4.899	1197	1200	1203	rBV4	494	391	0.00%	0.002%
18	5.040	1228	1244	1277	rVV2	608745	1568794	14.80%	6.933%
19	5.423	1360	1363	1367	rBV5	1252	1041	0.01%	0.005%
20	5.613	1410	1422	1453	rBV	459665	935305	8.82%	4.134%
21	5.905	1503	1513	1524	rBV9	5634	12857	0.12%	0.057%
22	6.066	1550	1563	1593	rBV	348654	727475	6.86%	3.215%
23	6.413	1668	1671	1673	rBV3	885	607	0.01%	0.003%
24	6.445	1678	1681	1684	rBV3	740	470	0.00%	0.002%
25	6.587	1722	1725	1728	rBV3	857	429	0.00%	0.002%
26	6.632	1736	1739	1741	rBV4	711	373	0.00%	0.002%
27	6.648	1741	1744	1745	rBV2	1254	639	0.01%	0.003%
28	6.760	1777	1779	1783	rBV3	738	554	0.01%	0.002%
29	6.931	1826	1832	1836	rBV6	1069	802	0.01%	0.004%
30	6.982	1836	1848	1874	rBV	210098	394739	3.72%	1.745%
31	7.310	1939	1950	1961	rBV	723773	1251792	11.81%	5.532%
32	7.381	1961	1972	1999	rVB	6328940	10599870	100.00%	46.847%
33	7.619	2037	2046	2065	rVB	137707	238625	2.25%	1.055%
34	8.085	2181	2191	2233	rBV	462640	921903	8.70%	4.074%
35	8.847	2417	2428	2451	rBV	648564	1071356	10.11%	4.735%
36	9.011	2470	2479	2498	rVB	48445	81638	0.77%	0.361%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028425.D
 Acq On : 07 Oct 2022 22:25
 Operator : SY/MD
 Sample : N4889-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	9.137	2509	2518	2539	rVB	50988	89809	0.85%	0.397%
38	9.307	2569	2571	2574	rBV3	574	321	0.00%	0.001%
39	9.355	2582	2586	2589	rBV4	1024	658	0.01%	0.003%
40	9.436	2609	2611	2613	rBV2	577	329	0.00%	0.001%
41	9.542	2637	2644	2654	rBV2	8254	13824	0.13%	0.061%
42	9.612	2663	2666	2668	rBV3	1013	655	0.01%	0.003%
43	9.661	2679	2681	2685	rVB4	1346	672	0.01%	0.003%
44	9.683	2685	2688	2694	rVB3	967	889	0.01%	0.004%
45	9.719	2694	2699	2700	rBV2	708	604	0.01%	0.003%
46	9.776	2715	2717	2724	rBV5	425	435	0.00%	0.002%
47	9.809	2724	2727	2728	rBV2	837	459	0.00%	0.002%
48	9.921	2760	2762	2764	rBV3	686	351	0.00%	0.002%
49	10.056	2802	2804	2806	rBV2	697	404	0.00%	0.002%
50	10.130	2825	2827	2831	rBV4	466	367	0.00%	0.002%
51	10.207	2840	2851	2872	rBV	469780	748898	7.07%	3.310%
52	10.445	2923	2925	2927	rVB3	845	398	0.00%	0.002%
53	10.600	2972	2973	2977	rVB3	671	351	0.00%	0.002%
54	10.632	2979	2983	2985	rBV3	502	454	0.00%	0.002%
55	10.683	2997	2999	3003	rBV2	500	416	0.00%	0.002%
56	10.751	3018	3020	3022	rBV3	629	426	0.00%	0.002%
57	10.809	3035	3038	3041	rBV5	432	330	0.00%	0.001%
58	10.857	3048	3053	3055	rBV4	931	606	0.01%	0.003%
59	11.050	3109	3113	3116	rBV4	657	559	0.01%	0.002%
60	11.079	3120	3122	3124	rVV3	718	337	0.00%	0.001%
61	11.140	3138	3141	3143	rBV3	520	426	0.00%	0.002%
62	11.153	3143	3145	3147	rBV3	658	353	0.00%	0.002%
63	11.194	3154	3158	3161	rBV5	802	660	0.01%	0.003%
64	11.239	3161	3172	3194	rBV	666788	1060208	10.00%	4.686%
65	11.413	3223	3226	3231	rVB5	1118	929	0.01%	0.004%
66	11.503	3252	3254	3257	rBV4	678	342	0.00%	0.002%
67	11.616	3273	3289	3310	rBV	687629	1096437	10.34%	4.846%
68	11.815	3348	3351	3352	rBV3	875	489	0.00%	0.002%
69	11.889	3369	3374	3376	rBV3	817	703	0.01%	0.003%
70	11.921	3382	3384	3387	rBV2	756	524	0.00%	0.002%
71	11.973	3395	3400	3401	rBV3	502	364	0.00%	0.002%
72	12.075	3427	3432	3433	rBV4	819	622	0.01%	0.003%
73	12.133	3448	3450	3455	rVB4	984	789	0.01%	0.003%
74	12.162	3455	3459	3461	rBV4	1008	664	0.01%	0.003%
75	12.201	3468	3471	3473	rVB2	905	417	0.00%	0.002%
76	12.223	3476	3478	3483	rVV5	638	570	0.01%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028425.D
 Acq On : 07 Oct 2022 22:25
 Operator : SY/MD
 Sample : N4889-05 200X
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EXZ63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.307	3500	3504	3505	rBV2	434	302	0.00%	0.001%
78	12.381	3524	3527	3529	rBV	811	581	0.01%	0.003%
79	12.493	3561	3562	3565	rBV2	525	288	0.00%	0.001%
80	12.606	3595	3597	3601	rVB4	625	412	0.00%	0.002%
81	12.686	3618	3622	3625	rBV4	853	572	0.01%	0.003%
82	12.744	3635	3640	3643	rBV4	818	743	0.01%	0.003%
83	12.763	3643	3646	3648	rBV2	797	578	0.01%	0.003%
84	12.915	3687	3693	3695	rBV5	1041	646	0.01%	0.003%
85	12.953	3703	3705	3707	rBV2	524	318	0.00%	0.001%
86	13.037	3727	3731	3735	rBV6	810	822	0.01%	0.004%
87	13.101	3747	3751	3752	rBV3	561	332	0.00%	0.001%
88	13.111	3752	3754	3759	rVB5	918	575	0.01%	0.003%
89	13.140	3759	3763	3765	rBV4	923	730	0.01%	0.003%
90	13.162	3768	3770	3775	rVB5	527	339	0.00%	0.001%
91	13.185	3775	3777	3783	rVB6	840	754	0.01%	0.003%
92	13.265	3799	3802	3804	rBV4	818	543	0.01%	0.002%
93	13.558	3891	3893	3896	rBV2	754	400	0.00%	0.002%
94	13.770	3957	3959	3962	rBV3	814	531	0.01%	0.002%
95	13.902	3998	4000	4004	rBV3	695	454	0.00%	0.002%
96	13.921	4004	4006	4011	rBV5	694	633	0.01%	0.003%
97	14.143	4073	4075	4076	rBV	885	361	0.00%	0.002%
98	14.230	4099	4102	4104	rBV4	874	577	0.01%	0.003%
99	14.352	4137	4140	4141	rBV2	1009	476	0.00%	0.002%
100	14.680	4240	4242	4243	rBV2	1034	442	0.00%	0.002%




Sum of corrected areas: 22626506

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028425.D
Acq On : 07 Oct 2022 22:25
Operator : SY/MD
Sample : N4889-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

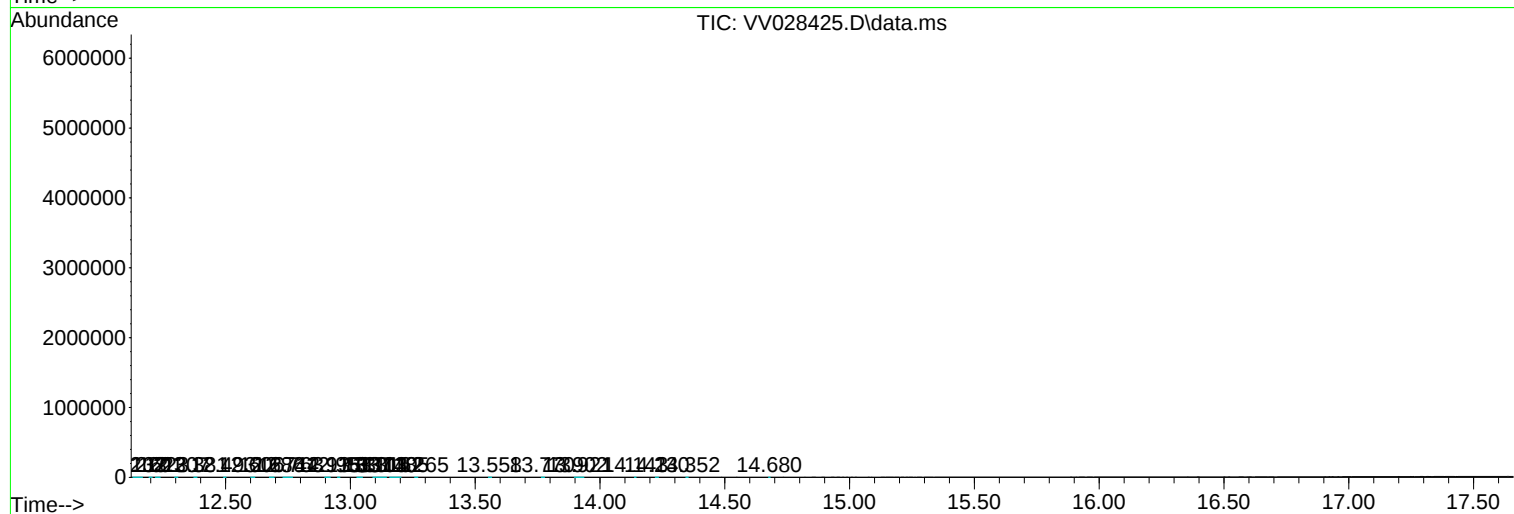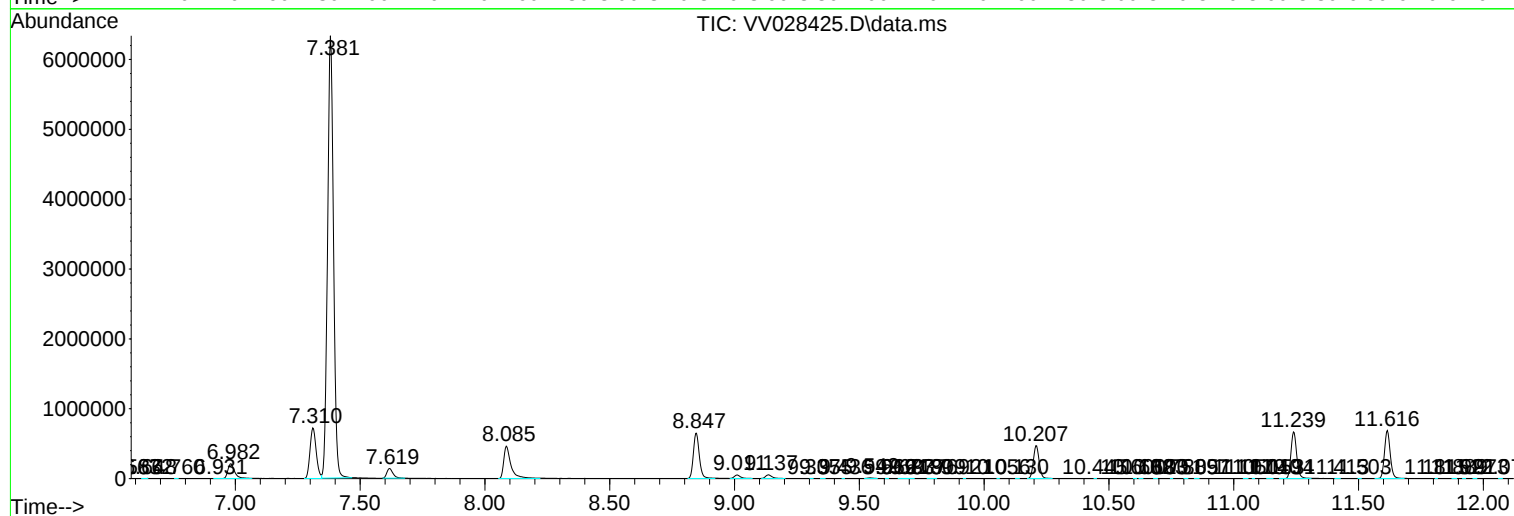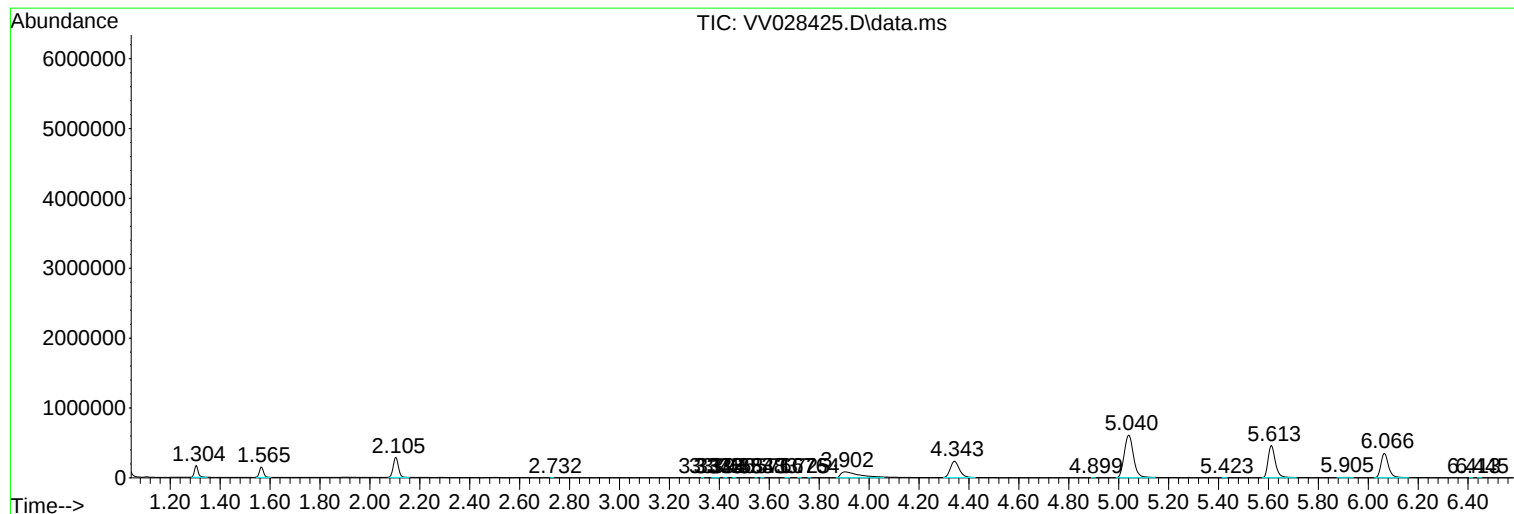

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028425.D
Acq On : 07 Oct 2022 22:25
Operator : SY/MD
Sample : N4889-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028425.D
Acq On : 07 Oct 2022 22:25
Operator : SY/MD
Sample : N4889-05 200X
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 33 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EXZ63

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------