

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028428.D
 Acq On : 08 Oct 2022 00:01
 Operator : SY/MD
 Sample : VV1007WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028428.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	187722	194510	12.08%	1.642%
2	1.564	156	163	178	rVB	158064	181726	11.29%	1.534%
3	2.105	322	331	344	rVB	311328	441109	27.39%	3.723%
4	2.863	565	567	571	rBV5	869	533	0.03%	0.004%
5	3.021	614	616	619	rBV2	683	342	0.02%	0.003%
6	3.243	682	685	686	rBV2	636	354	0.02%	0.003%
7	3.285	695	698	703	rVB3	572	479	0.03%	0.004%
8	3.314	703	707	708	rBV3	696	423	0.03%	0.004%
9	3.355	717	720	721	rBV4	596	348	0.02%	0.003%
10	3.436	739	745	748	rBV5	951	831	0.05%	0.007%
11	3.462	748	753	754	rVV3	477	341	0.02%	0.003%
12	3.770	846	849	852	rBV3	881	532	0.03%	0.004%
13	3.828	864	867	869	rBV3	524	408	0.03%	0.003%
14	3.905	880	891	936	rBV	79613	405135	25.16%	3.419%
15	4.343	1012	1027	1052	rBV	242077	608076	37.76%	5.132%
16	4.584	1097	1102	1104	rBV4	972	733	0.05%	0.006%
17	4.806	1168	1171	1173	rBV3	540	412	0.03%	0.003%
18	4.854	1182	1186	1189	rBV4	552	520	0.03%	0.004%
19	4.905	1200	1202	1204	rBV2	550	276	0.02%	0.002%
20	5.040	1228	1244	1282	rBV2	622024	1610297	100.00%	13.591%
21	5.423	1361	1363	1365	rBV2	900	525	0.03%	0.004%
22	5.613	1410	1422	1450	rBV	427359	878510	54.56%	7.415%
23	6.066	1549	1563	1595	rBV	353450	737325	45.79%	6.223%
24	6.387	1659	1663	1666	rBV5	659	659	0.04%	0.006%
25	6.442	1679	1680	1682	rBV2	708	293	0.02%	0.002%
26	6.455	1682	1684	1688	rVV3	704	497	0.03%	0.004%
27	6.596	1724	1728	1729	rBV3	600	448	0.03%	0.004%
28	6.641	1739	1742	1743	rBV3	704	400	0.02%	0.003%
29	6.796	1788	1790	1793	rBV3	801	506	0.03%	0.004%
30	6.863	1808	1811	1815	rBV5	556	397	0.02%	0.003%
31	6.905	1823	1824	1826	rBV2	670	214	0.01%	0.002%
32	6.982	1836	1848	1872	rBV	210144	391591	24.32%	3.305%
33	7.310	1939	1950	1970	rBV	727793	1286401	79.89%	10.857%
34	7.616	2036	2045	2068	rBV	143979	259380	16.11%	2.189%
35	7.969	2151	2155	2157	rBV2	849	581	0.04%	0.005%
36	8.085	2180	2191	2222	rBV	459563	929080	57.70%	7.841%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028428.D
 Acq On : 08 Oct 2022 00:01
 Operator : SY/MD
 Sample : VV1007WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.645	2361	2365	2366	rBV3	443	304	0.02%	0.003%
38	8.754	2393	2399	2401	rBV4	1123	1156	0.07%	0.010%
39	8.847	2417	2428	2448	rBV	624679	1020493	63.37%	8.613%
40	9.288	2563	2565	2566	rBV2	461	166	0.01%	0.001%
41	9.297	2566	2568	2572	rVV3	581	399	0.02%	0.003%
42	9.323	2574	2576	2578	rBV3	762	343	0.02%	0.003%
43	9.391	2595	2597	2601	rBV4	641	524	0.03%	0.004%
44	9.500	2628	2631	2633	rBV4	552	298	0.02%	0.003%
45	9.526	2633	2639	2641	rBV5	697	601	0.04%	0.005%
46	9.583	2656	2657	2658	rBV	585	146	0.01%	0.001%
47	9.622	2665	2669	2671	rBV5	584	399	0.02%	0.003%
48	9.696	2689	2692	2694	rBV2	655	478	0.03%	0.004%
49	9.799	2722	2724	2728	rVB4	634	266	0.02%	0.002%
50	9.815	2728	2729	2731	rBV2	526	212	0.01%	0.002%
51	9.854	2740	2741	2745	rBV2	422	196	0.01%	0.002%
52	9.873	2745	2747	2753	rVB5	497	429	0.03%	0.004%
53	10.053	2800	2803	2805	rBV4	690	497	0.03%	0.004%
54	10.143	2830	2831	2834	rBV3	698	419	0.03%	0.004%
55	10.165	2836	2838	2839	rVV2	505	198	0.01%	0.002%
56	10.207	2839	2851	2873	rVV	480763	764151	47.45%	6.449%
57	10.448	2924	2926	2931	rVB3	497	336	0.02%	0.003%
58	10.538	2947	2954	2959	rBV6	1077	1607	0.10%	0.014%
59	10.564	2960	2962	2968	rVV5	590	513	0.03%	0.004%
60	10.661	2987	2992	2994	rBV4	1002	629	0.04%	0.005%
61	10.673	2994	2996	2998	rBV2	424	230	0.01%	0.002%
62	10.744	3016	3018	3020	rVB3	570	230	0.01%	0.002%
63	10.799	3032	3035	3038	rVB3	1072	684	0.04%	0.006%
64	10.818	3038	3041	3044	rBV3	513	294	0.02%	0.002%
65	10.847	3044	3050	3052	rBV5	1255	991	0.06%	0.008%
66	10.976	3088	3090	3092	rBV2	432	135	0.01%	0.001%
67	11.046	3107	3112	3113	rBV3	687	479	0.03%	0.004%
68	11.095	3125	3127	3130	rBV3	548	324	0.02%	0.003%
69	11.239	3161	3172	3200	rBV	626000	998751	62.02%	8.429%
70	11.390	3218	3219	3224	rVB4	926	586	0.04%	0.005%
71	11.477	3242	3246	3250	rVB5	878	840	0.05%	0.007%
72	11.506	3250	3255	3258	rBV4	917	948	0.06%	0.008%
73	11.616	3276	3289	3305	rBV	693803	1096493	68.09%	9.254%
74	11.783	3339	3341	3346	rVB5	1004	546	0.03%	0.005%
75	11.860	3363	3365	3369	rBV4	990	511	0.03%	0.004%
76	11.898	3373	3377	3381	rBV5	929	815	0.05%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028428.D
 Acq On : 08 Oct 2022 00:01
 Operator : SY/MD
 Sample : VV1007WBL02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK270

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.918	3381	3383	3385	rVB2	475	174	0.01%	0.001%
78	12.095	3436	3438	3439	rBV2	946	366	0.02%	0.003%
79	12.133	3448	3450	3454	rBV5	731	484	0.03%	0.004%
80	12.178	3462	3464	3466	rBV	473	333	0.02%	0.003%
81	12.288	3495	3498	3502	rBV4	653	676	0.04%	0.006%
82	12.310	3503	3505	3510	rVV4	740	549	0.03%	0.005%
83	12.509	3565	3567	3571	rBV4	540	334	0.02%	0.003%
84	12.548	3577	3579	3587	rVB6	804	609	0.04%	0.005%
85	12.590	3590	3592	3595	rVV4	582	337	0.02%	0.003%
86	12.947	3701	3703	3706	rBV4	648	402	0.02%	0.003%
87	12.982	3712	3714	3715	rBV2	575	231	0.01%	0.002%
88	13.082	3739	3745	3747	rBV4	873	742	0.05%	0.006%
89	13.149	3764	3766	3768	rBV	760	256	0.02%	0.002%
90	13.172	3771	3773	3775	rBV2	452	186	0.01%	0.002%
91	13.194	3778	3780	3784	rBV5	453	239	0.01%	0.002%
92	13.320	3816	3819	3821	rBV3	1136	723	0.04%	0.006%
93	13.332	3821	3823	3828	rVV6	885	797	0.05%	0.007%
94	13.429	3851	3853	3855	rVB2	536	219	0.01%	0.002%
95	13.442	3855	3857	3860	rBV3	578	337	0.02%	0.003%
96	13.477	3866	3868	3869	rBV	776	371	0.02%	0.003%
97	13.500	3871	3875	3889	rVB3	4117	6987	0.43%	0.059%
98	13.725	3943	3945	3946	rBV2	1110	483	0.03%	0.004%
99	13.934	4008	4010	4012	rBV3	710	295	0.02%	0.002%
100	14.146	4074	4076	4078	rBV3	658	363	0.02%	0.003%



Sum of corrected areas: 11848302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028428.D
Acq On : 08 Oct 2022 00:01
Operator : SY/MD
Sample : VV1007WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

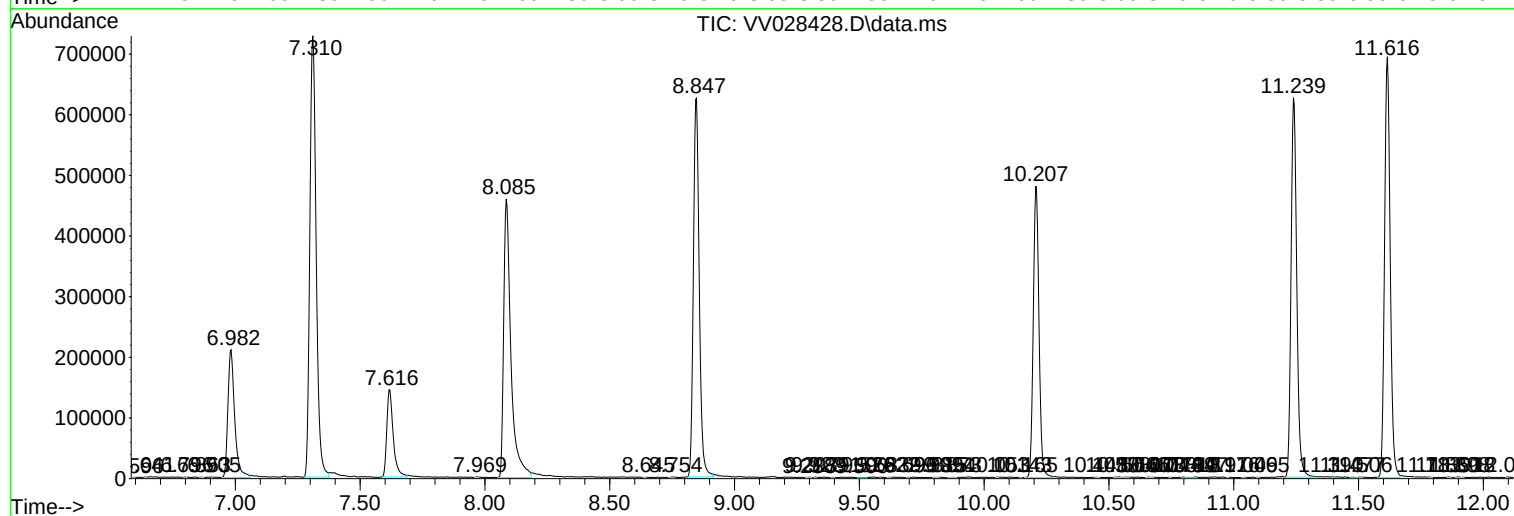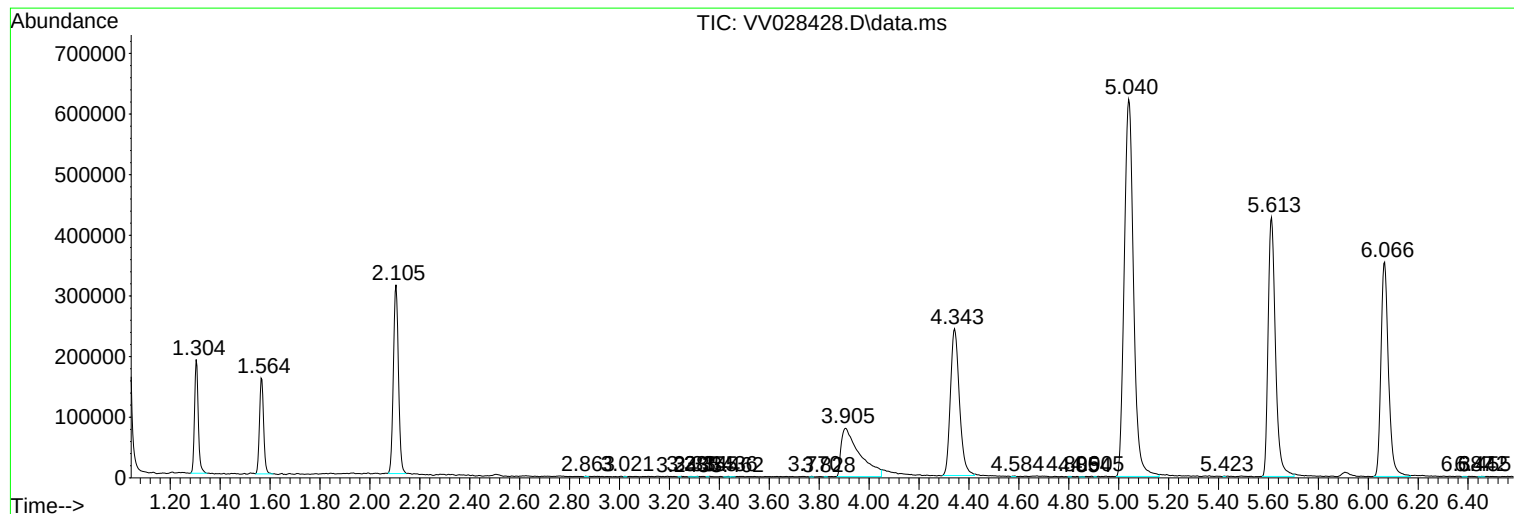

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028428.D
Acq On : 08 Oct 2022 00:01
Operator : SY/MD
Sample : VV1007WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028428.D
Acq On : 08 Oct 2022 00:01
Operator : SY/MD
Sample : VV1007WBL02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK270

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------