

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028429.D
 Acq On : 08 Oct 2022 00:25
 Operator : SY/MD
 Sample : N4942-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028429.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	157179	173033	11.63%	1.531%
2	1.568	157	164	176	rVB	140474	158285	10.64%	1.401%
3	2.105	321	331	344	rBV	266328	380796	25.60%	3.370%
4	2.799	545	547	549	rBV2	649	433	0.03%	0.004%
5	3.236	679	683	686	rBV5	966	654	0.04%	0.006%
6	3.336	712	714	722	rVB5	736	628	0.04%	0.006%
7	3.371	722	725	728	rVB3	778	555	0.04%	0.005%
8	3.391	728	731	734	rBV4	724	638	0.04%	0.006%
9	3.442	745	747	748	rBV	605	324	0.02%	0.003%
10	3.487	759	761	764	rVB3	570	286	0.02%	0.003%
11	3.625	800	804	805	rBV3	952	615	0.04%	0.005%
12	3.648	809	811	815	rVB4	823	416	0.03%	0.004%
13	3.667	815	817	819	rVB3	859	360	0.02%	0.003%
14	3.683	819	822	824	rBV2	631	371	0.02%	0.003%
15	3.728	832	836	840	rBV5	801	803	0.05%	0.007%
16	3.905	880	891	931	rBV	70881	324245	21.80%	2.869%
17	4.342	1013	1027	1052	rBV	223961	566550	38.09%	5.014%
18	4.719	1142	1144	1147	rBV3	1071	651	0.04%	0.006%
19	4.780	1159	1163	1165	rBV5	588	335	0.02%	0.003%
20	4.863	1188	1189	1194	rBV4	536	281	0.02%	0.002%
21	4.889	1194	1197	1199	rVB3	1039	543	0.04%	0.005%
22	4.902	1199	1201	1202	rBV2	497	266	0.02%	0.002%
23	5.040	1228	1244	1296	rBV2	569713	1487504	100.00%	13.163%
24	5.301	1322	1325	1328	rVB4	1001	564	0.04%	0.005%
25	5.333	1333	1335	1338	rBV4	941	579	0.04%	0.005%
26	5.613	1410	1422	1448	rBV	446207	905374	60.87%	8.012%
27	5.876	1501	1504	1505	rBV3	889	422	0.03%	0.004%
28	5.989	1536	1539	1540	rBV3	895	602	0.04%	0.005%
29	6.066	1549	1563	1591	rBV	328803	682486	45.88%	6.039%
30	6.429	1674	1676	1677	rBV	702	256	0.02%	0.002%
31	6.487	1691	1694	1699	rBV8	607	519	0.03%	0.005%
32	6.519	1702	1704	1707	rVB2	720	409	0.03%	0.004%
33	6.587	1723	1725	1729	rBV4	611	346	0.02%	0.003%
34	6.651	1738	1745	1748	rBV5	1209	1448	0.10%	0.013%
35	6.680	1752	1754	1756	rVB	1516	572	0.04%	0.005%
36	6.834	1799	1802	1804	rBV3	844	535	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028429.D
 Acq On : 08 Oct 2022 00:25
 Operator : SY/MD
 Sample : N4942-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.870	1809	1813	1814	rBV3	947	467	0.03%	0.004%
38	6.915	1819	1827	1829	rBV5	983	919	0.06%	0.008%
39	6.982	1836	1848	1880	rBV	200765	376744	25.33%	3.334%
40	7.310	1939	1950	1972	rBV	666313	1172589	78.83%	10.376%
41	7.558	2025	2027	2029	rBV3	821	537	0.04%	0.005%
42	7.616	2036	2045	2070	rBV2	134452	247124	16.61%	2.187%
43	7.973	2148	2156	2173	rVB4	20120	37379	2.51%	0.331%
44	8.047	2173	2179	2180	rBV3	754	594	0.04%	0.005%
45	8.085	2182	2191	2227	rBV	411394	840225	56.49%	7.435%
46	8.513	2322	2324	2327	rBV4	823	601	0.04%	0.005%
47	8.767	2401	2403	2407	rBV3	363	269	0.02%	0.002%
48	8.844	2417	2427	2456	rVV	642924	1067764	71.78%	9.449%
49	9.143	2515	2520	2521	rBV5	1392	1082	0.07%	0.010%
50	9.304	2568	2570	2573	rVB4	583	333	0.02%	0.003%
51	9.391	2591	2597	2599	rBV5	812	559	0.04%	0.005%
52	9.538	2639	2643	2645	rBV4	921	678	0.05%	0.006%
53	9.648	2675	2677	2681	rVV5	994	699	0.05%	0.006%
54	9.680	2685	2687	2689	rBV2	816	423	0.03%	0.004%
55	9.715	2695	2698	2700	rBV4	622	408	0.03%	0.004%
56	9.780	2714	2718	2721	rBV5	656	484	0.03%	0.004%
57	9.805	2721	2726	2727	rBV3	1162	1009	0.07%	0.009%
58	9.905	2754	2757	2759	rBV2	315	268	0.02%	0.002%
59	9.921	2759	2762	2763	rBV2	448	260	0.02%	0.002%
60	9.947	2768	2770	2774	rBV4	596	469	0.03%	0.004%
61	10.024	2792	2794	2796	rBV2	569	340	0.02%	0.003%
62	10.104	2813	2819	2823	rBV7	762	735	0.05%	0.007%
63	10.140	2828	2830	2832	rBV	796	416	0.03%	0.004%
64	10.207	2839	2851	2877	rBV	455967	726813	48.86%	6.432%
65	10.342	2891	2893	2896	rBV4	918	584	0.04%	0.005%
66	10.474	2931	2934	2936	rBV4	792	465	0.03%	0.004%
67	10.689	2997	3001	3004	rBV6	667	539	0.04%	0.005%
68	10.715	3004	3009	3011	rVB5	890	522	0.04%	0.005%
69	10.757	3019	3022	3027	rBV6	726	693	0.05%	0.006%
70	10.802	3033	3036	3039	rBV5	624	534	0.04%	0.005%
71	10.966	3084	3087	3089	rBV	574	386	0.03%	0.003%
72	10.998	3093	3097	3098	rBV3	684	347	0.02%	0.003%
73	11.050	3111	3113	3115	rBV3	649	313	0.02%	0.003%
74	11.082	3120	3123	3128	rBV4	1542	1153	0.08%	0.010%
75	11.149	3134	3144	3153	rBV7	7055	12850	0.86%	0.114%
76	11.239	3161	3172	3202	rBV	657794	1038439	69.81%	9.189%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028429.D
 Acq On : 08 Oct 2022 00:25
 Operator : SY/MD
 Sample : N4942-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.525	3259	3261	3266	rBV4	1162	1326	0.09%	0.012%
78	11.615	3278	3289	3311	rBV	652955	1031040	69.31%	9.124%
79	11.783	3337	3341	3342	rBV4	775	488	0.03%	0.004%
80	11.876	3367	3370	3372	rBV3	865	403	0.03%	0.004%
81	11.921	3382	3384	3387	rVB3	643	362	0.02%	0.003%
82	11.960	3392	3396	3397	rBV4	1056	765	0.05%	0.007%
83	12.149	3451	3455	3458	rBV4	865	698	0.05%	0.006%
84	12.230	3476	3480	3482	rBV3	947	746	0.05%	0.007%
85	12.342	3507	3515	3531	rVB5	13309	22307	1.50%	0.197%
86	12.734	3634	3637	3639	rBV4	457	360	0.02%	0.003%
87	12.802	3655	3658	3659	rBV3	697	416	0.03%	0.004%
88	12.850	3670	3673	3678	rBV3	1035	808	0.05%	0.007%
89	12.873	3678	3680	3682	rBV3	659	374	0.03%	0.003%
90	12.988	3714	3716	3718	rBV3	861	319	0.02%	0.003%
91	13.072	3738	3742	3747	rBV4	828	670	0.05%	0.006%
92	13.095	3747	3749	3753	rVB3	895	515	0.03%	0.005%
93	13.114	3753	3755	3757	rBV2	573	374	0.03%	0.003%
94	13.429	3851	3853	3856	rBV3	653	509	0.03%	0.005%
95	13.596	3903	3905	3908	rBV2	664	391	0.03%	0.003%
96	13.660	3923	3925	3927	rVB3	798	307	0.02%	0.003%
97	13.686	3927	3933	3936	rBV5	1024	1181	0.08%	0.010%
98	13.738	3943	3949	3960	rVB10	2483	4382	0.29%	0.039%
99	13.953	4014	4016	4022	rVB4	1113	798	0.05%	0.007%
100	14.175	4081	4085	4089	rBV7	1258	1245	0.08%	0.011%




Sum of corrected areas: 11300481

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028429.D
Acq On : 08 Oct 2022 00:25
Operator : SY/MD
Sample : N4942-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

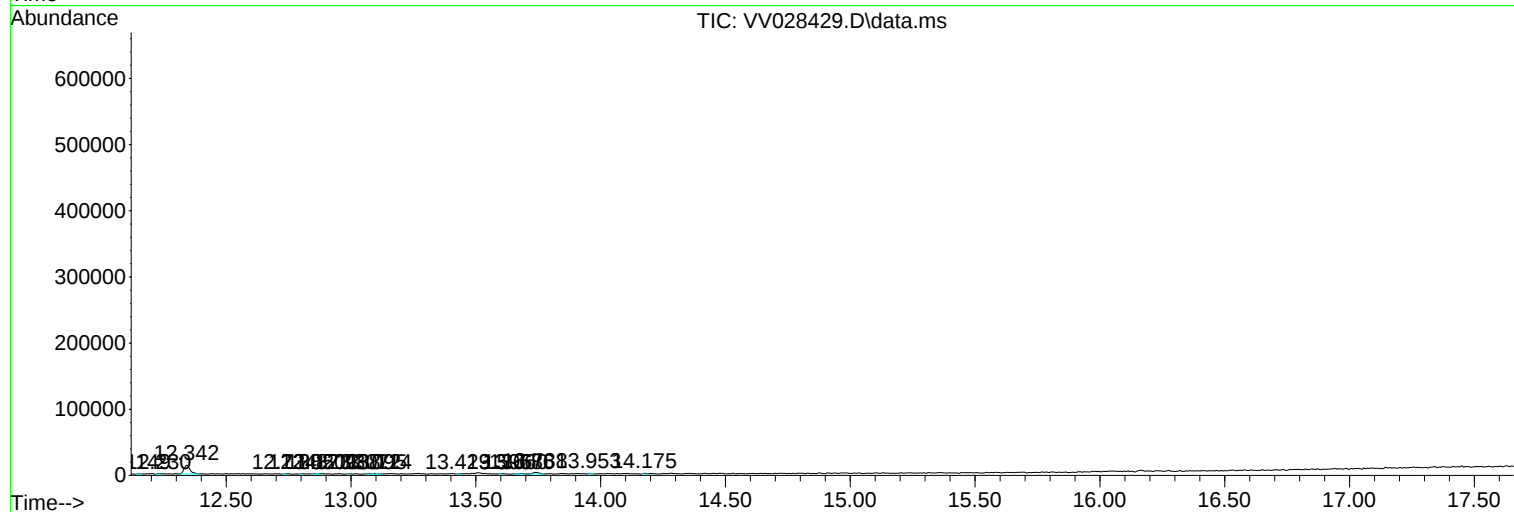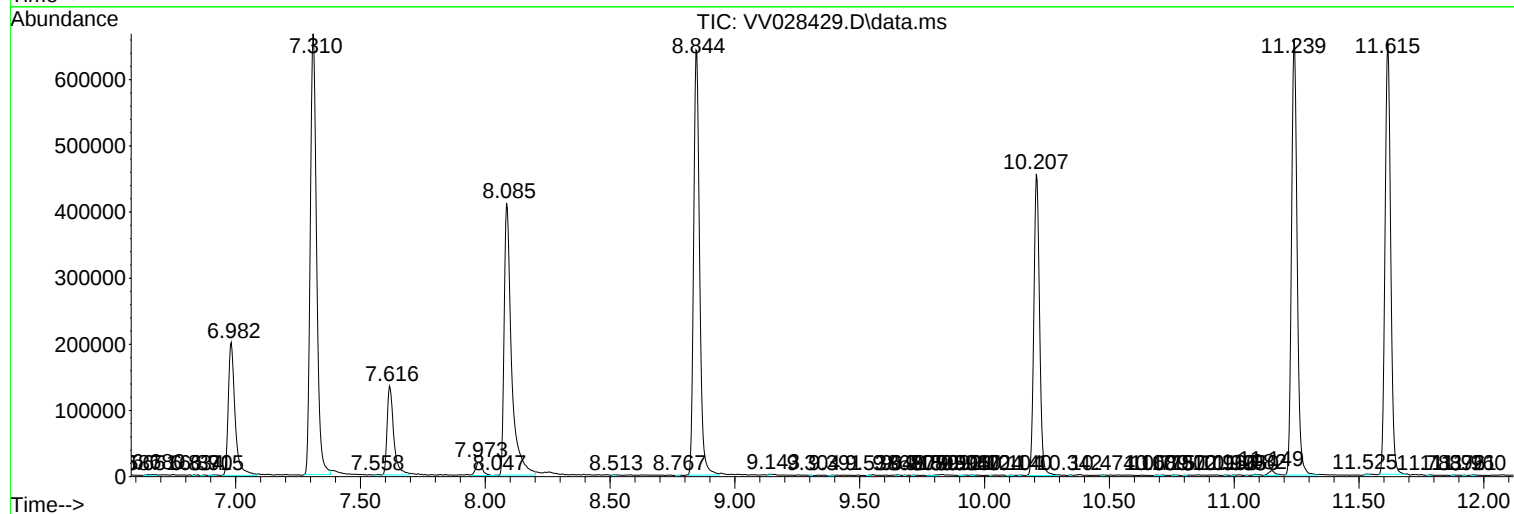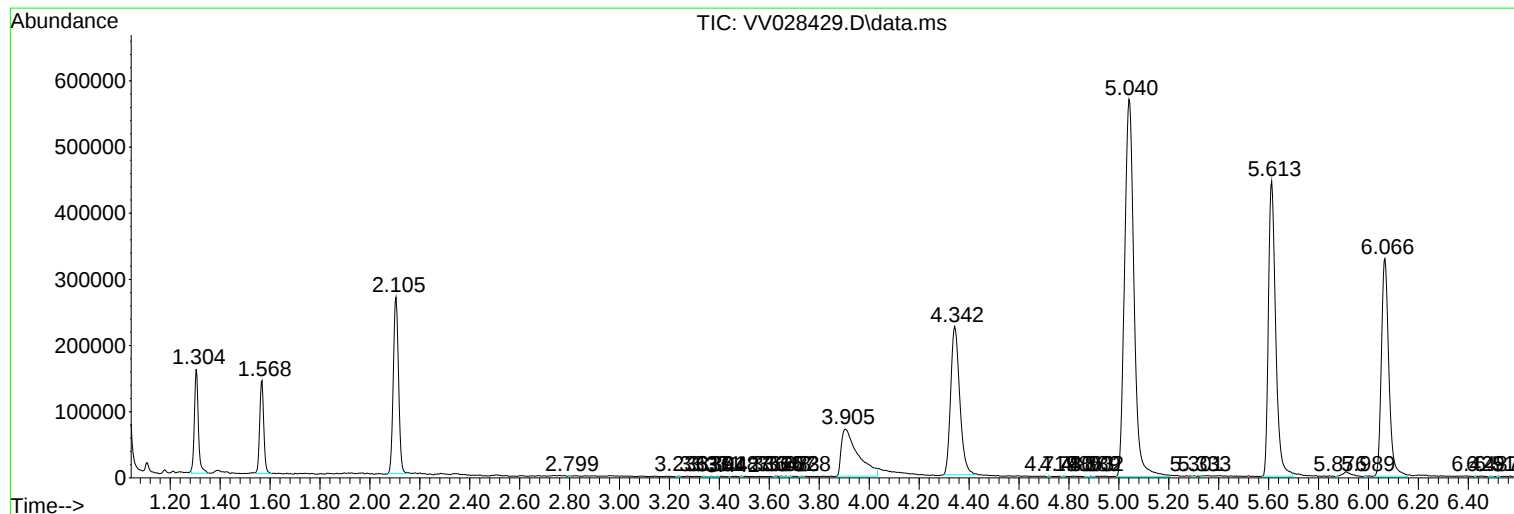

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028429.D
Acq On : 08 Oct 2022 00:25
Operator : SY/MD
Sample : N4942-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028429.D
Acq On : 08 Oct 2022 00:25
Operator : SY/MD
Sample : N4942-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 38 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc