

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028430.D
 Acq On : 08 Oct 2022 00:49
 Operator : SY/MD
 Sample : N4942-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028430.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	154832	162625	10.89%	1.408%
2	1.564	157	163	177	rVB	138129	159706	10.70%	1.383%
3	2.105	322	331	347	rVB	267253	382616	25.63%	3.313%
4	2.838	555	559	562	rVB4	997	737	0.05%	0.006%
5	2.931	585	588	589	rBV3	714	364	0.02%	0.003%
6	3.153	655	657	660	rBV3	456	355	0.02%	0.003%
7	3.452	746	750	751	rBV3	680	424	0.03%	0.004%
8	3.728	834	836	839	rVB2	738	323	0.02%	0.003%
9	3.751	839	843	845	rBV4	629	484	0.03%	0.004%
10	3.844	870	872	877	rVB4	613	502	0.03%	0.004%
11	3.908	877	892	935	rBV2	66862	346944	23.24%	3.004%
12	4.342	1014	1027	1051	rVB	226983	563762	37.76%	4.881%
13	4.619	1109	1113	1118	rBV4	1494	1545	0.10%	0.013%
14	4.793	1164	1167	1168	rBV3	665	360	0.02%	0.003%
15	4.982	1223	1226	1228	rBV2	583	423	0.03%	0.004%
16	5.040	1228	1244	1273	rBV3	581613	1492839	100.00%	12.926%
17	5.387	1350	1352	1355	rBV4	724	331	0.02%	0.003%
18	5.613	1406	1422	1447	rBV	449378	923383	61.85%	7.995%
19	6.002	1540	1543	1546	rBV3	1222	819	0.05%	0.007%
20	6.063	1546	1562	1590	rVV	336260	698640	46.80%	6.049%
21	6.346	1646	1650	1653	rVB5	726	530	0.04%	0.005%
22	6.551	1709	1714	1716	rBV3	686	646	0.04%	0.006%
23	6.622	1732	1736	1738	rBV4	834	608	0.04%	0.005%
24	6.767	1777	1781	1783	rBV2	575	355	0.02%	0.003%
25	6.783	1784	1786	1790	rVV4	659	334	0.02%	0.003%
26	6.931	1828	1832	1834	rBV5	597	351	0.02%	0.003%
27	6.982	1837	1848	1872	rBV	197989	374626	25.09%	3.244%
28	7.178	1906	1909	1911	rBV5	621	343	0.02%	0.003%
29	7.310	1938	1950	1972	rBV	676134	1185849	79.44%	10.268%
30	7.619	2036	2046	2075	rBV	138026	246205	16.49%	2.132%
31	7.921	2136	2140	2141	rBV3	1144	837	0.06%	0.007%
32	7.973	2146	2156	2175	rVB2	123534	213949	14.33%	1.852%
33	8.085	2182	2191	2228	rBV	413586	851165	57.02%	7.370%
34	8.506	2320	2322	2324	rBV4	597	321	0.02%	0.003%
35	8.564	2338	2340	2345	rVB4	703	481	0.03%	0.004%
36	8.587	2345	2347	2350	rBV4	690	313	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028430.D
 Acq On : 08 Oct 2022 00:49
 Operator : SY/MD
 Sample : N4942-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.722	2379	2389	2391	rBV8	753	1100	0.07%	0.010%
38	8.847	2416	2428	2445	rBV	639058	1060516	71.04%	9.182%
39	9.037	2484	2487	2490	rVB4	1259	759	0.05%	0.007%
40	9.194	2534	2536	2538	rBV3	651	350	0.02%	0.003%
41	9.226	2543	2546	2547	rBV3	695	521	0.03%	0.005%
42	9.268	2557	2559	2562	rVB2	724	392	0.03%	0.003%
43	9.487	2624	2627	2629	rBV4	848	523	0.04%	0.005%
44	9.526	2636	2639	2642	rBV5	633	413	0.03%	0.004%
45	9.577	2652	2655	2658	rBV5	700	623	0.04%	0.005%
46	9.673	2682	2685	2689	rVB3	903	648	0.04%	0.006%
47	9.696	2689	2692	2696	rBV5	891	690	0.05%	0.006%
48	9.735	2701	2704	2708	rBV4	859	582	0.04%	0.005%
49	9.821	2726	2731	2735	rBV5	1639	1828	0.12%	0.016%
50	9.860	2739	2743	2748	rVB6	941	908	0.06%	0.008%
51	9.905	2755	2757	2759	rBV	562	346	0.02%	0.003%
52	9.963	2771	2775	2778	rBV5	747	523	0.04%	0.005%
53	10.001	2785	2787	2792	rVB5	604	374	0.03%	0.003%
54	10.207	2840	2851	2878	rVV	452792	725466	48.60%	6.281%
55	10.304	2878	2881	2882	rBV2	749	411	0.03%	0.004%
56	10.378	2899	2904	2910	rVB6	2544	3096	0.21%	0.027%
57	10.448	2921	2926	2929	rBV4	626	554	0.04%	0.005%
58	10.635	2981	2984	2989	rBV4	538	467	0.03%	0.004%
59	10.780	3027	3029	3031	rVB2	731	314	0.02%	0.003%
60	10.825	3039	3043	3045	rBV4	869	587	0.04%	0.005%
61	10.844	3045	3049	3052	rBV6	881	688	0.05%	0.006%
62	10.924	3072	3074	3077	rVB3	1027	444	0.03%	0.004%
63	10.979	3087	3091	3095	rVV5	745	762	0.05%	0.007%
64	11.024	3103	3105	3110	rBV3	798	656	0.04%	0.006%
65	11.050	3111	3113	3115	rVB3	778	352	0.02%	0.003%
66	11.091	3124	3126	3134	rVB5	1268	1015	0.07%	0.009%
67	11.149	3134	3144	3154	rBV8	7561	14304	0.96%	0.124%
68	11.239	3161	3172	3201	rVB	658085	1041219	69.75%	9.015%
69	11.339	3201	3203	3204	rBV2	999	382	0.03%	0.003%
70	11.532	3258	3263	3271	rBV8	2960	4993	0.33%	0.043%
71	11.615	3278	3289	3310	rBV	650995	1033020	69.20%	8.944%
72	11.828	3352	3355	3357	rBV3	963	672	0.05%	0.006%
73	12.030	3415	3418	3421	rBV3	884	573	0.04%	0.005%
74	12.095	3436	3438	3442	rBV3	696	550	0.04%	0.005%
75	12.133	3447	3450	3451	rBV2	792	412	0.03%	0.004%
76	12.146	3451	3454	3457	rVB3	861	645	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028430.D
 Acq On : 08 Oct 2022 00:49
 Operator : SY/MD
 Sample : N4942-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.197	3468	3470	3475	rVB6	1080	558	0.04%	0.005%
78	12.294	3497	3500	3502	rBV	588	385	0.03%	0.003%
79	12.342	3506	3515	3525	rBV6	10718	18662	1.25%	0.162%
80	12.400	3531	3533	3540	rVB3	955	694	0.05%	0.006%
81	12.448	3545	3548	3552	rBV6	766	734	0.05%	0.006%
82	12.638	3603	3607	3612	rBV7	1315	1386	0.09%	0.012%
83	12.889	3684	3685	3688	rVB3	866	452	0.03%	0.004%
84	12.959	3705	3707	3714	rVB6	791	749	0.05%	0.006%
85	12.988	3714	3716	3719	rVB3	813	334	0.02%	0.003%
86	13.120	3753	3757	3758	rBV4	645	512	0.03%	0.004%
87	13.188	3775	3778	3780	rBV2	945	708	0.05%	0.006%
88	13.223	3786	3789	3795	rBV4	713	584	0.04%	0.005%
89	13.307	3813	3815	3820	rVB4	530	335	0.02%	0.003%
90	13.345	3824	3827	3829	rBV4	565	368	0.02%	0.003%
91	13.397	3841	3843	3846	rVB3	875	559	0.04%	0.005%
92	13.419	3846	3850	3854	rBV5	984	894	0.06%	0.008%
93	13.500	3870	3875	3877	rBV3	1109	1013	0.07%	0.009%
94	13.561	3893	3894	3897	rBV2	700	337	0.02%	0.003%
95	13.644	3913	3920	3922	rBV4	1087	1161	0.08%	0.010%
96	13.908	4000	4002	4004	rBV2	547	338	0.02%	0.003%
97	14.210	4094	4096	4098	rBV3	804	458	0.03%	0.004%
98	14.242	4104	4106	4109	rBV4	738	436	0.03%	0.004%
99	14.313	4125	4128	4129	rBV2	764	416	0.03%	0.004%
100	14.975	4331	4334	4336	rBV3	880	546	0.04%	0.005%




Sum of corrected areas: 11549392

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028430.D
Acq On : 08 Oct 2022 00:49
Operator : SY/MD
Sample : N4942-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

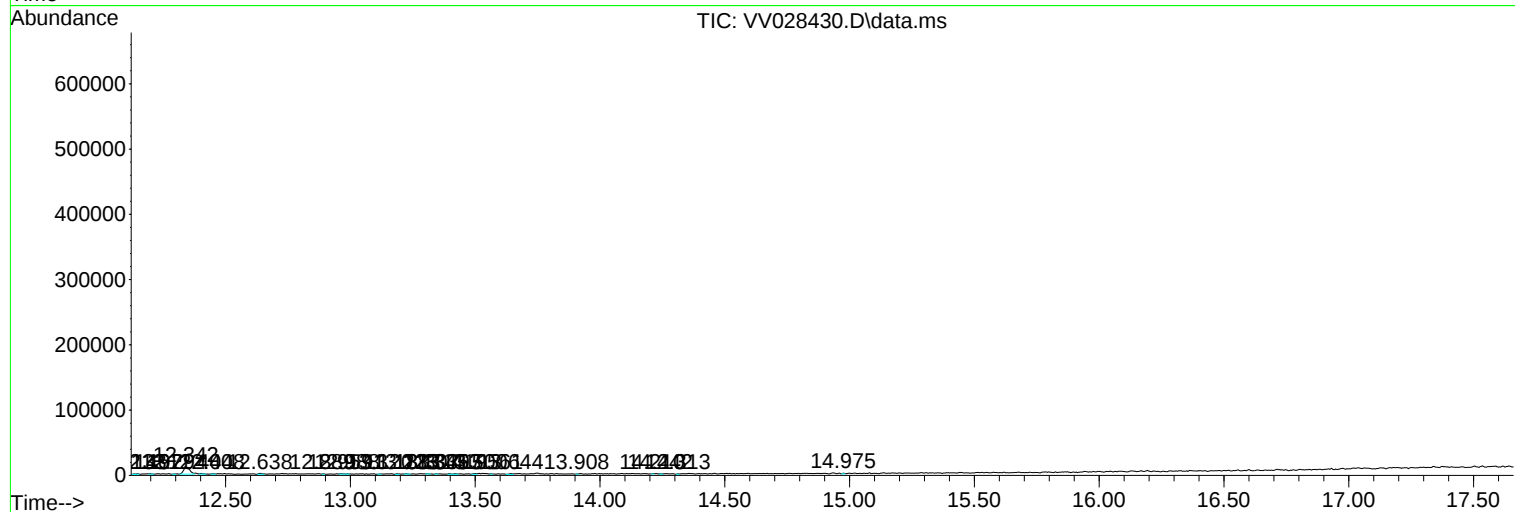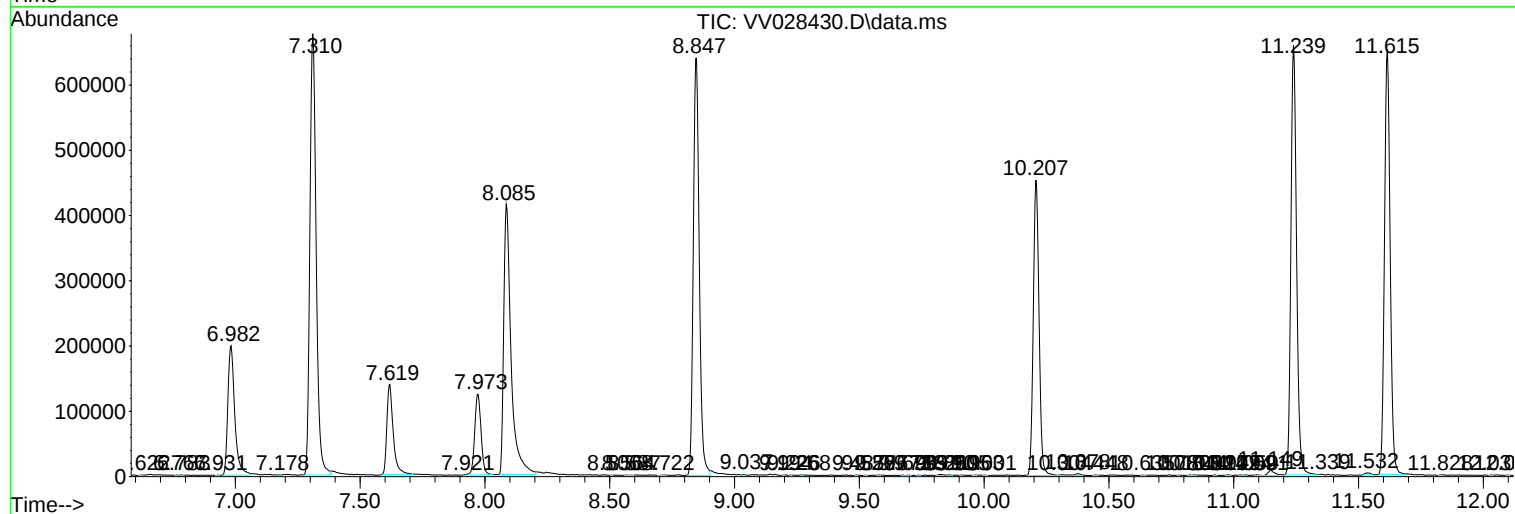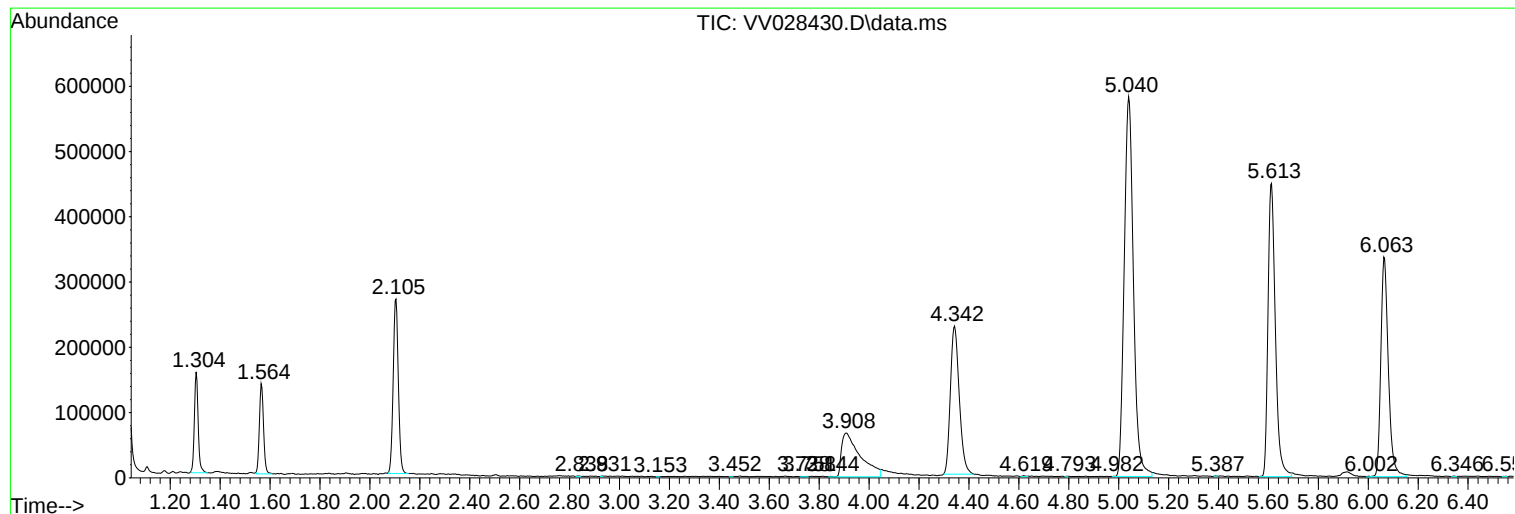

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028430.D
Acq On : 08 Oct 2022 00:49
Operator : SY/MD
Sample : N4942-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028430.D
Acq On : 08 Oct 2022 00:49
Operator : SY/MD
Sample : N4942-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc