

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028431.D
 Acq On : 08 Oct 2022 01:13
 Operator : SY/MD
 Sample : N4942-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M

Title : VOC Analysis

Signal : TIC: VV028431.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	33	rVB	21846	21535	1.49%	0.192%
2	1.304	76	82	95	rVB	155423	163006	11.29%	1.451%
3	1.564	157	163	175	rVB	132419	153111	10.61%	1.362%
4	2.105	322	331	348	rVB	258803	370982	25.70%	3.301%
5	2.818	551	553	556	rVB3	785	410	0.03%	0.004%
6	3.066	628	630	631	rBV	861	383	0.03%	0.003%
7	3.201	669	672	673	rBV2	699	357	0.02%	0.003%
8	3.230	678	681	683	rBV2	620	330	0.02%	0.003%
9	3.314	705	707	713	rVB4	608	514	0.04%	0.005%
10	3.387	727	730	736	rBV7	773	703	0.05%	0.006%
11	3.420	738	740	744	rBV4	551	327	0.02%	0.003%
12	3.455	749	751	754	rVB2	659	352	0.02%	0.003%
13	3.603	795	797	800	rBV2	599	360	0.02%	0.003%
14	3.629	803	805	808	rVB4	896	465	0.03%	0.004%
15	3.693	823	825	829	rVB3	665	330	0.02%	0.003%
16	3.908	880	892	941	rBV2	62448	345337	23.92%	3.073%
17	4.342	1014	1027	1061	rVB	217535	550981	38.17%	4.903%
18	4.567	1091	1097	1099	rBV7	1042	1071	0.07%	0.010%
19	4.661	1119	1126	1130	rBV8	1093	1416	0.10%	0.013%
20	4.796	1166	1168	1172	rVB3	536	406	0.03%	0.004%
21	4.931	1204	1210	1211	rBV3	662	530	0.04%	0.005%
22	4.963	1217	1220	1227	rVB5	900	711	0.05%	0.006%
23	5.040	1227	1244	1283	rBV2	557193	1443576	100.00%	12.846%
24	5.362	1341	1344	1347	rBV3	1058	787	0.05%	0.007%
25	5.487	1378	1383	1387	rBV7	735	838	0.06%	0.007%
26	5.612	1410	1422	1456	rBV	435806	889001	61.58%	7.911%
27	6.066	1545	1563	1591	rBV	318384	671412	46.51%	5.975%
28	6.297	1633	1635	1639	rBV4	719	482	0.03%	0.004%
29	6.375	1656	1659	1662	rBV3	625	440	0.03%	0.004%
30	6.455	1680	1684	1686	rBV4	1287	827	0.06%	0.007%
31	6.481	1689	1692	1697	rBV3	685	486	0.03%	0.004%
32	6.503	1697	1699	1706	rBV4	802	743	0.05%	0.007%
33	6.532	1706	1708	1713	rVB6	859	523	0.04%	0.005%
34	6.587	1722	1725	1726	rBV3	835	381	0.03%	0.003%
35	6.638	1738	1741	1743	rBV3	1020	531	0.04%	0.005%
36	6.664	1744	1749	1750	rBV3	1180	827	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028431.D
 Acq On : 08 Oct 2022 01:13
 Operator : SY/MD
 Sample : N4942-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	6.821	1792	1798	1803	rVV7	816	977	0.07%	0.009%
38	6.876	1811	1815	1818	rBV3	966	702	0.05%	0.006%
39	6.982	1837	1848	1870	rBV	189876	356289	24.68%	3.170%
40	7.310	1938	1950	1974	rBV	651221	1148128	79.53%	10.217%
41	7.616	2035	2045	2069	rBV	130122	238373	16.51%	2.121%
42	7.969	2138	2155	2172	rBV	142723	254194	17.61%	2.262%
43	8.085	2182	2191	2232	rBV	402971	818020	56.67%	7.279%
44	8.683	2374	2377	2382	rBV6	682	723	0.05%	0.006%
45	8.847	2415	2428	2447	rBV	625971	1037895	71.90%	9.236%
46	9.130	2515	2516	2518	rBV	733	342	0.02%	0.003%
47	9.214	2537	2542	2545	rVB4	1258	1162	0.08%	0.010%
48	9.288	2561	2565	2567	rBV4	920	599	0.04%	0.005%
49	9.326	2573	2577	2581	rBV6	452	350	0.02%	0.003%
50	9.362	2583	2588	2589	rBV2	789	599	0.04%	0.005%
51	9.455	2614	2617	2618	rBV2	1170	507	0.04%	0.005%
52	9.529	2636	2640	2642	rBV2	854	635	0.04%	0.006%
53	9.567	2650	2652	2654	rVB3	945	346	0.02%	0.003%
54	9.625	2667	2670	2672	rBV3	999	471	0.03%	0.004%
55	9.735	2700	2704	2705	rBV2	853	592	0.04%	0.005%
56	9.796	2716	2723	2724	rBV5	607	608	0.04%	0.005%
57	9.831	2728	2734	2737	rBV5	1036	1169	0.08%	0.010%
58	9.895	2752	2754	2758	rVB3	744	444	0.03%	0.004%
59	9.953	2769	2772	2778	rBV5	809	691	0.05%	0.006%
60	9.992	2781	2784	2789	rVB3	812	521	0.04%	0.005%
61	10.027	2794	2795	2798	rBV2	585	395	0.03%	0.004%
62	10.207	2839	2851	2870	rBV	436551	701419	48.59%	6.242%
63	10.445	2922	2925	2932	rBV6	752	860	0.06%	0.008%
64	10.500	2938	2942	2943	rBV3	758	601	0.04%	0.005%
65	10.654	2986	2990	2992	rVB4	1093	867	0.06%	0.008%
66	10.677	2992	2997	3004	rVB6	621	751	0.05%	0.007%
67	10.776	3024	3028	3032	rBV6	582	643	0.04%	0.006%
68	11.069	3113	3119	3121	rBV3	463	467	0.03%	0.004%
69	11.091	3121	3126	3130	rBV6	1069	1198	0.08%	0.011%
70	11.156	3139	3146	3154	rBV8	2244	3720	0.26%	0.033%
71	11.239	3161	3172	3197	rBV	644814	1002146	69.42%	8.918%
72	11.397	3217	3221	3226	rBV7	1033	1078	0.07%	0.010%
73	11.464	3239	3242	3245	rVB4	851	645	0.04%	0.006%
74	11.493	3245	3251	3254	rBV5	795	873	0.06%	0.008%
75	11.535	3254	3264	3277	rBV8	5063	12097	0.84%	0.108%
76	11.615	3277	3289	3309	rVV	625724	1001017	69.34%	8.908%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028431.D
 Acq On : 08 Oct 2022 01:13
 Operator : SY/MD
 Sample : N4942-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.805	3346	3348	3352	rBV3	533	428	0.03%	0.004%
78	11.844	3355	3360	3364	rVB4	877	632	0.04%	0.006%
79	11.866	3364	3367	3370	rBV3	599	496	0.03%	0.004%
80	11.895	3373	3376	3379	rBV4	577	450	0.03%	0.004%
81	12.056	3424	3426	3429	rBV4	855	515	0.04%	0.005%
82	12.262	3488	3490	3493	rVB3	1250	625	0.04%	0.006%
83	12.287	3493	3498	3499	rBV3	646	608	0.04%	0.005%
84	12.349	3508	3517	3524	rBV7	5131	7884	0.55%	0.070%
85	12.516	3567	3569	3572	rBV2	883	466	0.03%	0.004%
86	12.570	3582	3586	3589	rBV5	748	588	0.04%	0.005%
87	12.631	3602	3605	3607	rBV4	537	394	0.03%	0.004%
88	12.702	3624	3627	3628	rBV3	869	366	0.03%	0.003%
89	12.795	3654	3656	3660	rBV3	463	321	0.02%	0.003%
90	12.873	3677	3680	3681	rBV2	736	446	0.03%	0.004%
91	12.959	3704	3707	3709	rBV3	512	368	0.03%	0.003%
92	13.188	3773	3778	3782	rBV3	826	707	0.05%	0.006%
93	13.339	3821	3825	3826	rBV3	582	404	0.03%	0.004%
94	13.448	3856	3859	3860	rBV2	790	416	0.03%	0.004%
95	13.487	3868	3871	3875	rBV4	863	538	0.04%	0.005%
96	13.725	3941	3945	3947	rBV3	768	691	0.05%	0.006%
97	14.017	4034	4036	4038	rBV3	633	396	0.03%	0.004%
98	14.072	4051	4053	4057	rBV3	860	607	0.04%	0.005%
99	14.204	4090	4094	4098	rBV4	988	856	0.06%	0.008%
100	14.500	4180	4186	4188	rBV4	1199	1078	0.07%	0.010%




Sum of corrected areas: 11237865

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028431.D
Acq On : 08 Oct 2022 01:13
Operator : SY/MD
Sample : N4942-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

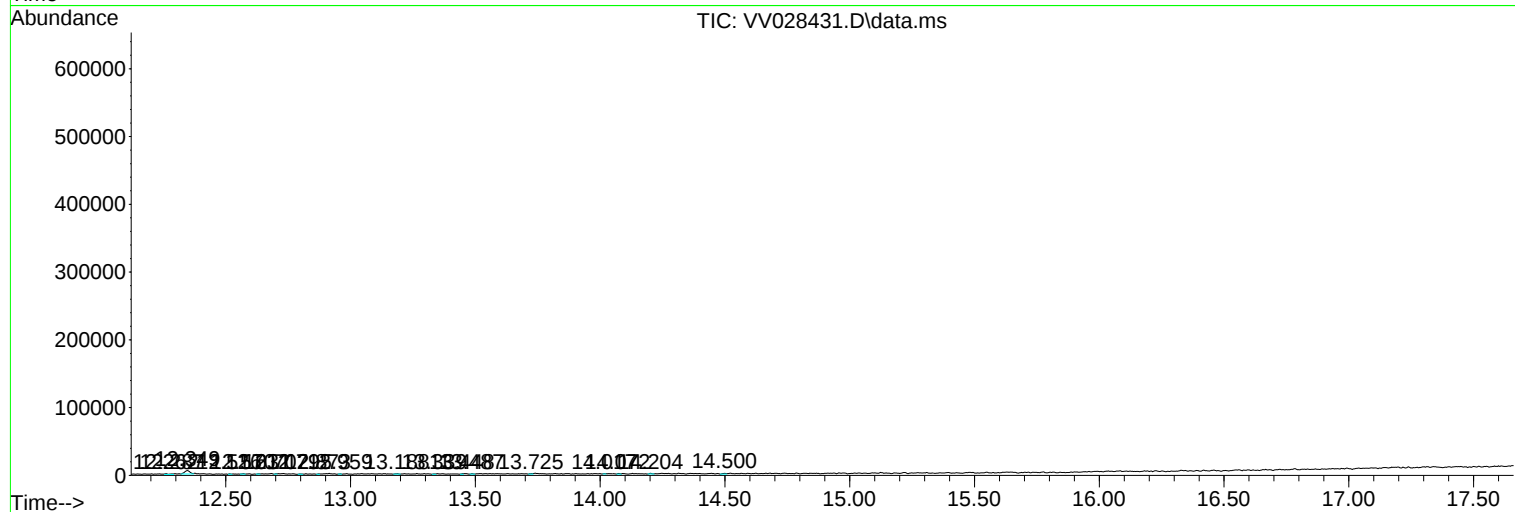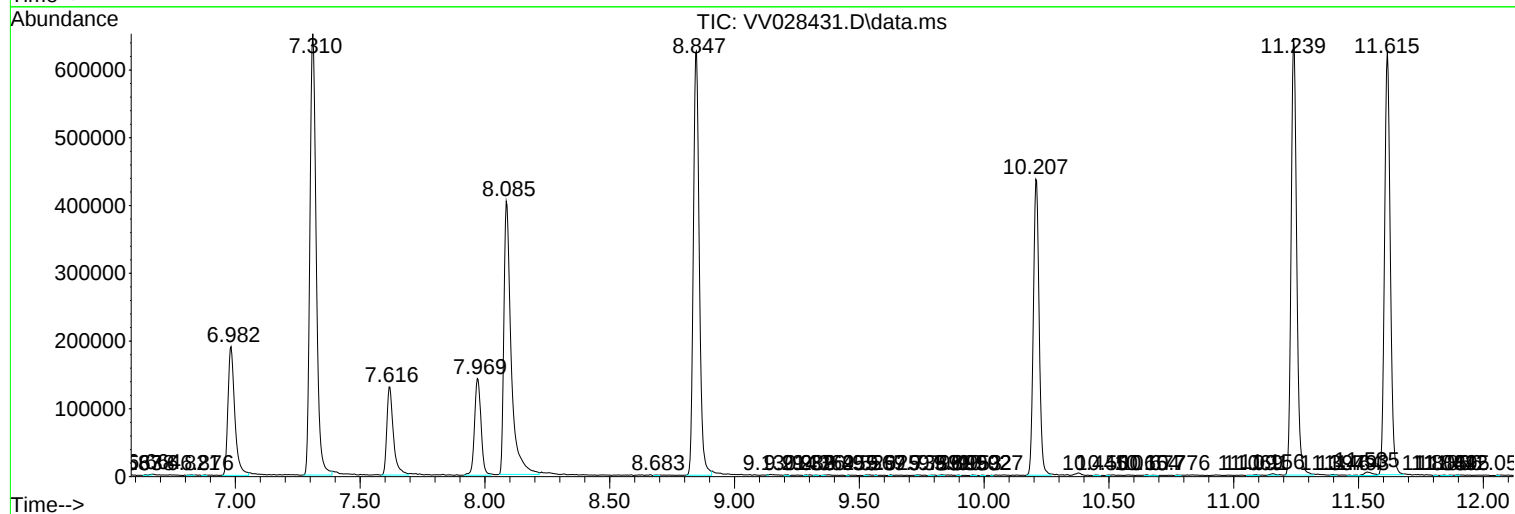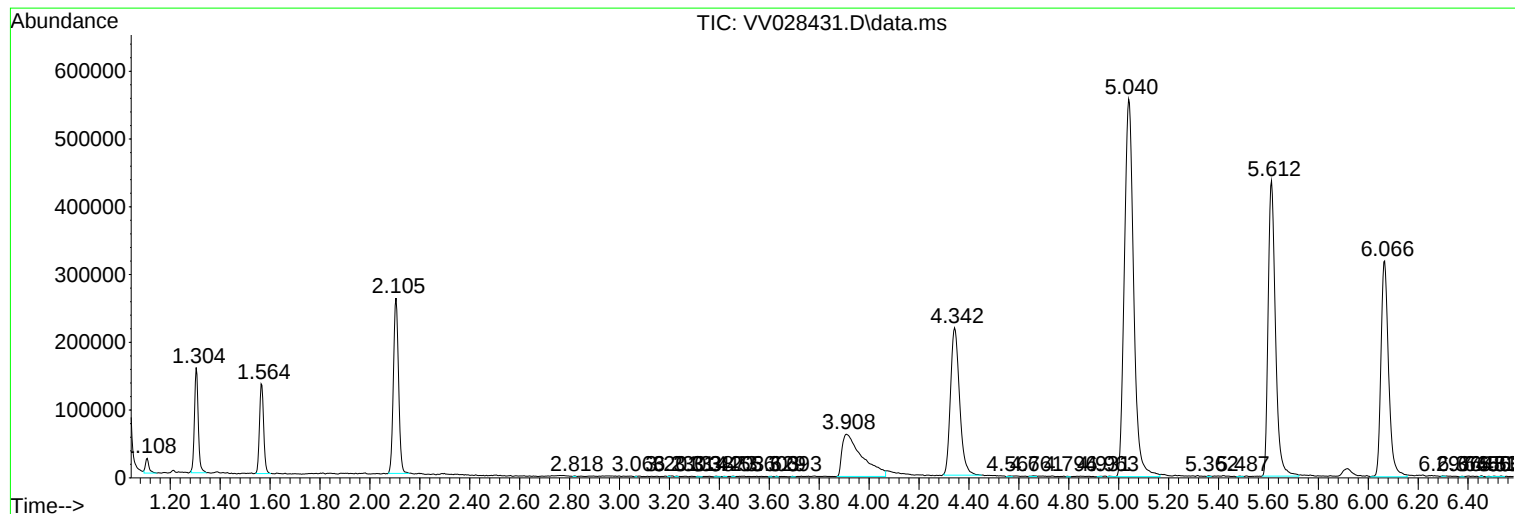

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028431.D
Acq On : 08 Oct 2022 01:13
Operator : SY/MD
Sample : N4942-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028431.D
Acq On : 08 Oct 2022 01:13
Operator : SY/MD
Sample : N4942-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc