

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028435.D
 Acq On : 08 Oct 2022 02:49
 Operator : SY/MD
 Sample : N4942-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028435.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	94	rVB	148800	153006	10.49%	1.366%
2	1.568	157	164	181	rVB	132171	154654	10.61%	1.381%
3	2.105	322	331	349	rVB	252994	364669	25.01%	3.257%
4	2.616	485	490	492	rBV4	1101	1167	0.08%	0.010%
5	3.220	676	678	683	rVB3	562	374	0.03%	0.003%
6	3.288	696	699	702	rVB4	648	419	0.03%	0.004%
7	3.330	707	712	715	rBV4	679	587	0.04%	0.005%
8	3.513	766	769	772	rBV2	752	371	0.03%	0.003%
9	3.532	772	775	776	rBV3	588	290	0.02%	0.003%
10	3.735	836	838	843	rVB4	515	292	0.02%	0.003%
11	3.773	843	850	853	rBV4	675	841	0.06%	0.008%
12	3.802	857	859	861	rBV3	523	263	0.02%	0.002%
13	3.908	880	892	935	rBV2	70181	371004	25.44%	3.313%
14	4.343	1014	1027	1056	rVB	221003	553938	37.99%	4.947%
15	4.773	1158	1161	1166	rBV5	702	497	0.03%	0.004%
16	4.799	1166	1169	1171	rBV3	495	306	0.02%	0.003%
17	4.924	1205	1208	1211	rVB5	1100	720	0.05%	0.006%
18	4.941	1211	1213	1214	rBV	795	313	0.02%	0.003%
19	5.040	1228	1244	1281	rBV2	558516	1458116	100.00%	13.021%
20	5.481	1378	1381	1382	rBV2	800	465	0.03%	0.004%
21	5.613	1410	1422	1444	rBV	432766	873965	59.94%	7.805%
22	6.066	1549	1563	1587	rBV	321433	678055	46.50%	6.055%
23	6.323	1641	1643	1646	rVB3	1138	636	0.04%	0.006%
24	6.400	1665	1667	1670	rBV2	831	445	0.03%	0.004%
25	6.420	1671	1673	1680	rBV7	1103	813	0.06%	0.007%
26	6.474	1689	1690	1694	rVB2	849	483	0.03%	0.004%
27	6.513	1700	1702	1704	rBV2	624	265	0.02%	0.002%
28	6.561	1716	1717	1721	rVB4	680	320	0.02%	0.003%
29	6.918	1826	1828	1831	rBV2	690	394	0.03%	0.004%
30	6.982	1837	1848	1880	rBV	190418	361864	24.82%	3.232%
31	7.310	1938	1950	1973	rBV	661561	1157980	79.42%	10.341%
32	7.619	2033	2046	2065	rBV	129801	241429	16.56%	2.156%
33	7.821	2107	2109	2113	rBV3	569	319	0.02%	0.003%
34	7.886	2125	2129	2131	rBV3	701	419	0.03%	0.004%
35	7.973	2145	2156	2171	rVB	84906	145255	9.96%	1.297%
36	8.085	2181	2191	2232	rBV	425955	894452	61.34%	7.988%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028435.D
 Acq On : 08 Oct 2022 02:49
 Operator : SY/MD
 Sample : N4942-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	8.477	2311	2313	2316	rBV4	652	417	0.03%	0.004%
38	8.693	2379	2380	2383	rVB2	664	280	0.02%	0.003%
39	8.738	2391	2394	2396	rBV4	688	447	0.03%	0.004%
40	8.770	2401	2404	2405	rBV3	749	471	0.03%	0.004%
41	8.844	2416	2427	2450	rBV	613611	1021940	70.09%	9.126%
42	9.143	2517	2520	2521	rBV3	845	546	0.04%	0.005%
43	9.175	2527	2530	2533	rBV4	815	396	0.03%	0.004%
44	9.210	2539	2541	2545	rVB2	698	507	0.03%	0.005%
45	9.252	2552	2554	2559	rVB5	898	815	0.06%	0.007%
46	9.278	2559	2562	2563	rBV3	993	591	0.04%	0.005%
47	9.301	2566	2569	2570	rBV3	590	314	0.02%	0.003%
48	9.329	2575	2578	2580	rBV3	433	340	0.02%	0.003%
49	9.358	2585	2587	2589	rBV3	475	259	0.02%	0.002%
50	9.407	2598	2602	2604	rBV4	621	365	0.03%	0.003%
51	9.448	2611	2615	2618	rBV3	549	387	0.03%	0.003%
52	9.490	2625	2628	2630	rVB3	844	467	0.03%	0.004%
53	9.506	2630	2633	2634	rBV2	576	334	0.02%	0.003%
54	9.612	2663	2666	2670	rBV5	823	787	0.05%	0.007%
55	9.651	2676	2678	2681	rBV4	506	364	0.02%	0.003%
56	9.693	2687	2691	2692	rBV3	493	298	0.02%	0.003%
57	9.728	2698	2702	2703	rBV4	545	287	0.02%	0.003%
58	9.783	2717	2719	2721	rBV	472	312	0.02%	0.003%
59	9.818	2728	2730	2732	rVV2	609	269	0.02%	0.002%
60	9.915	2758	2760	2764	rVB5	476	294	0.02%	0.003%
61	10.114	2819	2822	2823	rBV2	517	251	0.02%	0.002%
62	10.207	2839	2851	2871	rBV	449590	719696	49.36%	6.427%
63	10.429	2918	2920	2922	rVB3	1065	469	0.03%	0.004%
64	10.445	2922	2925	2928	rBV3	988	721	0.05%	0.006%
65	10.464	2928	2931	2933	rVV3	441	278	0.02%	0.002%
66	10.635	2982	2984	2988	rVB4	448	300	0.02%	0.003%
67	10.706	3004	3006	3009	rBV4	517	273	0.02%	0.002%
68	10.744	3015	3018	3021	rBV4	882	503	0.03%	0.004%
69	10.844	3045	3049	3052	rBV5	747	610	0.04%	0.005%
70	10.937	3077	3078	3080	rBV	553	289	0.02%	0.003%
71	11.021	3101	3104	3106	rBV2	660	356	0.02%	0.003%
72	11.101	3127	3129	3132	rVB3	909	482	0.03%	0.004%
73	11.162	3140	3148	3151	rBV6	1242	1532	0.11%	0.014%
74	11.239	3161	3172	3199	rBV	628774	989697	67.88%	8.838%
75	11.416	3225	3227	3229	rBV2	635	262	0.02%	0.002%
76	11.468	3241	3243	3246	rBV2	576	379	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028435.D
 Acq On : 08 Oct 2022 02:49
 Operator : SY/MD
 Sample : N4942-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.490	3248	3250	3253	rVB3	696	304	0.02%	0.003%
78	11.538	3257	3265	3274	rBV10	3088	6046	0.41%	0.054%
79	11.616	3278	3289	3312	rVV	633993	1012848	69.46%	9.045%
80	11.776	3337	3339	3342	rBV4	1001	580	0.04%	0.005%
81	11.960	3393	3396	3399	rBV4	634	418	0.03%	0.004%
82	12.124	3445	3447	3450	rVV3	562	247	0.02%	0.002%
83	12.239	3480	3483	3489	rBV7	1225	1056	0.07%	0.009%
84	12.384	3526	3528	3531	rBV2	749	368	0.03%	0.003%
85	12.435	3542	3544	3547	rBV3	543	394	0.03%	0.004%
86	12.525	3570	3572	3575	rVB2	835	404	0.03%	0.004%
87	12.542	3575	3577	3582	rBV4	1052	644	0.04%	0.006%
88	12.583	3588	3590	3593	rBV4	556	355	0.02%	0.003%
89	12.677	3614	3619	3620	rBV4	678	492	0.03%	0.004%
90	12.876	3676	3681	3684	rBV6	638	660	0.05%	0.006%
91	12.911	3688	3692	3696	rBV4	819	885	0.06%	0.008%
92	13.033	3729	3730	3733	rBV	613	389	0.03%	0.003%
93	13.114	3750	3755	3756	rBV2	743	615	0.04%	0.005%
94	13.246	3795	3796	3801	rBV4	620	578	0.04%	0.005%
95	13.326	3817	3821	3824	rBV5	445	377	0.03%	0.003%
96	13.596	3903	3905	3908	rBV3	598	390	0.03%	0.003%
97	13.622	3911	3913	3916	rBV	676	397	0.03%	0.004%
98	13.821	3972	3975	3977	rBV3	849	616	0.04%	0.006%
99	14.066	4047	4051	4054	rBV3	929	971	0.07%	0.009%
100	14.947	4323	4325	4328	rBV4	1142	851	0.06%	0.008%




Sum of corrected areas: 11197856

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028435.D
Acq On : 08 Oct 2022 02:49
Operator : SY/MD
Sample : N4942-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

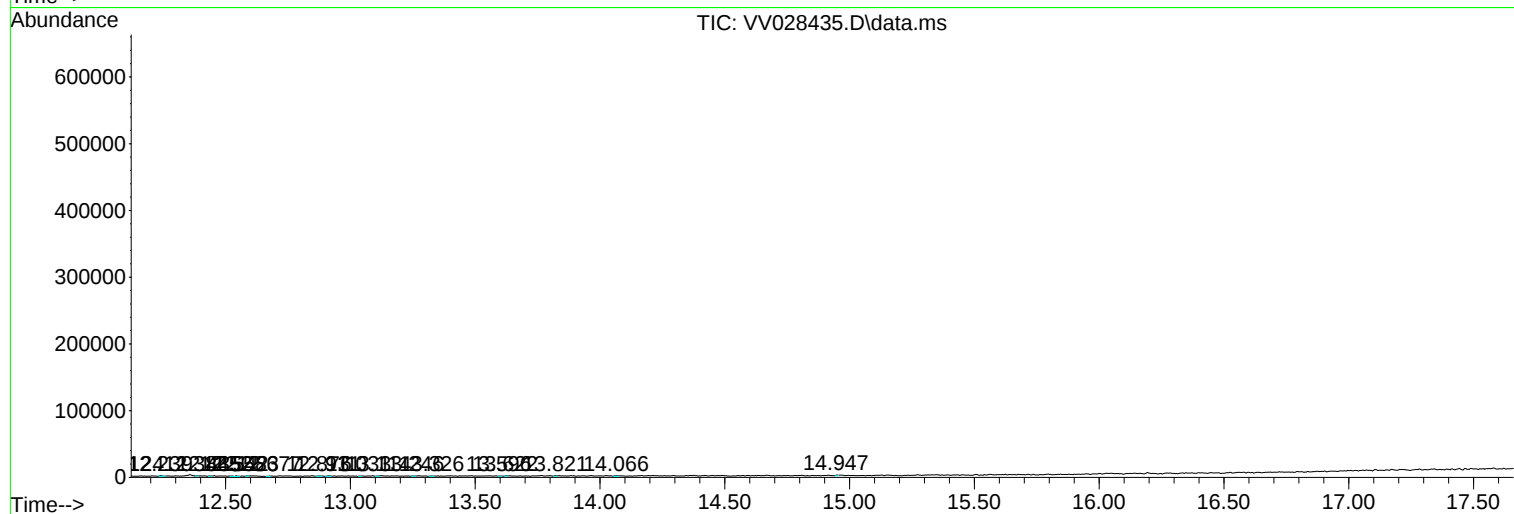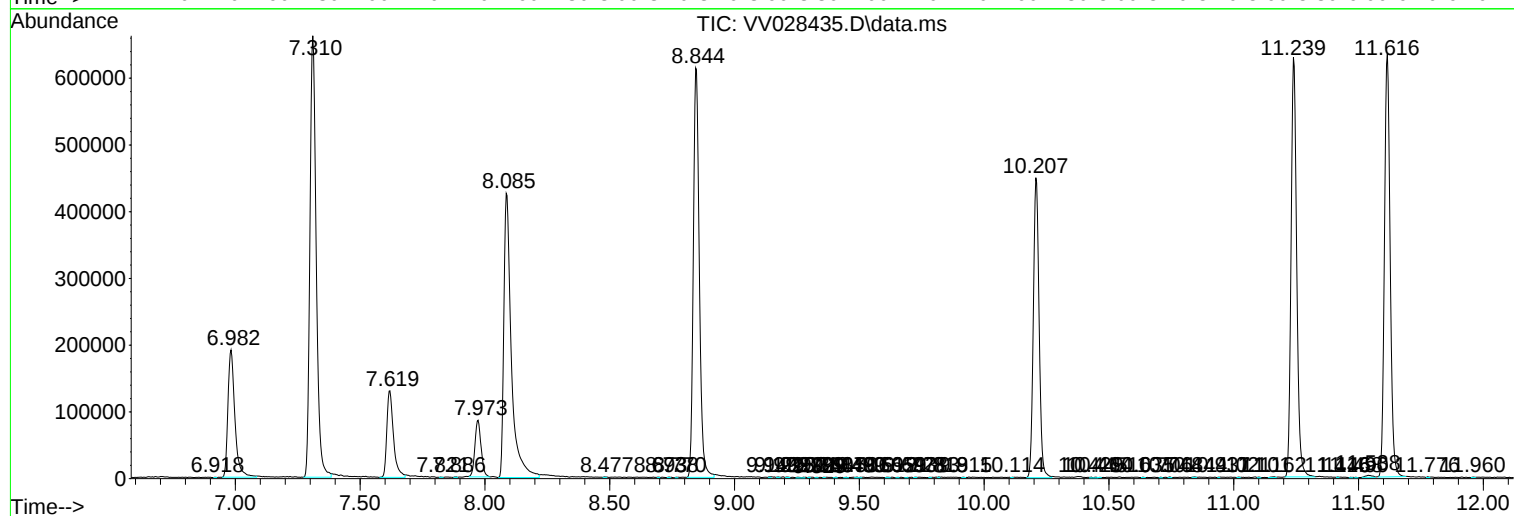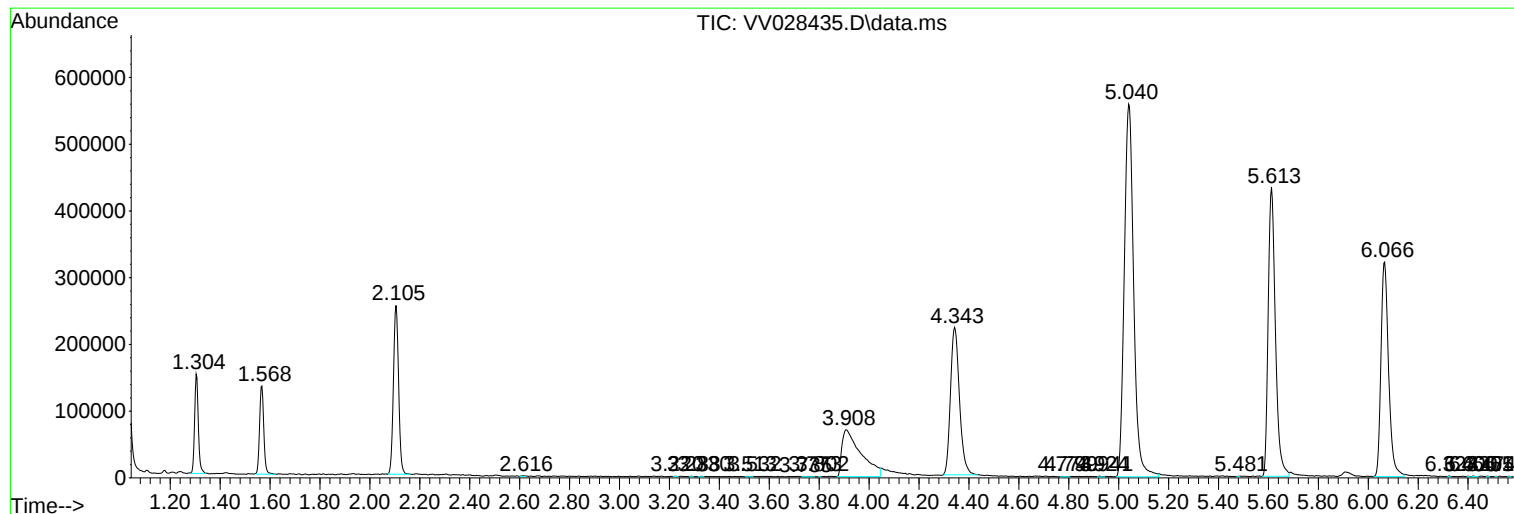

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028435.D
Acq On : 08 Oct 2022 02:49
Operator : SY/MD
Sample : N4942-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028435.D
Acq On : 08 Oct 2022 02:49
Operator : SY/MD
Sample : N4942-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc