

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028436.D
 Acq On : 08 Oct 2022 03:13
 Operator : SY/MD
 Sample : N4942-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028436.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.108	17	21	30	rVB	27995	26277	1.87%	0.246%
2	1.304	75	82	95	rVB	147224	153619	10.94%	1.437%
3	1.565	156	163	178	rVB	125842	146152	10.41%	1.367%
4	2.105	321	331	350	rVB	241691	348591	24.83%	3.260%
5	3.076	630	633	635	rVB4	741	437	0.03%	0.004%
6	3.121	645	647	652	rBV3	455	456	0.03%	0.004%
7	3.163	656	660	661	rBV3	706	464	0.03%	0.004%
8	3.452	747	750	755	rBV4	647	502	0.04%	0.005%
9	3.548	778	780	782	rBV3	275	118	0.01%	0.001%
10	3.584	789	791	792	rBV2	940	355	0.03%	0.003%
11	3.645	807	810	815	rBV4	547	529	0.04%	0.005%
12	3.677	818	820	822	rBV2	627	375	0.03%	0.004%
13	3.728	834	836	839	rBV4	420	289	0.02%	0.003%
14	3.745	839	841	842	rBV2	607	245	0.02%	0.002%
15	3.847	869	873	876	rBV4	936	527	0.04%	0.005%
16	3.899	876	889	917	rBV	74031	294046	20.94%	2.750%
17	4.343	1014	1027	1053	rVB	211660	524188	37.33%	4.902%
18	4.719	1143	1144	1148	rBV2	610	475	0.03%	0.004%
19	4.899	1197	1200	1203	rBV3	447	332	0.02%	0.003%
20	4.918	1203	1206	1207	rBV3	728	359	0.03%	0.003%
21	5.040	1228	1244	1277	rBV2	543898	1404046	100.00%	13.130%
22	5.371	1343	1347	1350	rBV4	878	756	0.05%	0.007%
23	5.548	1397	1402	1407	rBV5	1086	1287	0.09%	0.012%
24	5.568	1407	1408	1409	rBV	593	208	0.01%	0.002%
25	5.613	1410	1422	1447	rBV	426228	866670	61.73%	8.104%
26	5.873	1501	1503	1504	rBV2	854	361	0.03%	0.003%
27	6.066	1549	1563	1588	rBV	311220	649299	46.24%	6.072%
28	6.394	1662	1665	1669	rBV4	755	622	0.04%	0.006%
29	6.510	1695	1701	1703	rBV5	468	479	0.03%	0.004%
30	6.613	1731	1733	1738	rBV5	673	613	0.04%	0.006%
31	6.741	1769	1773	1778	rBV5	705	815	0.06%	0.008%
32	6.783	1781	1786	1788	rBV5	773	573	0.04%	0.005%
33	6.863	1808	1811	1814	rBV3	935	465	0.03%	0.004%
34	6.883	1814	1817	1818	rBV	365	278	0.02%	0.003%
35	6.899	1820	1822	1824	rBV	499	205	0.01%	0.002%
36	6.982	1836	1848	1878	rBV	181991	348983	24.86%	3.263%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100722\
 Data File : VW028436.D
 Acq On : 08 Oct 2022 03:13
 Operator : SY/MD
 Sample : N4942-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.185	1905	1911	1914	rBV6	1313	1659	0.12%	0.016%
38	7.310	1939	1950	1969	rBV	642396	1107286	78.86%	10.354%
39	7.616	2036	2045	2067	rBV	124931	227869	16.23%	2.131%
40	7.924	2136	2141	2142	rBV4	1241	1150	0.08%	0.011%
41	7.976	2149	2157	2168	rVB8	8542	15997	1.14%	0.150%
42	8.021	2168	2171	2172	rBV2	720	422	0.03%	0.004%
43	8.085	2181	2191	2226	rBV	405400	835644	59.52%	7.814%
44	8.561	2337	2339	2344	rBV4	605	369	0.03%	0.003%
45	8.616	2353	2356	2362	rVB5	838	751	0.05%	0.007%
46	8.680	2374	2376	2377	rBV2	369	172	0.01%	0.002%
47	8.741	2390	2395	2397	rBV4	658	550	0.04%	0.005%
48	8.847	2416	2428	2454	rBV	618921	1018671	72.55%	9.526%
49	9.117	2510	2512	2514	rBV3	598	254	0.02%	0.002%
50	9.268	2554	2559	2560	rBV3	744	579	0.04%	0.005%
51	9.336	2578	2580	2581	rBV	555	263	0.02%	0.002%
52	9.394	2595	2598	2603	rBV4	855	842	0.06%	0.008%
53	9.426	2605	2608	2609	rBV2	590	311	0.02%	0.003%
54	9.484	2624	2626	2628	rBV	384	211	0.02%	0.002%
55	9.500	2629	2631	2635	rVV4	468	350	0.02%	0.003%
56	9.603	2657	2663	2668	rBV6	594	694	0.05%	0.006%
57	9.625	2668	2670	2672	rBV2	321	202	0.01%	0.002%
58	9.712	2695	2697	2699	rBV2	891	476	0.03%	0.004%
59	9.767	2711	2714	2717	rBV4	439	381	0.03%	0.004%
60	9.911	2757	2759	2763	rBV2	689	448	0.03%	0.004%
61	10.011	2786	2790	2792	rBV3	866	677	0.05%	0.006%
62	10.153	2832	2834	2836	rBV2	358	156	0.01%	0.001%
63	10.207	2840	2851	2874	rVV	432503	687042	48.93%	6.425%
64	10.423	2916	2918	2920	rBV2	394	172	0.01%	0.002%
65	10.439	2920	2923	2927	rBV5	468	418	0.03%	0.004%
66	10.474	2930	2934	2935	rBV3	440	210	0.01%	0.002%
67	10.493	2938	2940	2942	rBV2	442	235	0.02%	0.002%
68	10.577	2962	2966	2975	rVB7	927	1278	0.09%	0.012%
69	10.612	2975	2977	2981	rBV4	566	471	0.03%	0.004%
70	10.921	3071	3073	3075	rBV2	866	378	0.03%	0.004%
71	11.011	3098	3101	3103	rVB3	555	295	0.02%	0.003%
72	11.024	3103	3105	3107	rBV2	491	285	0.02%	0.003%
73	11.056	3109	3115	3118	rVB6	919	893	0.06%	0.008%
74	11.079	3118	3122	3124	rBV4	823	755	0.05%	0.007%
75	11.149	3135	3144	3154	rBV5	10120	16542	1.18%	0.155%
76	11.239	3161	3172	3194	rBV	612827	978128	69.66%	9.147%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028436.D
 Acq On : 08 Oct 2022 03:13
 Operator : SY/MD
 Sample : N4942-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGS2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.616	3277	3289	3311	rBV	622848	978542	69.69%	9.151%
78	11.796	3342	3345	3348	rBV3	643	573	0.04%	0.005%
79	11.854	3361	3363	3369	rVB4	722	613	0.04%	0.006%
80	11.882	3369	3372	3375	rBV3	557	533	0.04%	0.005%
81	12.101	3438	3440	3441	rBV	412	186	0.01%	0.002%
82	12.207	3471	3473	3475	rVB2	698	336	0.02%	0.003%
83	12.223	3475	3478	3479	rBV2	698	325	0.02%	0.003%
84	12.252	3485	3487	3490	rBV2	512	267	0.02%	0.002%
85	12.310	3503	3505	3506	rBV2	830	401	0.03%	0.004%
86	12.339	3507	3514	3527	rVB3	17386	28016	2.00%	0.262%
87	12.683	3618	3621	3623	rBV3	699	360	0.03%	0.003%
88	12.924	3693	3696	3697	rBV	630	372	0.03%	0.003%
89	12.944	3700	3702	3708	rVB4	880	657	0.05%	0.006%
90	13.046	3732	3734	3736	rBV2	488	243	0.02%	0.002%
91	13.130	3758	3760	3762	rBV2	591	319	0.02%	0.003%
92	13.249	3795	3797	3798	rBV2	495	165	0.01%	0.002%
93	13.320	3817	3819	3821	rBV	717	462	0.03%	0.004%
94	13.374	3831	3836	3837	rBV3	817	570	0.04%	0.005%
95	13.509	3876	3878	3880	rBV	762	387	0.03%	0.004%
96	13.638	3915	3918	3920	rBV3	888	471	0.03%	0.004%
97	13.702	3935	3938	3942	rBV4	887	785	0.06%	0.007%
98	13.853	3982	3985	3986	rBV3	646	306	0.02%	0.003%
99	14.201	4091	4093	4098	rBV4	1009	440	0.03%	0.004%
100	14.879	4301	4304	4307	rBV4	1201	975	0.07%	0.009%




Sum of corrected areas: 10693786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028436.D
Acq On : 08 Oct 2022 03:13
Operator : SY/MD
Sample : N4942-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

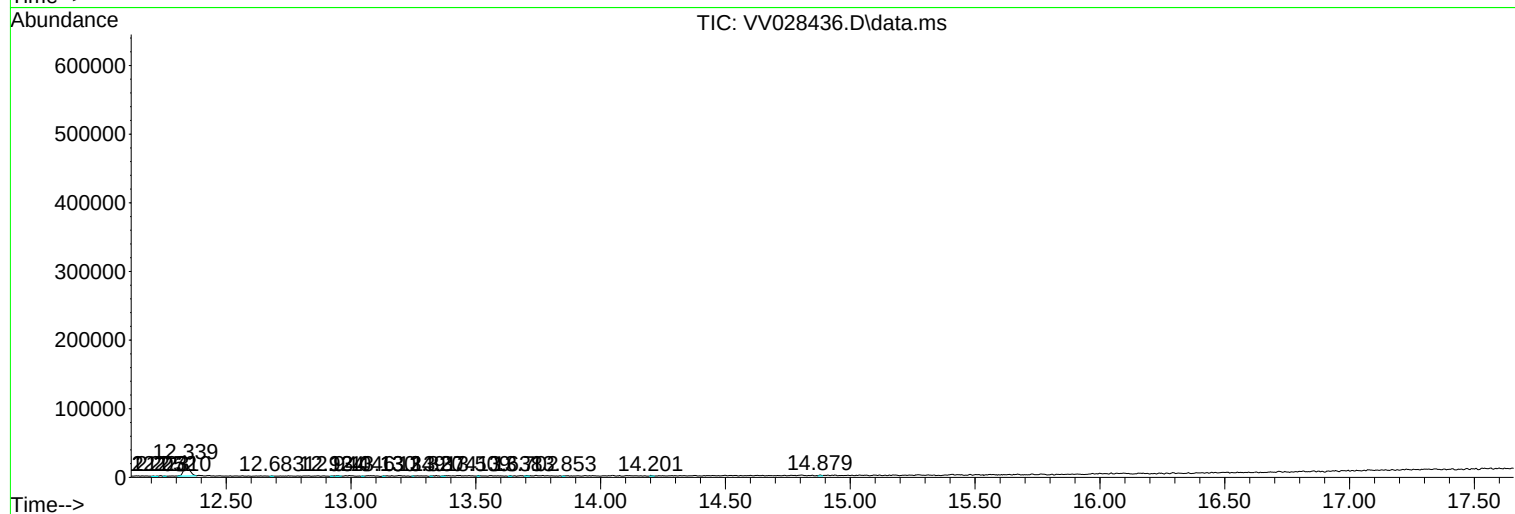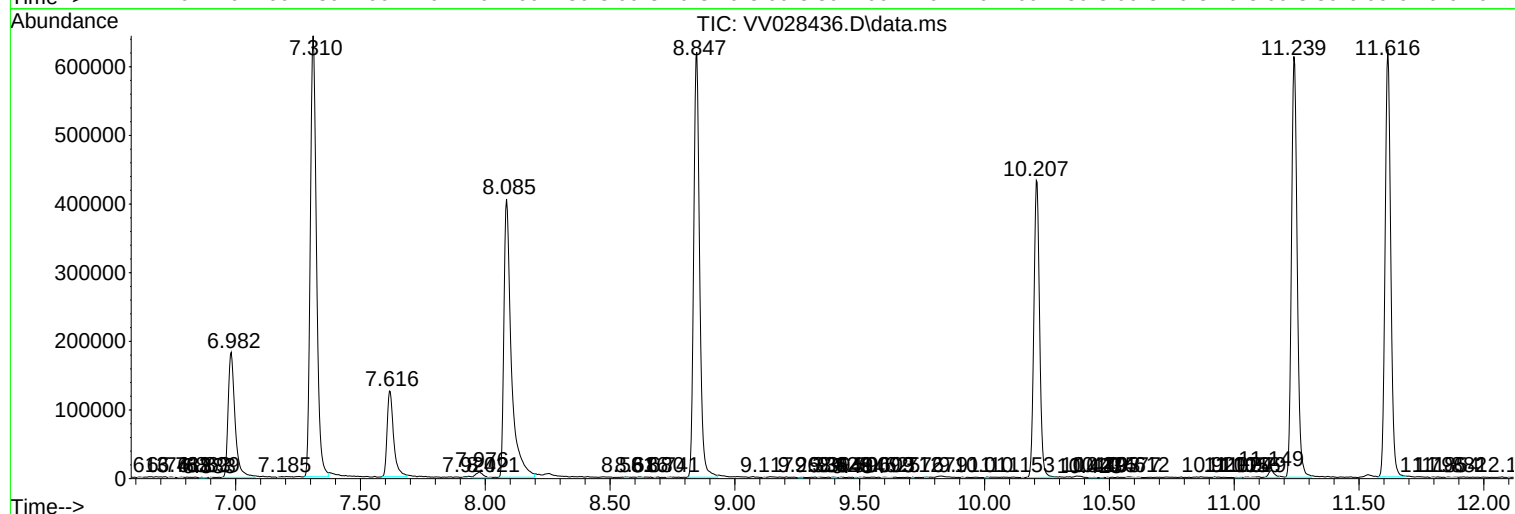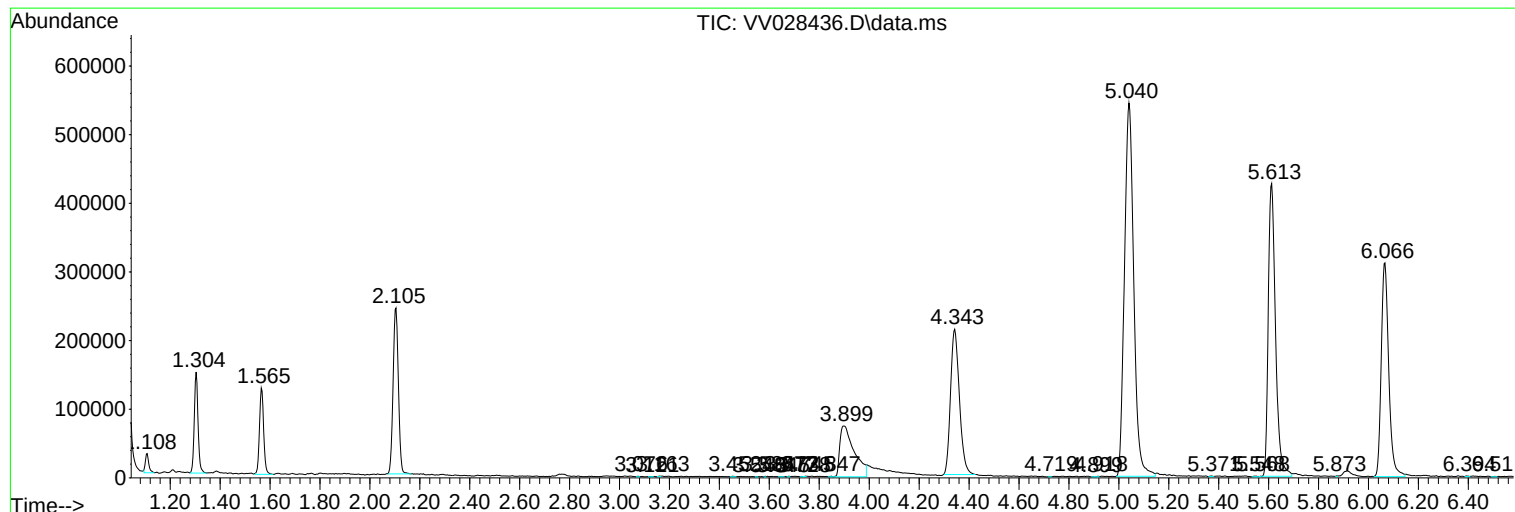

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028436.D
Acq On : 08 Oct 2022 03:13
Operator : SY/MD
Sample : N4942-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGS2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028436.D
Acq On : 08 Oct 2022 03:13
Operator : SY/MD
Sample : N4942-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 45 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc