

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028437.D
 Acq On : 08 Oct 2022 03:38
 Operator : SY/MD
 Sample : N4942-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028437.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	96	rVB	141023	144506	10.19%	1.343%
2	1.564	157	163	176	rVB	123562	143842	10.15%	1.337%
3	2.105	322	331	348	rVB	245778	350675	24.74%	3.259%
4	3.088	633	637	639	rBV5	626	486	0.03%	0.005%
5	3.127	646	649	652	rVV4	811	534	0.04%	0.005%
6	3.150	654	656	659	rVB3	789	519	0.04%	0.005%
7	3.182	663	666	670	rBV5	917	782	0.06%	0.007%
8	3.211	670	675	676	rBV3	627	341	0.02%	0.003%
9	3.365	719	723	730	rVB7	797	977	0.07%	0.009%
10	3.400	730	734	736	rBV3	490	400	0.03%	0.004%
11	3.551	779	781	787	rVB4	878	796	0.06%	0.007%
12	3.587	787	792	794	rBV5	618	554	0.04%	0.005%
13	3.664	812	816	817	rBV3	589	312	0.02%	0.003%
14	3.696	823	826	830	rBV6	760	503	0.04%	0.005%
15	3.773	847	850	852	rBV2	850	467	0.03%	0.004%
16	3.905	879	891	929	rBV2	72508	348571	24.59%	3.239%
17	4.342	1012	1027	1057	rBV	213826	546459	38.55%	5.078%
18	4.703	1137	1139	1143	rBV3	444	308	0.02%	0.003%
19	4.741	1147	1151	1155	rBV6	796	836	0.06%	0.008%
20	4.870	1190	1191	1198	rVB5	1046	946	0.07%	0.009%
21	4.905	1198	1202	1206	rBV4	1108	1095	0.08%	0.010%
22	5.040	1226	1244	1287	rBV2	545825	1417492	100.00%	13.171%
23	5.339	1334	1337	1341	rBV6	681	483	0.03%	0.004%
24	5.416	1359	1361	1370	rVB7	1155	1208	0.09%	0.011%
25	5.612	1410	1422	1447	rBV	426925	869709	61.36%	8.081%
26	5.905	1506	1513	1527	rBV	6463	14207	1.00%	0.132%
27	6.014	1544	1547	1549	rBV4	1167	846	0.06%	0.008%
28	6.066	1550	1563	1586	rVV	314895	644945	45.50%	5.993%
29	6.484	1690	1693	1697	rBV5	589	494	0.03%	0.005%
30	6.522	1702	1705	1707	rBV4	1044	583	0.04%	0.005%
31	6.651	1742	1745	1750	rBV6	1062	1017	0.07%	0.009%
32	6.751	1773	1776	1781	rVB5	670	520	0.04%	0.005%
33	6.863	1809	1811	1815	rBV4	678	494	0.03%	0.005%
34	6.924	1828	1830	1833	rVB4	780	305	0.02%	0.003%
35	6.982	1834	1848	1874	rBV	185942	349062	24.63%	3.244%
36	7.194	1910	1914	1918	rBV4	1513	1704	0.12%	0.016%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028437.D
 Acq On : 08 Oct 2022 03:38
 Operator : SY/MD
 Sample : N4942-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.310	1939	1950	1972	rBV	639529	1106794	78.08%	10.284%
38	7.619	2036	2046	2068	rBV	124917	228362	16.11%	2.122%
39	7.812	2102	2106	2111	rVB5	1082	832	0.06%	0.008%
40	7.979	2154	2158	2159	rBV4	639	378	0.03%	0.004%
41	7.989	2159	2161	2166	rVV4	552	470	0.03%	0.004%
42	8.085	2182	2191	2231	rBV	417883	824468	58.16%	7.661%
43	8.574	2341	2343	2345	rBV3	707	375	0.03%	0.003%
44	8.599	2348	2351	2355	rVB4	550	450	0.03%	0.004%
45	8.780	2403	2407	2410	rBV6	410	364	0.03%	0.003%
46	8.796	2410	2412	2413	rBV2	592	290	0.02%	0.003%
47	8.847	2416	2428	2459	rVV	614358	1011112	71.33%	9.395%
48	9.095	2501	2505	2508	rBV5	1135	1159	0.08%	0.011%
49	9.236	2545	2549	2554	rBV4	859	962	0.07%	0.009%
50	9.567	2649	2652	2654	rVB5	806	428	0.03%	0.004%
51	9.664	2679	2682	2683	rBV2	735	360	0.03%	0.003%
52	9.734	2699	2704	2707	rBV3	866	778	0.05%	0.007%
53	9.821	2723	2731	2738	rBV9	3138	5179	0.37%	0.048%
54	9.963	2773	2775	2779	rBV4	534	386	0.03%	0.004%
55	9.995	2783	2785	2790	rBV4	441	327	0.02%	0.003%
56	10.075	2808	2810	2817	rVB5	866	971	0.07%	0.009%
57	10.107	2817	2820	2823	rBV3	689	542	0.04%	0.005%
58	10.207	2840	2851	2873	rBV	428473	687198	48.48%	6.386%
59	10.419	2914	2917	2920	rBV4	484	318	0.02%	0.003%
60	10.464	2929	2931	2932	rBV	614	290	0.02%	0.003%
61	10.519	2942	2948	2949	rBV2	1378	1256	0.09%	0.012%
62	10.606	2972	2975	2976	rBV2	750	407	0.03%	0.004%
63	10.654	2987	2990	2992	rVB3	619	393	0.03%	0.004%
64	10.683	2992	2999	3000	rBV4	940	836	0.06%	0.008%
65	10.709	3004	3007	3010	rBV3	734	586	0.04%	0.005%
66	10.892	3062	3064	3068	rVB3	726	390	0.03%	0.004%
67	10.911	3068	3070	3072	rBV2	799	365	0.03%	0.003%
68	11.033	3105	3108	3109	rBV2	776	500	0.04%	0.005%
69	11.146	3134	3143	3155	rBV7	15194	27736	1.96%	0.258%
70	11.239	3161	3172	3196	rBV	616427	964060	68.01%	8.958%
71	11.426	3227	3230	3233	rBV4	770	596	0.04%	0.006%
72	11.480	3243	3247	3251	rBV4	840	756	0.05%	0.007%
73	11.535	3259	3264	3275	rVB9	3994	6670	0.47%	0.062%
74	11.615	3277	3289	3312	rBV	620733	980274	69.16%	9.109%
75	11.754	3329	3332	3336	rBV6	1230	1078	0.08%	0.010%
76	11.818	3350	3352	3355	rBV5	838	483	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028437.D
 Acq On : 08 Oct 2022 03:38
 Operator : SY/MD
 Sample : N4942-09
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	11.869	3365	3368	3370	rBV3	453	325	0.02%	0.003%
78	11.940	3387	3390	3392	rBV2	631	413	0.03%	0.004%
79	12.146	3452	3454	3459	rVV4	852	558	0.04%	0.005%
80	12.172	3459	3462	3466	rVB3	609	565	0.04%	0.005%
81	12.226	3474	3479	3480	rBV4	753	600	0.04%	0.006%
82	12.339	3505	3514	3528	rBV2	28470	43497	3.07%	0.404%
83	12.435	3542	3544	3547	rBV3	579	338	0.02%	0.003%
84	12.503	3562	3565	3569	rVB4	1199	842	0.06%	0.008%
85	12.522	3569	3571	3574	rBV2	586	370	0.03%	0.003%
86	12.622	3599	3602	3605	rVV3	658	560	0.04%	0.005%
87	12.657	3608	3613	3614	rVV3	951	649	0.05%	0.006%
88	12.676	3617	3619	3621	rVV2	896	340	0.02%	0.003%
89	12.770	3646	3648	3650	rBV3	737	323	0.02%	0.003%
90	12.844	3669	3671	3676	rVB6	911	652	0.05%	0.006%
91	12.879	3679	3682	3684	rBV3	752	430	0.03%	0.004%
92	13.053	3732	3736	3740	rBV5	777	586	0.04%	0.005%
93	13.085	3743	3746	3749	rVV4	601	462	0.03%	0.004%
94	13.474	3864	3867	3870	rBV5	790	725	0.05%	0.007%
95	13.583	3898	3901	3906	rVB4	995	859	0.06%	0.008%
96	13.609	3906	3909	3911	rBV4	686	395	0.03%	0.004%
97	13.992	4026	4028	4033	rVB5	720	320	0.02%	0.003%
98	14.127	4068	4070	4075	rVB3	676	502	0.04%	0.005%
99	14.156	4075	4079	4082	rBV5	980	842	0.06%	0.008%
100	14.258	4108	4111	4112	rBV	805	512	0.04%	0.005%




Sum of corrected areas: 10761822

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028437.D
Acq On : 08 Oct 2022 03:38
Operator : SY/MD
Sample : N4942-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

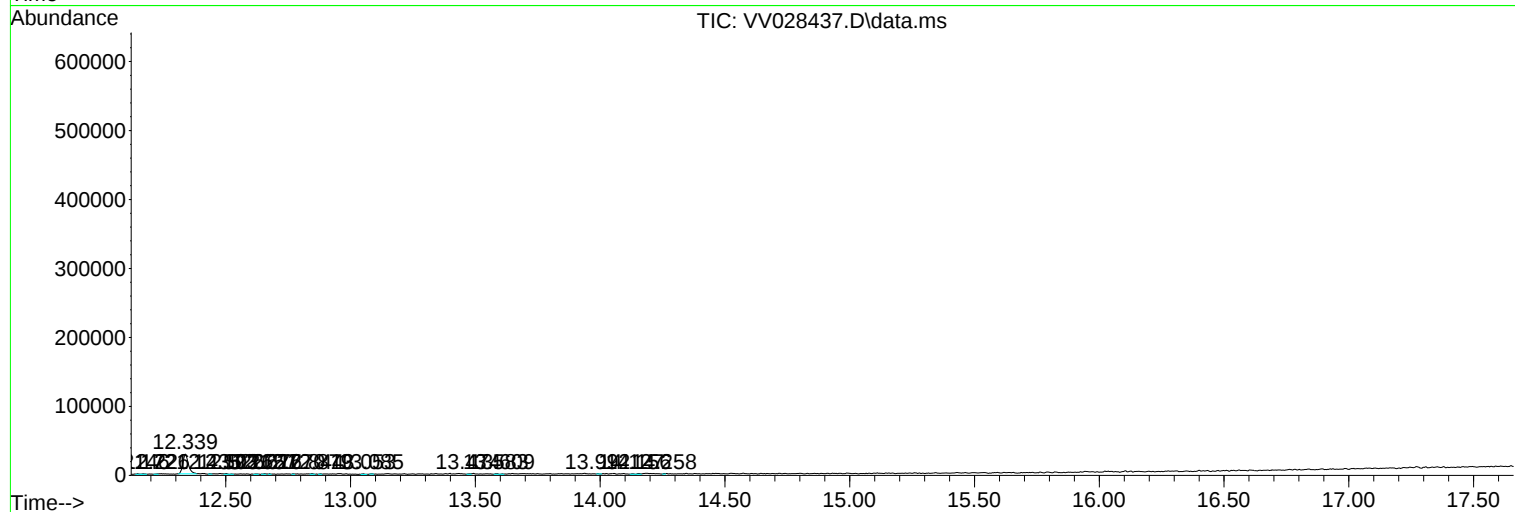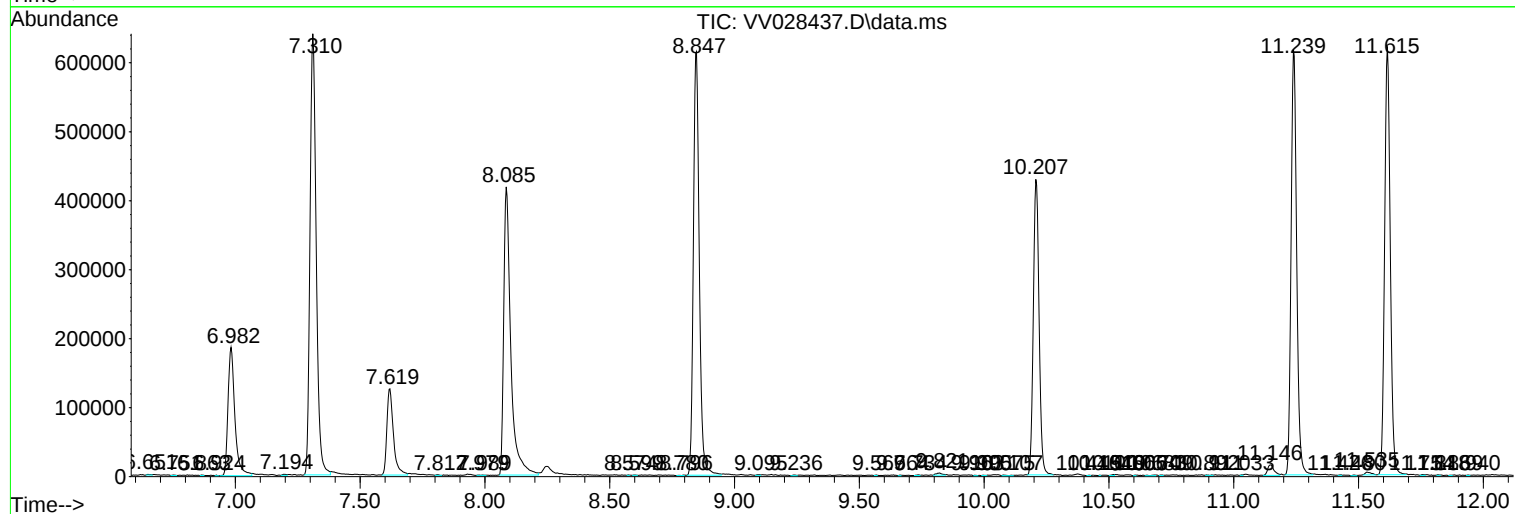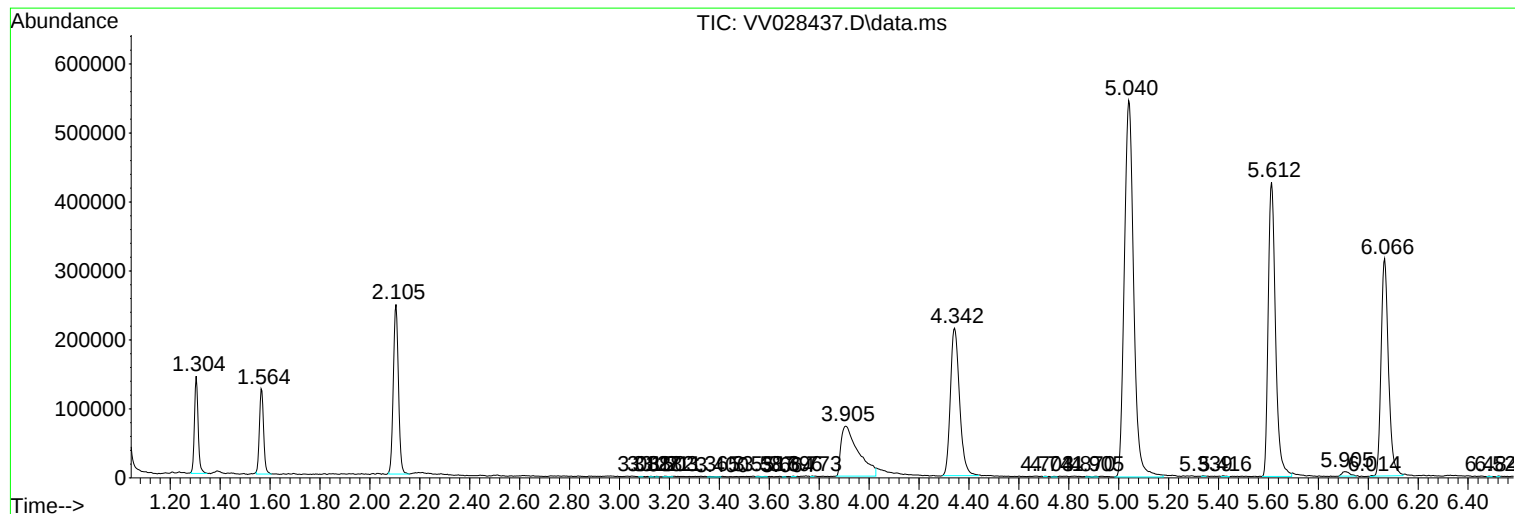

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028437.D
Acq On : 08 Oct 2022 03:38
Operator : SY/MD
Sample : N4942-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028437.D
Acq On : 08 Oct 2022 03:38
Operator : SY/MD
Sample : N4942-09
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 46 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc