

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028438.D
 Acq On : 08 Oct 2022 04:02
 Operator : SY/MD
 Sample : N4942-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

Signal : TIC: VV028438.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	147179	152333	10.74%	1.388%
2	1.565	156	163	177	rVB	124625	141828	10.00%	1.293%
3	2.101	321	330	345	rVB	242671	349032	24.61%	3.181%
4	2.564	472	474	477	rBV4	833	452	0.03%	0.004%
5	3.111	642	644	648	rBV4	422	349	0.02%	0.003%
6	3.500	760	765	767	rBV3	874	611	0.04%	0.006%
7	3.529	767	774	776	rBV5	899	685	0.05%	0.006%
8	3.587	787	792	793	rBV	704	504	0.04%	0.005%
9	3.677	815	820	823	rBV6	692	717	0.05%	0.007%
10	3.783	850	853	855	rBV	560	407	0.03%	0.004%
11	3.892	877	887	922	rBV2	80558	310632	21.90%	2.831%
12	4.343	1013	1027	1060	rVB	215254	547954	38.63%	4.994%
13	4.603	1105	1108	1109	rBV2	857	417	0.03%	0.004%
14	4.674	1124	1130	1131	rBV5	708	608	0.04%	0.006%
15	4.754	1152	1155	1156	rBV	535	344	0.02%	0.003%
16	5.040	1228	1244	1281	rBV2	541482	1418395	100.00%	12.927%
17	5.352	1338	1341	1342	rBV3	808	350	0.02%	0.003%
18	5.474	1377	1379	1381	rVB3	966	363	0.03%	0.003%
19	5.500	1382	1387	1391	rVV4	899	970	0.07%	0.009%
20	5.613	1409	1422	1449	rBV	429329	873043	61.55%	7.957%
21	6.021	1546	1549	1550	rBV3	549	333	0.02%	0.003%
22	6.066	1550	1563	1596	rVV	317302	660221	46.55%	6.017%
23	6.320	1640	1642	1647	rVB5	835	669	0.05%	0.006%
24	6.342	1647	1649	1651	rBV2	1021	507	0.04%	0.005%
25	6.478	1688	1691	1693	rBV4	870	498	0.04%	0.005%
26	6.490	1693	1695	1697	rVV2	750	366	0.03%	0.003%
27	6.542	1706	1711	1714	rBV4	762	815	0.06%	0.007%
28	6.844	1796	1805	1809	rBV7	878	1699	0.12%	0.015%
29	6.886	1816	1818	1820	rBV2	668	419	0.03%	0.004%
30	6.912	1823	1826	1828	rBV3	532	388	0.03%	0.004%
31	6.982	1835	1848	1878	rBV	187008	357362	25.19%	3.257%
32	7.175	1906	1908	1910	rBV2	647	300	0.02%	0.003%
33	7.310	1939	1950	1975	rBV	637734	1123704	79.22%	10.242%
34	7.616	2035	2045	2075	rBV	130503	241421	17.02%	2.200%
35	7.760	2088	2090	2093	rBV3	793	444	0.03%	0.004%
36	7.902	2132	2134	2138	rBV2	923	484	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW100722\
 Data File : VW028438.D
 Acq On : 08 Oct 2022 04:02
 Operator : SY/MD
 Sample : N4942-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

37	7.969	2138	2155	2173	rBV	121566	209386	14.76%	1.908%
38	8.085	2181	2191	2230	rBV	406823	834994	58.87%	7.610%
39	8.487	2314	2316	2318	rBV2	685	363	0.03%	0.003%
40	8.545	2332	2334	2337	rBV2	475	299	0.02%	0.003%
41	8.577	2342	2344	2347	rVB2	663	298	0.02%	0.003%
42	8.648	2361	2366	2369	rBV4	446	483	0.03%	0.004%
43	8.686	2375	2378	2382	rBV4	579	548	0.04%	0.005%
44	8.744	2393	2396	2397	rBV2	619	316	0.02%	0.003%
45	8.799	2411	2413	2416	rBV3	645	429	0.03%	0.004%
46	8.847	2416	2428	2447	rBV	612522	1001601	70.62%	9.129%
47	9.124	2512	2514	2516	rBV3	820	388	0.03%	0.004%
48	9.137	2516	2518	2520	rBV4	995	650	0.05%	0.006%
49	9.214	2539	2542	2544	rBV3	585	368	0.03%	0.003%
50	9.265	2555	2558	2562	rBV3	740	552	0.04%	0.005%
51	9.510	2632	2634	2638	rVB3	664	377	0.03%	0.003%
52	9.535	2638	2642	2644	rBV3	460	368	0.03%	0.003%
53	9.632	2670	2672	2674	rBV4	662	364	0.03%	0.003%
54	9.760	2709	2712	2715	rBV3	581	326	0.02%	0.003%
55	9.931	2760	2765	2767	rBV5	737	680	0.05%	0.006%
56	10.018	2790	2792	2795	rVB5	692	370	0.03%	0.003%
57	10.079	2808	2811	2814	rVB5	879	663	0.05%	0.006%
58	10.108	2816	2820	2823	rBV4	573	557	0.04%	0.005%
59	10.207	2839	2851	2875	rBV	432323	693195	48.87%	6.318%
60	10.371	2897	2902	2903	rBV4	1661	1283	0.09%	0.012%
61	10.628	2980	2982	2986	rVB5	692	386	0.03%	0.004%
62	10.645	2986	2987	2992	rVB3	502	317	0.02%	0.003%
63	10.686	2997	3000	3002	rBV2	540	369	0.03%	0.003%
64	10.722	3008	3011	3014	rBV3	687	455	0.03%	0.004%
65	10.815	3038	3040	3044	rVB4	535	354	0.02%	0.003%
66	10.841	3044	3048	3052	rVB4	752	580	0.04%	0.005%
67	11.098	3125	3128	3132	rBV	8019	4474	0.32%	0.041%
68	11.149	3137	3144	3157	rVB7	7609	11913	0.84%	0.109%
69	11.243	3162	3173	3191	rBV	632608	978658	69.00%	8.920%
70	11.532	3254	3263	3278	rBV6	6618	14849	1.05%	0.135%
71	11.616	3278	3289	3311	rVV	621729	985413	69.47%	8.981%
72	11.808	3345	3349	3350	rBV3	542	378	0.03%	0.003%
73	11.969	3396	3399	3402	rBV4	588	378	0.03%	0.003%
74	12.024	3410	3416	3417	rBV4	777	694	0.05%	0.006%
75	12.091	3431	3437	3439	rBV5	493	574	0.04%	0.005%
76	12.117	3443	3445	3448	rVB2	795	379	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
 Data File : VV028438.D
 Acq On : 08 Oct 2022 04:02
 Operator : SY/MD
 Sample : N4942-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGSJ6

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
 Title : VOC Analysis

77	12.136	3448	3451	3454	rBV2	787	471	0.03%	0.004%
78	12.342	3506	3515	3531	rBV6	11495	20698	1.46%	0.189%
79	12.435	3541	3544	3546	rBV4	799	502	0.04%	0.005%
80	12.734	3635	3637	3638	rBV2	731	369	0.03%	0.003%
81	12.812	3659	3661	3664	rBV3	601	364	0.03%	0.003%
82	12.924	3694	3696	3700	rBV4	688	504	0.04%	0.005%
83	12.943	3700	3702	3704	rBV3	624	327	0.02%	0.003%
84	13.181	3774	3776	3778	rBV2	817	515	0.04%	0.005%
85	13.294	3808	3811	3813	rBV3	771	510	0.04%	0.005%
86	13.333	3819	3823	3824	rBV5	621	387	0.03%	0.004%
87	13.368	3831	3834	3838	rBV4	611	578	0.04%	0.005%
88	13.419	3848	3850	3853	rBV2	1049	428	0.03%	0.004%
89	13.580	3897	3900	3902	rBV4	753	479	0.03%	0.004%
90	13.654	3920	3923	3927	rBV5	865	674	0.05%	0.006%
91	13.725	3940	3945	3946	rBV2	761	626	0.04%	0.006%
92	13.796	3964	3967	3969	rBV3	1356	721	0.05%	0.007%
93	13.828	3975	3977	3980	rBV4	722	445	0.03%	0.004%
94	13.953	4014	4016	4020	rBV4	715	576	0.04%	0.005%
95	14.014	4033	4035	4038	rBV3	663	431	0.03%	0.004%
96	14.207	4092	4095	4096	rBV2	910	518	0.04%	0.005%
97	14.310	4125	4127	4131	rBV4	1046	909	0.06%	0.008%
98	14.609	4217	4220	4224	rBV5	1428	898	0.06%	0.008%
99	14.648	4228	4232	4235	rBV5	893	725	0.05%	0.007%
100	15.239	4413	4416	4417	rBV2	1145	659	0.05%	0.006%




Sum of corrected areas: 10971967

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028438.D
Acq On : 08 Oct 2022 04:02
Operator : SY/MD
Sample : N4942-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

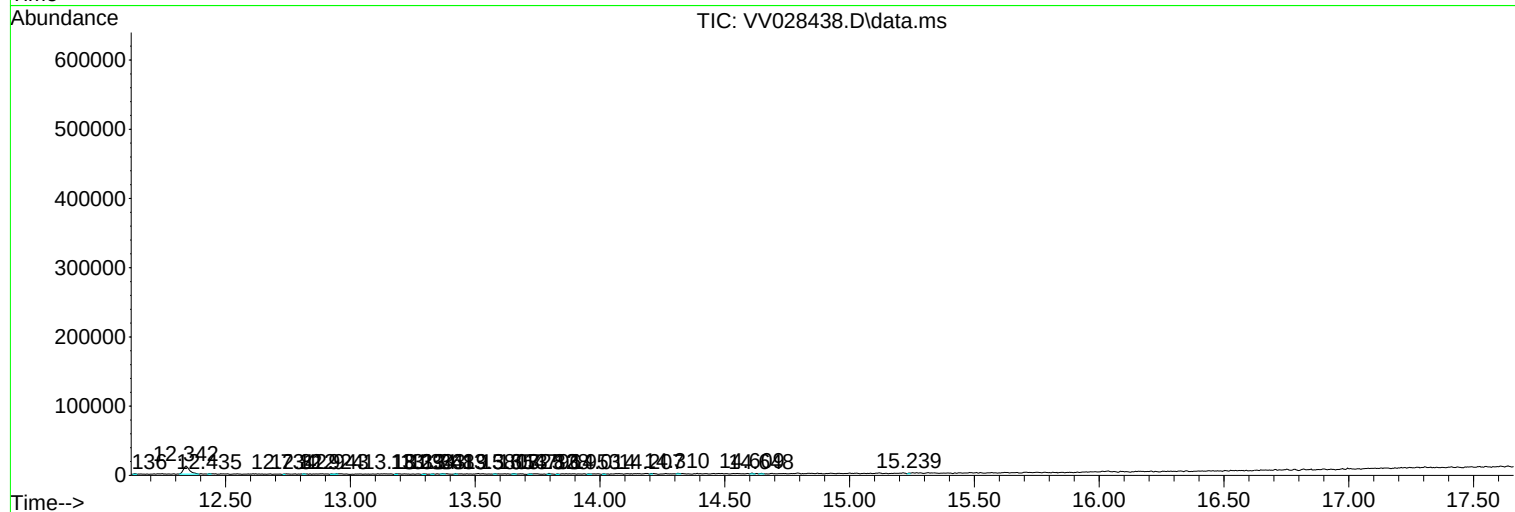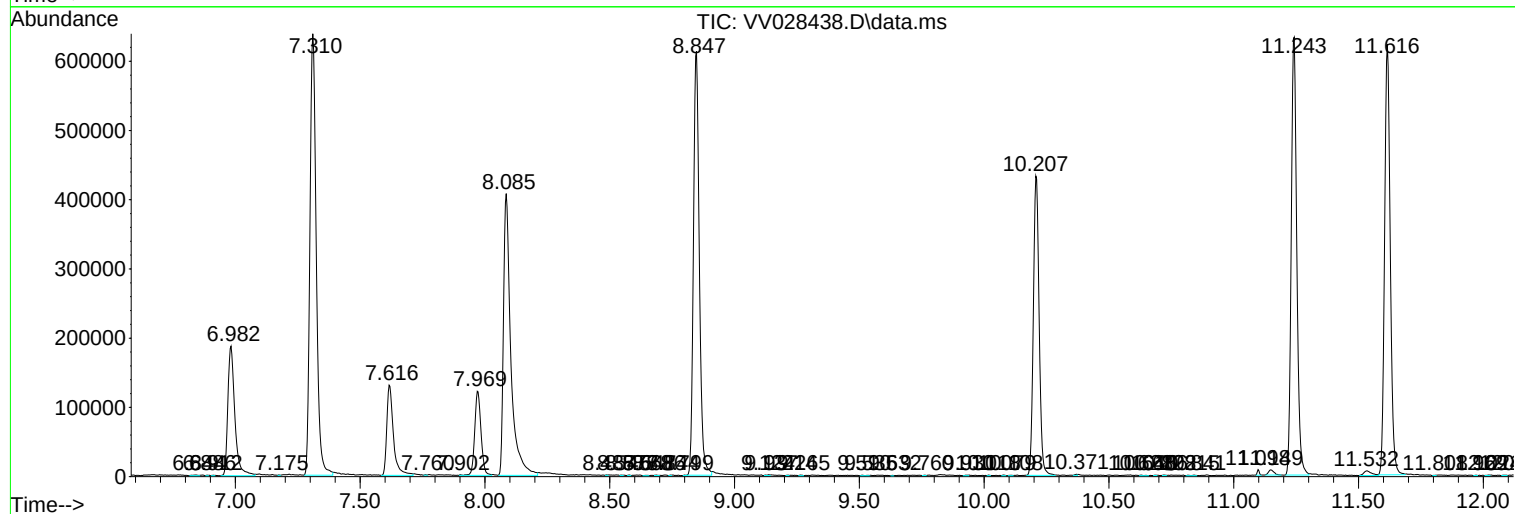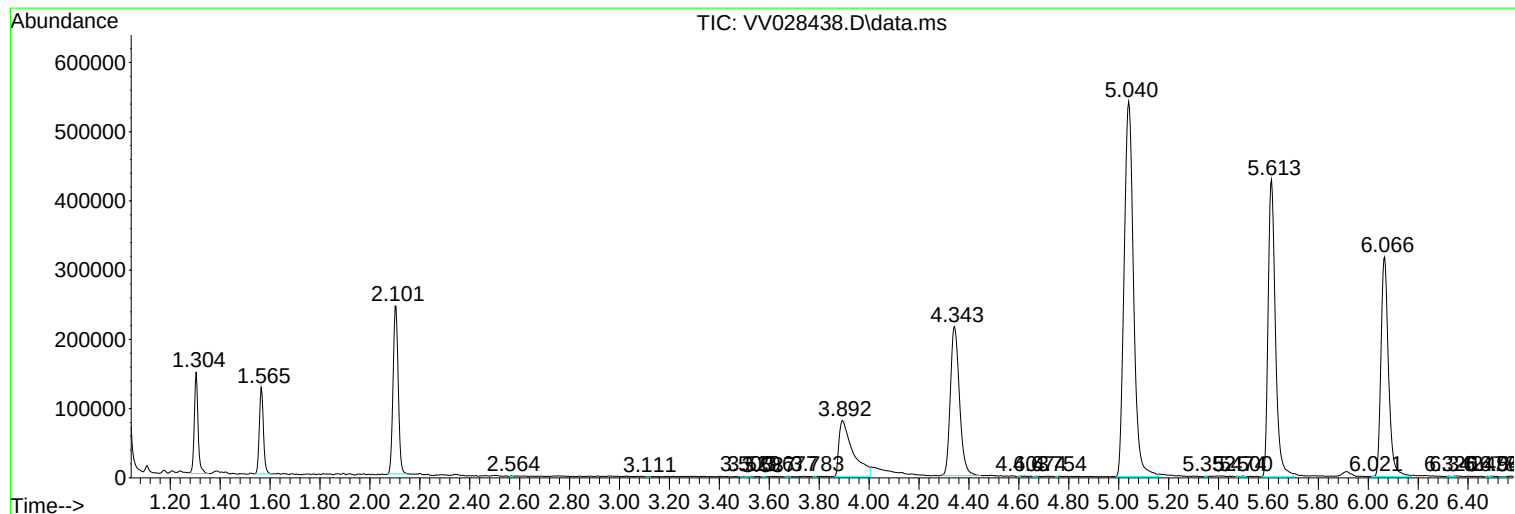

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028438.D
Acq On : 08 Oct 2022 04:02
Operator : SY/MD
Sample : N4942-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV100722\
Data File : VV028438.D
Acq On : 08 Oct 2022 04:02
Operator : SY/MD
Sample : N4942-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGSJ6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM100722WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc