

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037749.D
 Acq On : 07 Oct 2024 09:56
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 08 04:30:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 08 04:30:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	669580	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.777	117	662315	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	306007	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	245879	41.832	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	83.660%
7) Chloroethane-d5	1.532	69	203911	44.693	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	89.380%
11) 1,1-Dichloroethene-d2	2.060	65	106684	43.443	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	86.880%
21) 2-Butanone-d5	3.793	46	180234	86.089	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	86.090%
24) Chloroform-d	4.243	84	471240	45.063	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.120%
26) 1,2-Dichloroethane-d4	4.937	65	287323	46.941	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	93.880%
32) Benzene-d6	4.954	84	934702	45.100	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	90.200%
36) 1,2-Dichloropropane-d6	5.982	67	296329	44.902	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	89.800%
41) Toluene-d8	7.236	98	810286	43.117	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	86.240%
43) trans-1,3-Dichloroprop...	7.548	79	129020	42.085	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	84.160%
47) 2-Hexanone-d5	8.024	63	108788	78.066	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	78.070%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	337530	44.017	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	88.040%
66) 1,2-Dichlorobenzene-d4	11.551	152	314243	48.734	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	97.460%
Target Compounds						
39) cis-1,3-Dichloropropene	6.912	75	7900	0.959	ug/L	Qvalue # 49


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037749.D
Acq On : 07 Oct 2024 09:56
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 08 04:30:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 08 04:30:01 2024
Response via : Initial Calibration

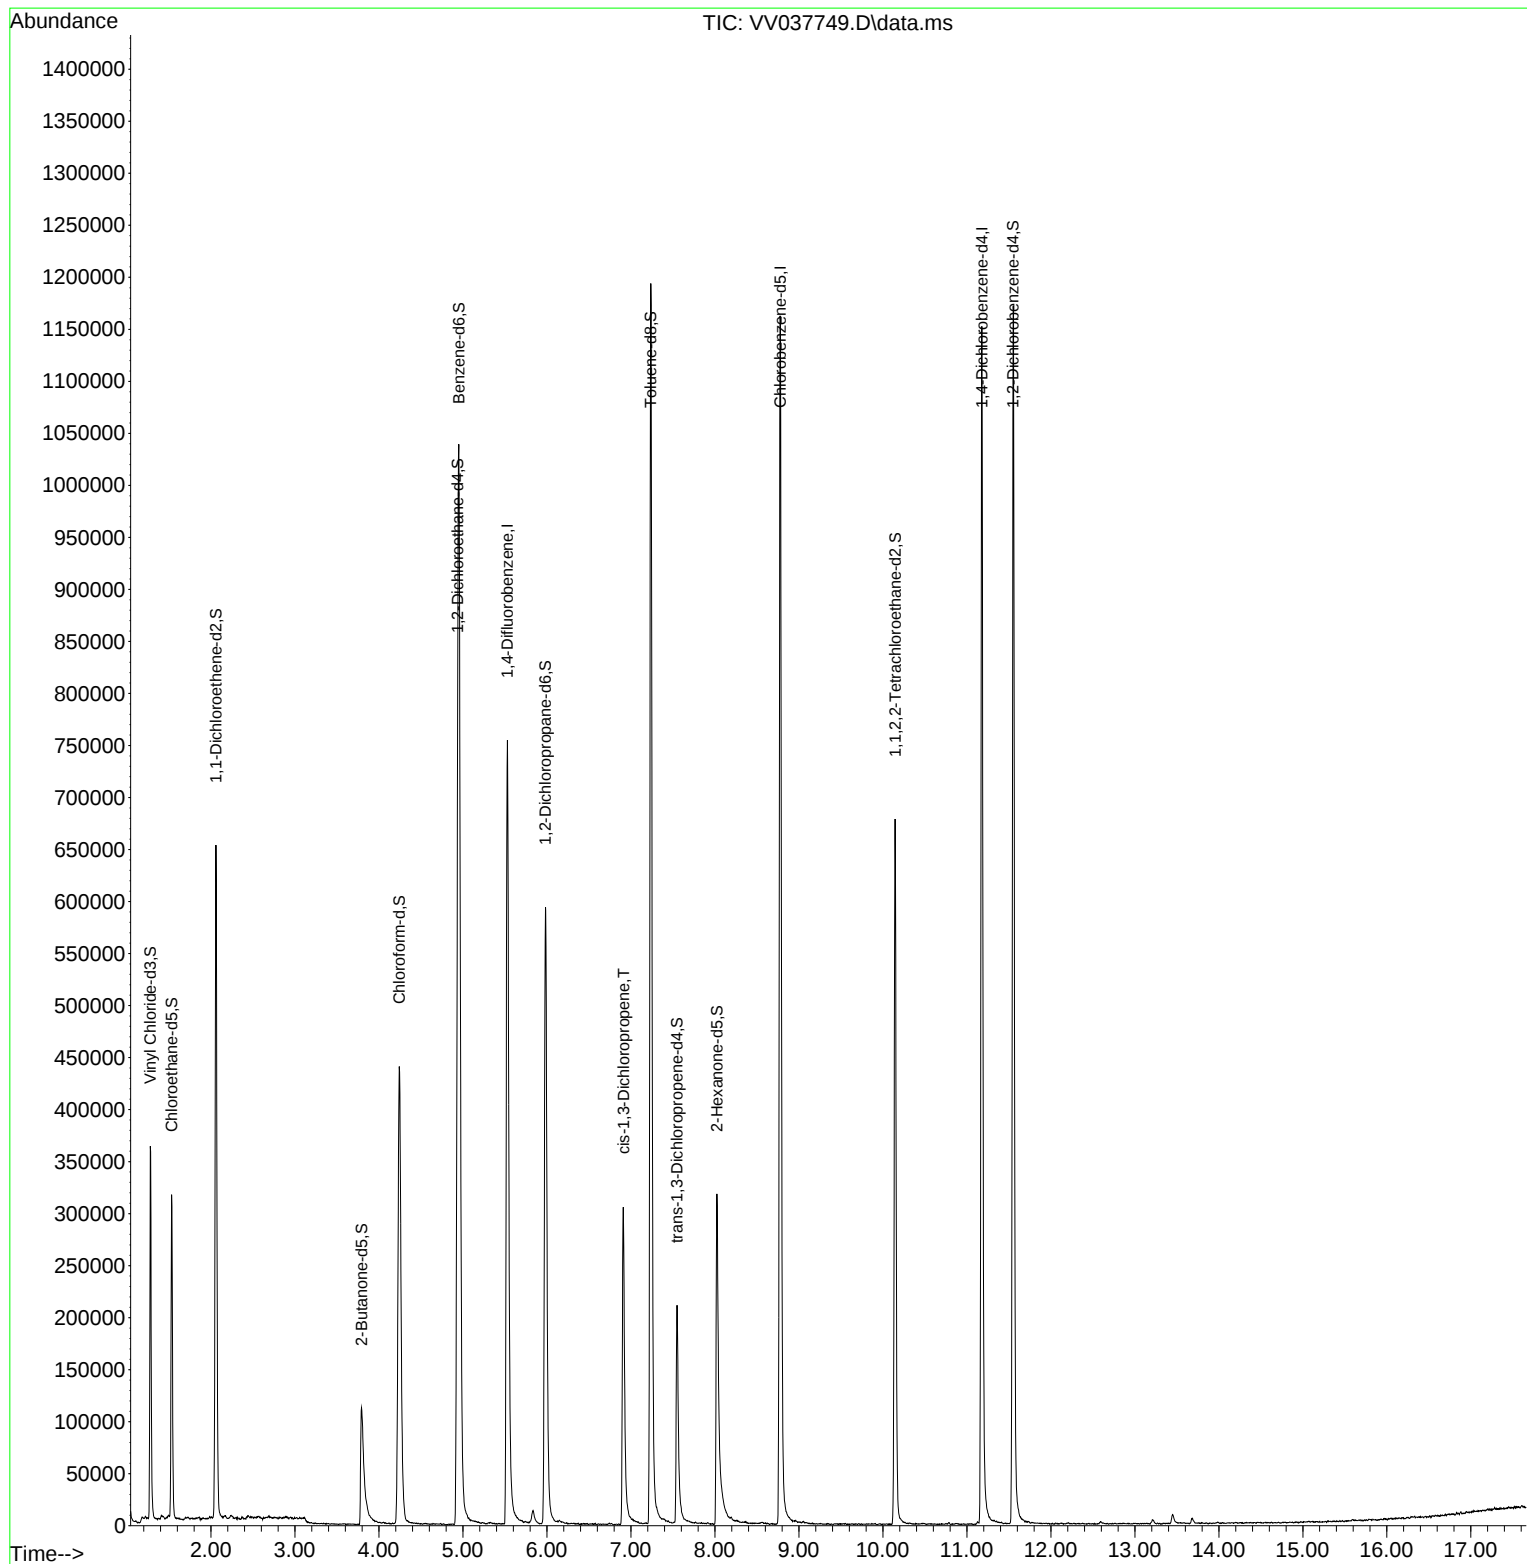

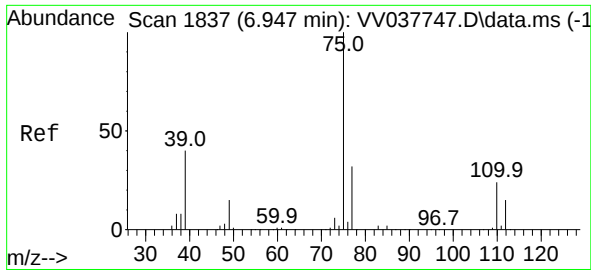

#39
cis-1,3-Dichloropropene
Concen: 0.959 ug/L
RT: 6.912 min Scan# 11
Delta R.T. -0.035 min
Lab File: VV037749.D
Acq: 07 Oct 2024 09:56

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 7900
Ion Ratio Lower Upper
75 100
77 59.4 21.8 40.4#

