

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037755.D
 Acq On : 07 Oct 2024 14:23
 Operator : SY/MD
 Sample : VIBLK
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 08 04:32:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 08 04:30:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	590983	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	587198	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	271799	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	239150	46.098	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	92.200%
7) Chloroethane-d5	1.532	69	195242	48.484	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	96.960%
11) 1,1-Dichloroethene-d2	2.060	65	103787	47.884	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	95.760%
21) 2-Butanone-d5	3.789	46	162482	87.931	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	87.930%
24) Chloroform-d	4.240	84	444381	48.146	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	96.300%
26) 1,2-Dichloroethane-d4	4.934	65	267719	49.555	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	99.100%
32) Benzene-d6	4.950	84	879773	47.880	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	95.760%
36) 1,2-Dichloropropane-d6	5.982	67	280414	47.926	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	95.860%
41) Toluene-d8	7.236	98	776386	46.598	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.200%
43) trans-1,3-Dichloroprop...	7.548	79	116436	42.838	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	85.680%
47) 2-Hexanone-d5	8.024	63	93329	75.540	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	75.540%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	295585	43.478	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	86.960%
66) 1,2-Dichlorobenzene-d4	11.554	152	292008	50.985	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	101.960%
Target Compounds						
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3449	0.819	ug/L	Qvalue # 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037755.D
Acq On : 07 Oct 2024 14:23
Operator : SY/MD
Sample : VIBLK
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 08 04:32:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 08 04:30:01 2024
Response via : Initial Calibration

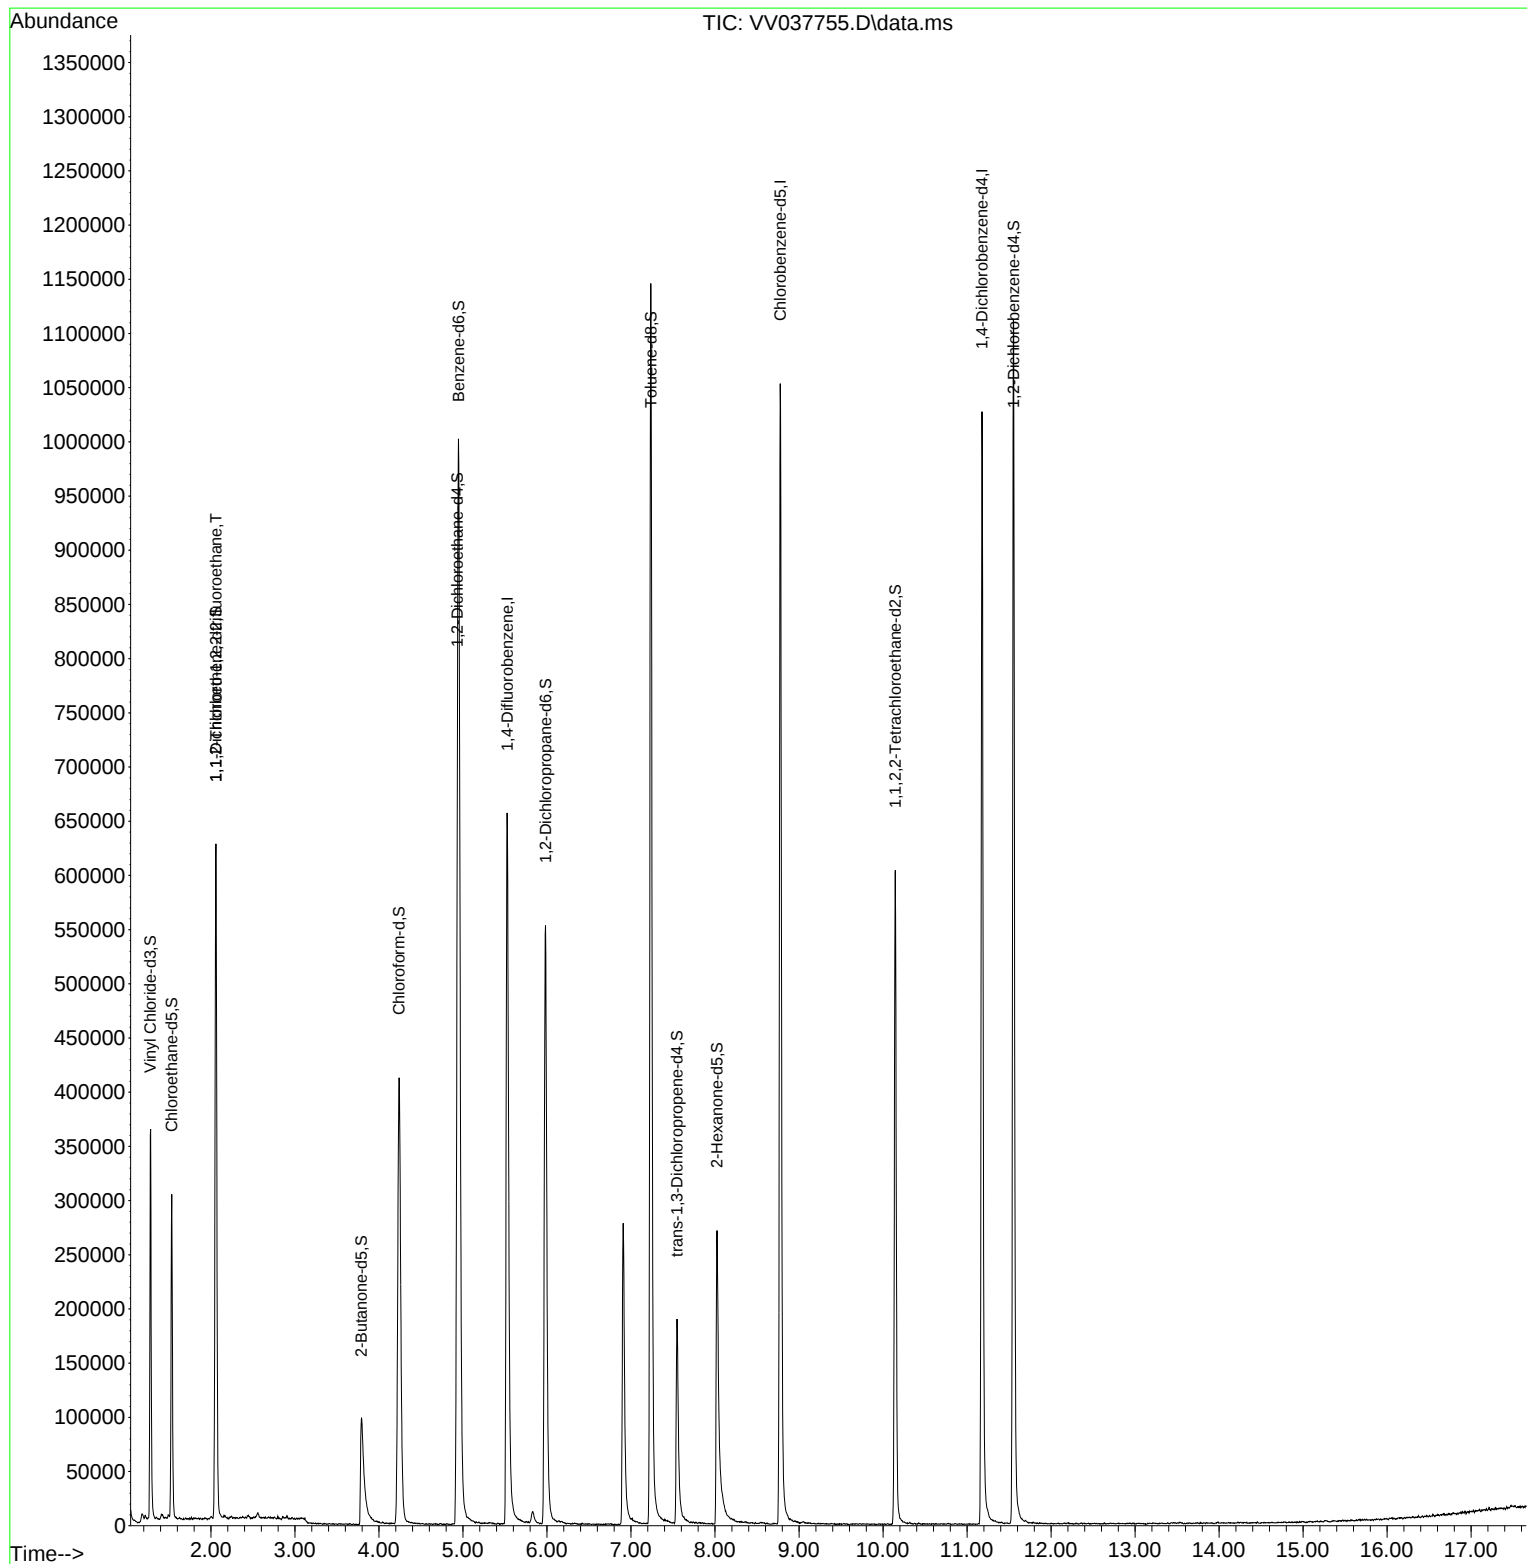

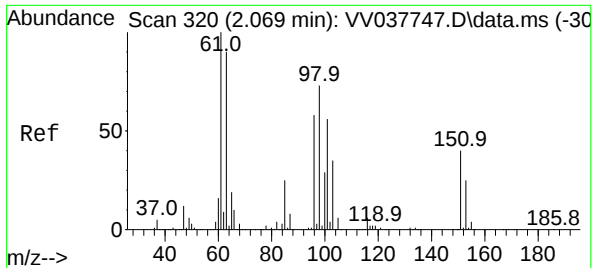

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.819 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.010 min
 Lab File: VV037755.D
 Acq: 07 Oct 2024 14:23

Instrument :
 MSVOA_V
 ClientSampleId :

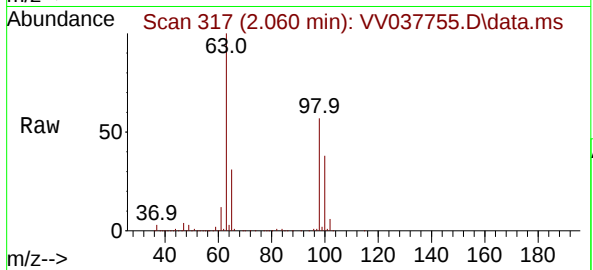

Tgt Ion:101 Resp: 3449
 Ion Ratio Lower Upper
 101 100
 85 1.3 34.6 52.0#
 151 0.0 57.5 86.3#

