

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037750.D
 Acq On : 07 Oct 2024 10:33
 Operator : SY/MD
 Sample : P4329-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD8

Quant Time: Oct 08 04:31:08 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 08 04:30:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	624770	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.777	117	622693	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	298756	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	72590	13.236	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	26.480%#
7) Chloroethane-d5	1.532	69	78270	18.386	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	36.780%#
11) 1,1-Dichloroethene-d2	2.060	65	32290	14.092	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	28.180%#
21) 2-Butanone-d5	3.790	46	147684	75.601	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	75.600%
24) Chloroform-d	4.240	84	278946	28.588	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	57.180%#
26) 1,2-Dichloroethane-d4	4.934	65	167338	29.299	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	58.600%#
32) Benzene-d6	4.950	84	392886	20.163	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	40.320%#
36) 1,2-Dichloropropane-d6	5.982	67	168606	27.174	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	54.340%#
41) Toluene-d8	7.236	98	302968	17.147	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	34.300%#
43) trans-1,3-Dichloroprop...	7.551	79	70868	24.587	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	49.180%#
47) 2-Hexanone-d5	8.021	63	79343	60.559	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	60.560%
56) 1,1,2,2-Tetrachloroeth...	10.146	84	259668	36.018	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	72.040%
66) 1,2-Dichlorobenzene-d4	11.551	152	226910	36.044	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	72.080%#
Target Compounds						
13) Acetone	2.111	43	58254	30.420	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037750.D
Acq On : 07 Oct 2024 10:33
Operator : SY/MD
Sample : P4329-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD8

Quant Time: Oct 08 04:31:08 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 08 04:30:01 2024
Response via : Initial Calibration

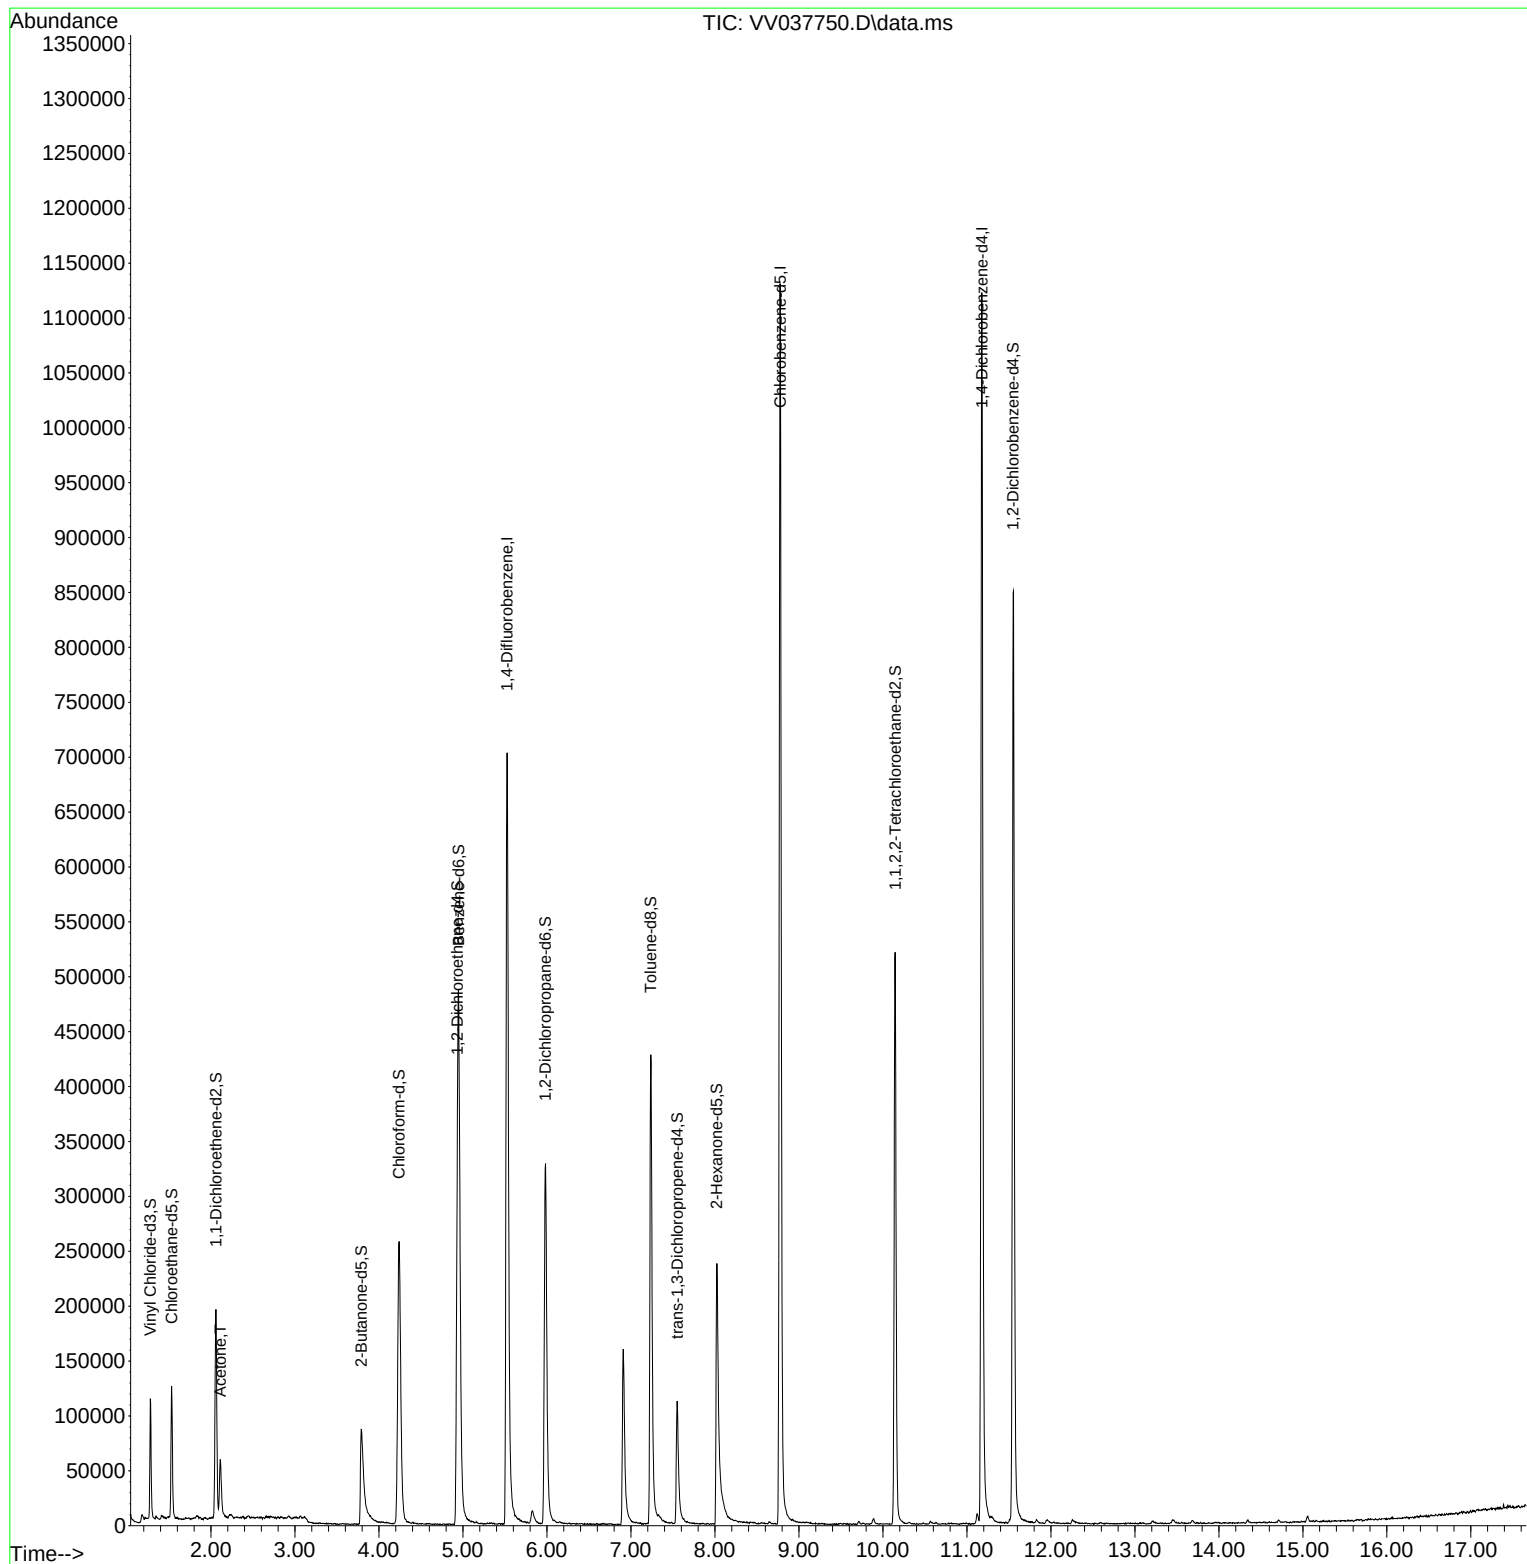

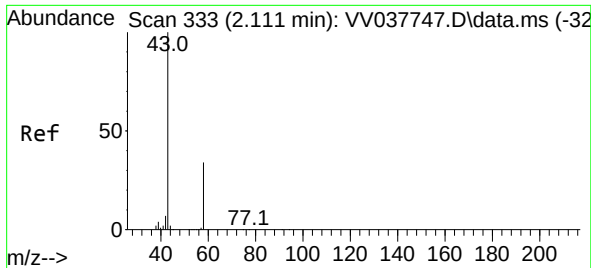

#13

Acetone

Concen: 30.420 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV037750.D

Acq: 07 Oct 2024 10:33

Instrument :

MSVOA_V

ClientSampleId :

A4FD8

Tgt Ion: 43 Resp: 58254

Ion Ratio Lower Upper

43 100

58 32.6 0.0 66.6

