

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037751.D
 Acq On : 07 Oct 2024 11:37
 Operator : SY/MD
 Sample : P4329-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD8

Quant Time: Oct 08 04:31:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Tue Oct 08 04:30:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	609253	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	595962	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	284616	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	241992	45.247	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	90.500%		
7) Chloroethane-d5	1.532	69	203257	48.961	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	97.920%		
11) 1,1-Dichloroethene-d2	2.056	65	107948	48.311	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	96.620%		
21) 2-Butanone-d5	3.789	46	170213	89.353	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	89.350%		
24) Chloroform-d	4.236	84	468064	49.191	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.380%		
26) 1,2-Dichloroethane-d4	4.931	65	279718	50.223	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	100.440%		
32) Benzene-d6	4.950	84	910634	48.831	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.660%		
36) 1,2-Dichloropropane-d6	5.979	67	292552	49.265	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.520%		
41) Toluene-d8	7.236	98	789616	46.695	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	93.380%		
43) trans-1,3-Dichloroprop...	7.548	79	124518	45.138	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.280%		
47) 2-Hexanone-d5	8.024	63	95332	76.026	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	76.030%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	306110	44.364	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	88.720%		
66) 1,2-Dichlorobenzene-d4	11.554	152	306175	51.051	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.100%		
Target Compounds					Qvalue	
13) Acetone	2.111	43	58817	31.496	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037751.D
Acq On : 07 Oct 2024 11:37
Operator : SY/MD
Sample : P4329-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD8

Quant Time: Oct 08 04:31:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Tue Oct 08 04:30:01 2024
Response via : Initial Calibration

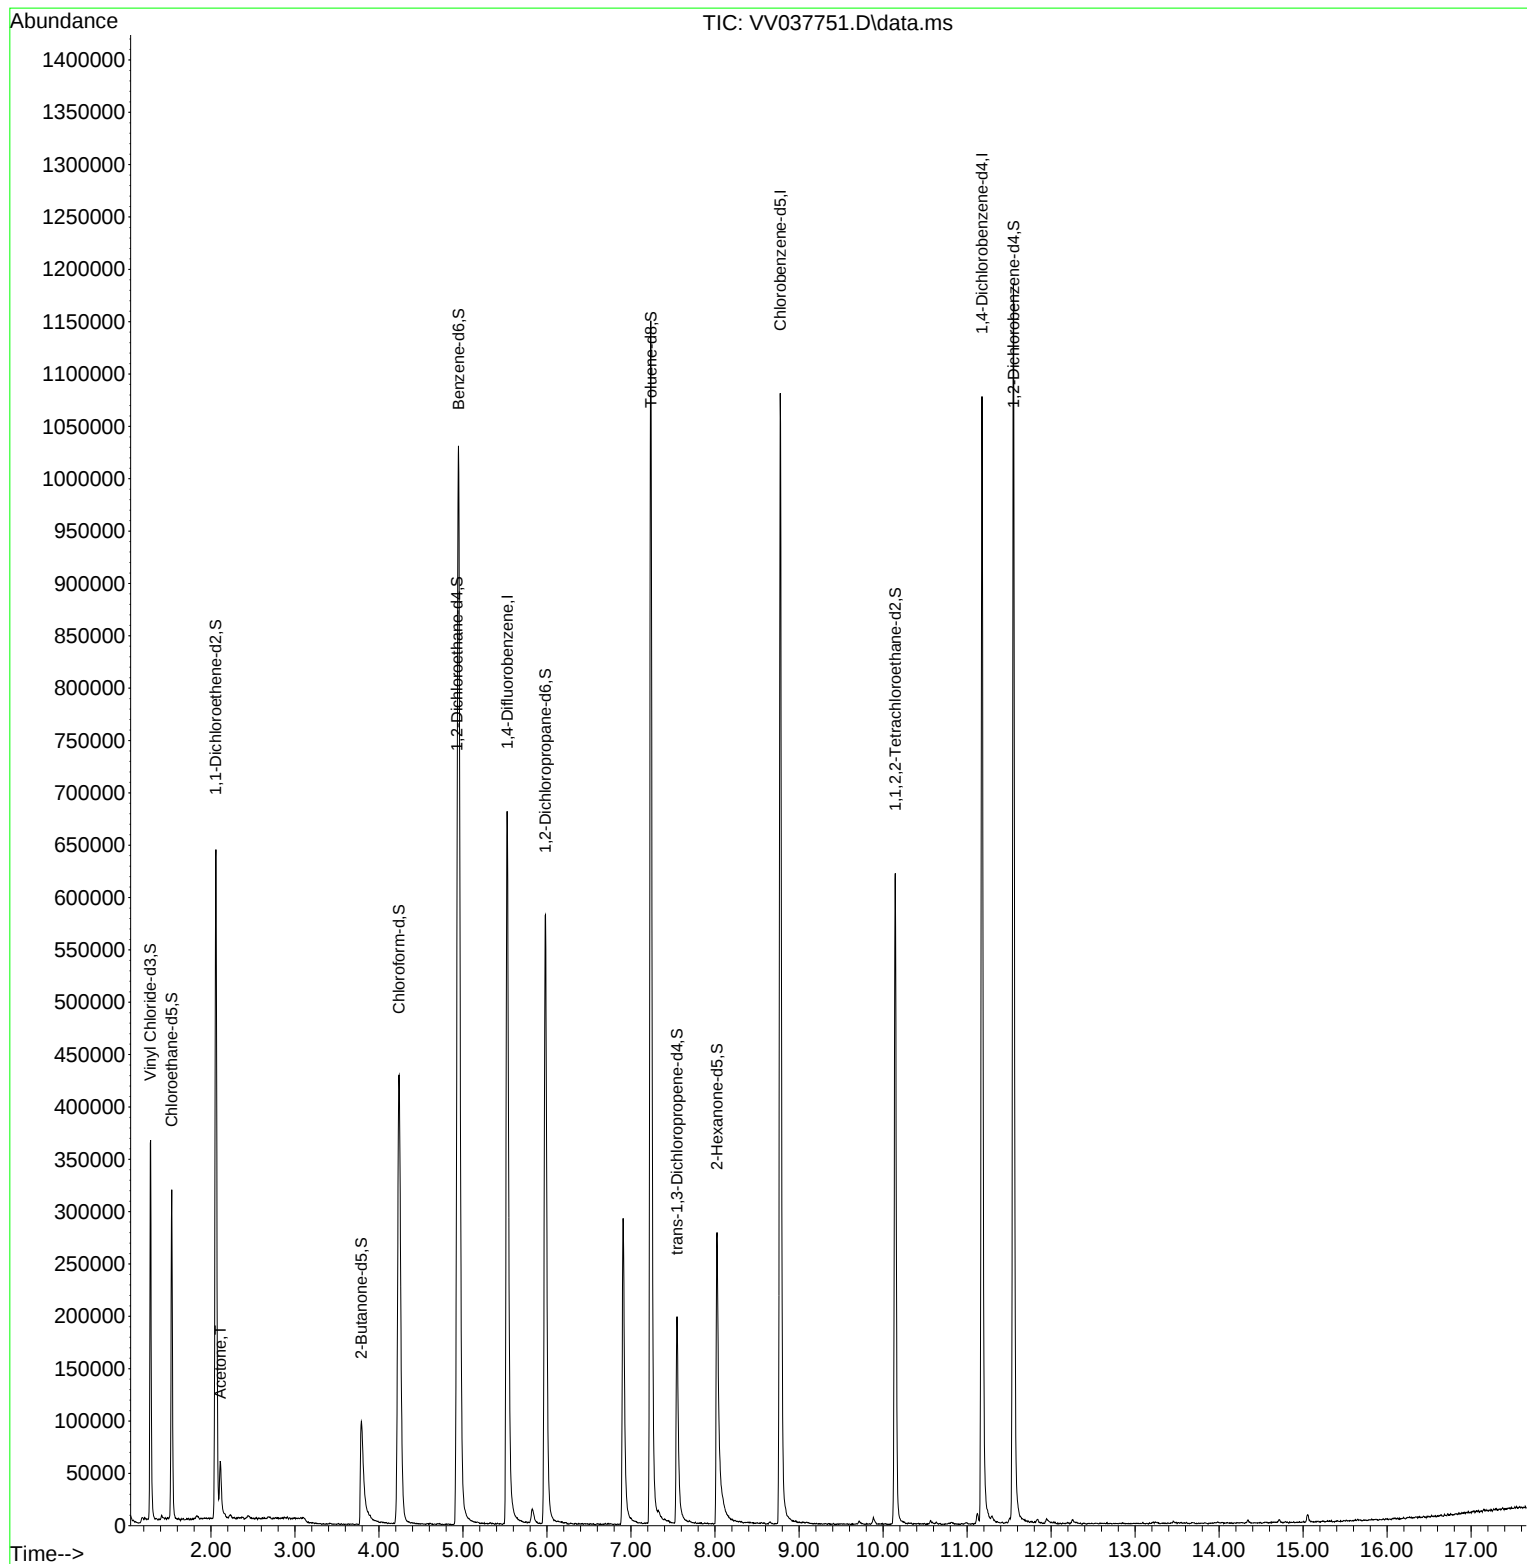

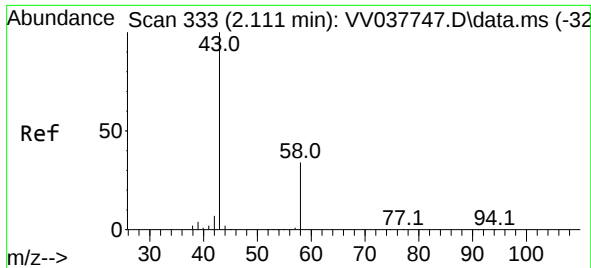

#13

Acetone

Concen: 31.496 ug/L

RT: 2.111 min Scan# 31

Delta R.T. 0.000 min

Lab File: VV037751.D


Acq: 07 Oct 2024 11:37

Instrument :

MSVOA_V

ClientSampleId :

A4FD8

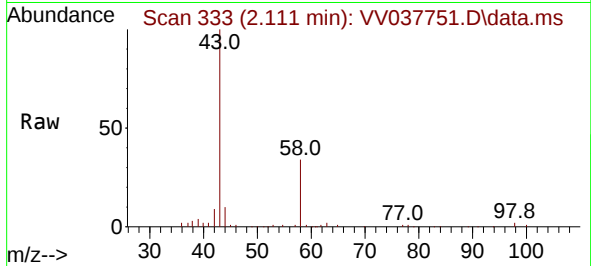

Tgt Ion: 43 Resp: 58817

Ion Ratio Lower Upper

43 100

58 33.4 0.0 66.6

