

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037748.D
 Acq On : 07 Oct 2024 09:35
 Operator : SY/MD
 Sample : VV1007MBL01
 Misc : 5.00g/5mL/100ul/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037748.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.282	68	75	90	rVB	385323	416813	15.06%	2.149%
2	1.532	146	153	171	rVB	328940	386175	13.95%	1.991%
3	2.060	307	317	333	rBV	669886	968906	35.01%	4.996%
4	3.371	722	725	727	rBV2	915	533	0.02%	0.003%
5	3.494	761	763	768	rBV4	612	526	0.02%	0.003%
6	3.539	774	777	779	rVB	553	326	0.01%	0.002%
7	3.693	824	825	831	rVB	527	347	0.01%	0.002%
8	3.719	831	833	836	rBV3	727	359	0.01%	0.002%
9	3.789	846	855	885	rBV2	105963	320423	11.58%	1.652%
10	4.240	978	995	1026	rBV	451747	1154357	41.71%	5.953%
11	4.564	1093	1096	1098	rBV2	1259	739	0.03%	0.004%
12	4.629	1114	1116	1117	rBV2	410	178	0.01%	0.001%
13	4.664	1126	1127	1128	rBV2	242	71	0.00%	0.000%
14	4.674	1128	1130	1132	rVV3	414	226	0.01%	0.001%
15	4.696	1135	1137	1140	rBV2	614	429	0.02%	0.002%
16	4.764	1153	1158	1160	rBV3	547	380	0.01%	0.002%
17	4.777	1160	1162	1164	rVB	423	155	0.01%	0.001%
18	4.841	1179	1182	1184	rBV2	572	394	0.01%	0.002%
19	4.947	1195	1215	1248	rBV2	1082294	2767602	100.00%	14.271%
20	5.439	1365	1368	1371	rBV5	835	463	0.02%	0.002%
21	5.526	1384	1395	1428	rBV	699430	1453458	52.52%	7.495%
22	5.982	1523	1537	1566	rBV	604085	1267605	45.80%	6.536%
23	6.378	1658	1660	1662	rBV3	337	171	0.01%	0.001%
24	6.391	1662	1664	1666	rVV3	549	200	0.01%	0.001%
25	6.429	1673	1676	1679	rBV5	1005	698	0.03%	0.004%
26	6.494	1691	1696	1701	rVB5	934	877	0.03%	0.005%
27	6.522	1701	1705	1708	rBV4	1195	972	0.04%	0.005%
28	6.561	1714	1717	1718	rBV3	416	216	0.01%	0.001%
29	6.612	1731	1733	1734	rVB2	497	155	0.01%	0.001%
30	6.625	1734	1737	1740	rBV3	376	257	0.01%	0.001%
31	6.641	1740	1742	1745	rVV4	486	366	0.01%	0.002%
32	6.658	1745	1747	1750	rVB3	1128	594	0.02%	0.003%
33	6.677	1751	1753	1755	rBV2	569	277	0.01%	0.001%
34	6.731	1768	1770	1772	rBV3	633	325	0.01%	0.002%
35	6.802	1789	1792	1793	rBV2	262	122	0.00%	0.001%
36	6.828	1797	1800	1804	rBV2	561	545	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037748.D
 Acq On : 07 Oct 2024 09:35
 Operator : SY/MD
 Sample : VV1007MBL01
 Misc : 5.00g/5mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.854	1807	1808	1812	rVB3	590	309	0.01%	0.002%
38	6.905	1813	1824	1853	rBV	311772	604094	21.83%	3.115%
39	7.236	1916	1927	1963	rBV	1243957	2194701	79.30%	11.317%
40	7.548	2015	2024	2048	rBV	207818	389414	14.07%	2.008%
41	8.024	2163	2172	2211	rBV2	298250	676320	24.44%	3.487%
42	8.474	2307	2312	2316	rVB5	1259	1228	0.04%	0.006%
43	8.638	2361	2363	2366	rVB3	577	335	0.01%	0.002%
44	8.683	2375	2377	2378	rBV	853	377	0.01%	0.002%
45	8.725	2387	2390	2392	rBV3	730	445	0.02%	0.002%
46	8.776	2395	2406	2433	rBV	1095557	1833622	66.25%	9.455%
47	9.169	2525	2528	2530	rBV4	1039	676	0.02%	0.003%
48	9.265	2556	2558	2561	rVB4	781	376	0.01%	0.002%
49	9.294	2563	2567	2569	rBV2	597	376	0.01%	0.002%
50	9.317	2572	2574	2576	rBV3	800	441	0.02%	0.002%
51	9.374	2588	2592	2596	rVB5	548	532	0.02%	0.003%
52	9.394	2596	2598	2599	rBV	317	105	0.00%	0.001%
53	9.442	2610	2613	2616	rVB4	1223	741	0.03%	0.004%
54	9.474	2616	2623	2624	rBV2	2106	1492	0.05%	0.008%
55	9.580	2653	2656	2659	rBV4	708	542	0.02%	0.003%
56	9.612	2664	2666	2668	rBV3	529	258	0.01%	0.001%
57	9.670	2680	2684	2687	rBV5	724	656	0.02%	0.003%
58	9.754	2704	2710	2714	rBV4	896	983	0.04%	0.005%
59	9.770	2714	2715	2716	rBV4	320	65	0.00%	0.000%
60	9.783	2716	2719	2723	rBV3	338	265	0.01%	0.001%
61	9.818	2727	2730	2732	rBV3	514	282	0.01%	0.001%
62	9.866	2738	2745	2753	rBV7	2889	4735	0.17%	0.024%
63	9.972	2776	2778	2780	rBV2	389	219	0.01%	0.001%
64	10.017	2790	2792	2796	rVB4	479	329	0.01%	0.002%
65	10.072	2808	2809	2810	rBV	384	115	0.00%	0.001%
66	10.095	2814	2816	2817	rBV3	483	134	0.00%	0.001%
67	10.146	2820	2832	2855	rBV	649987	1060361	38.31%	5.468%
68	10.445	2922	2925	2926	rBV2	456	268	0.01%	0.001%
69	10.481	2931	2936	2945	rVV7	2557	3586	0.13%	0.018%
70	10.519	2947	2948	2951	rVB3	760	308	0.01%	0.002%
71	10.564	2958	2962	2963	rBV2	442	338	0.01%	0.002%
72	10.574	2963	2965	2967	rVB2	580	210	0.01%	0.001%
73	10.603	2972	2974	2976	rBV	270	88	0.00%	0.000%
74	10.619	2976	2979	2983	rVB4	684	614	0.02%	0.003%
75	10.654	2988	2990	2991	rBV	432	210	0.01%	0.001%
76	10.741	3015	3017	3020	rBV2	347	213	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037748.D
Acq On : 07 Oct 2024 09:35
Operator : SY/MD
Sample : VV1007MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	10.763	3020	3024	3025	rVV3	218	147	0.01%	0.001%
78	10.780	3025	3029	3039	rVV7	1233	1750	0.06%	0.009%
79	10.847	3046	3050	3051	rBV4	1295	937	0.03%	0.005%
80	10.934	3075	3077	3079	rBV	584	187	0.01%	0.001%
81	10.985	3090	3093	3094	rBV2	630	328	0.01%	0.002%
82	10.995	3094	3096	3099	rVB2	556	322	0.01%	0.002%
83	11.091	3122	3126	3130	rBV4	697	627	0.02%	0.003%
84	11.130	3130	3138	3142	rBV7	6057	9688	0.35%	0.050%
85	11.178	3143	3153	3178	rVV	1069457	1705917	61.64%	8.797%
86	11.554	3258	3270	3297	rBV	1217608	1980200	71.55%	10.211%
87	12.355	3517	3519	3521	rBV2	963	535	0.02%	0.003%
88	12.448	3545	3548	3550	rVB2	636	301	0.01%	0.002%
89	12.532	3570	3574	3578	rBV4	455	486	0.02%	0.003%
90	12.587	3580	3591	3601	rBV3	9861	17409	0.63%	0.090%
91	12.767	3644	3647	3653	rVB4	723	721	0.03%	0.004%
92	12.796	3653	3656	3657	rBV2	689	343	0.01%	0.002%
93	12.921	3691	3695	3697	rBV4	1086	880	0.03%	0.005%
94	13.033	3726	3730	3733	rBV5	942	795	0.03%	0.004%
95	13.053	3734	3736	3740	rBV4	742	436	0.02%	0.002%
96	13.201	3774	3782	3792	rBV4	17270	29165	1.05%	0.150%
97	13.442	3848	3857	3874	rBV2	40358	76102	2.75%	0.392%
98	13.680	3923	3931	3945	rVB2	23816	38847	1.40%	0.200%




Sum of corrected areas: 19392726

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037748.D
Acq On : 07 Oct 2024 09:35
Operator : SY/MD
Sample : VV1007MBL01
Misc : 5.00g/5mL/100ul/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

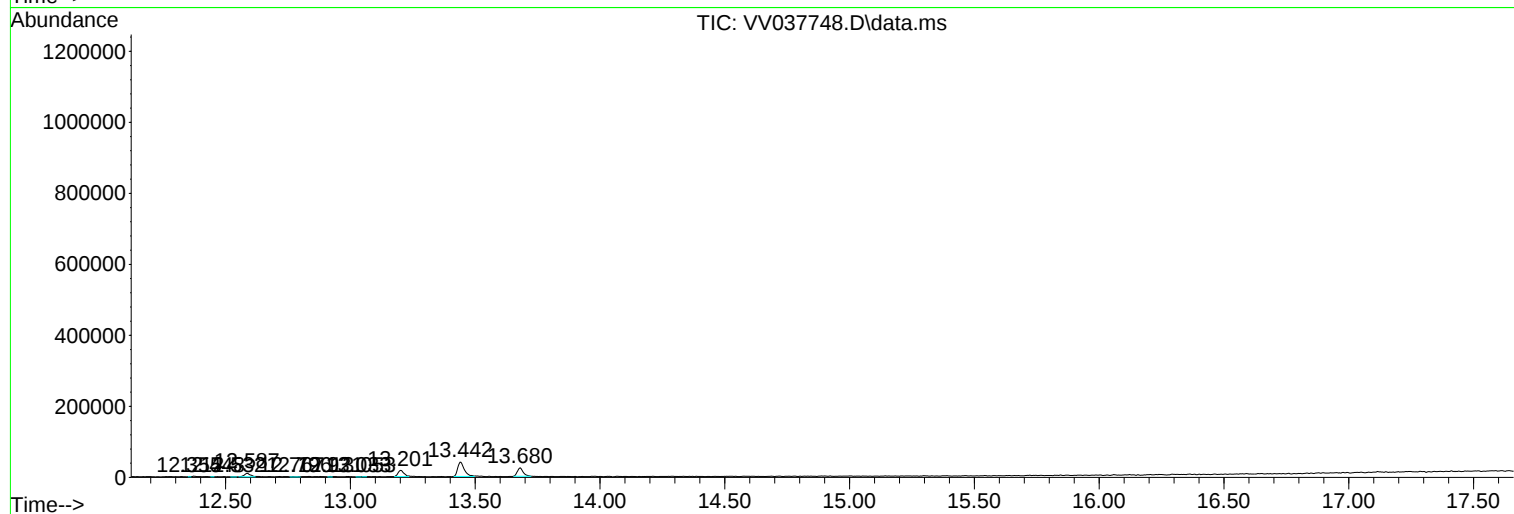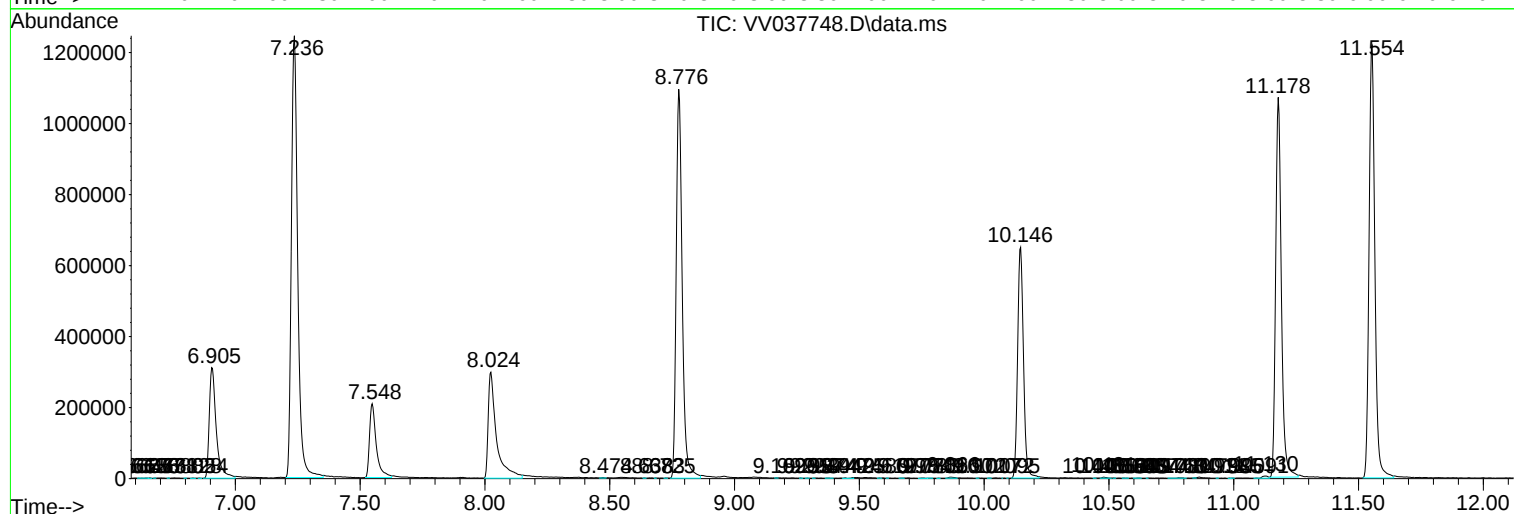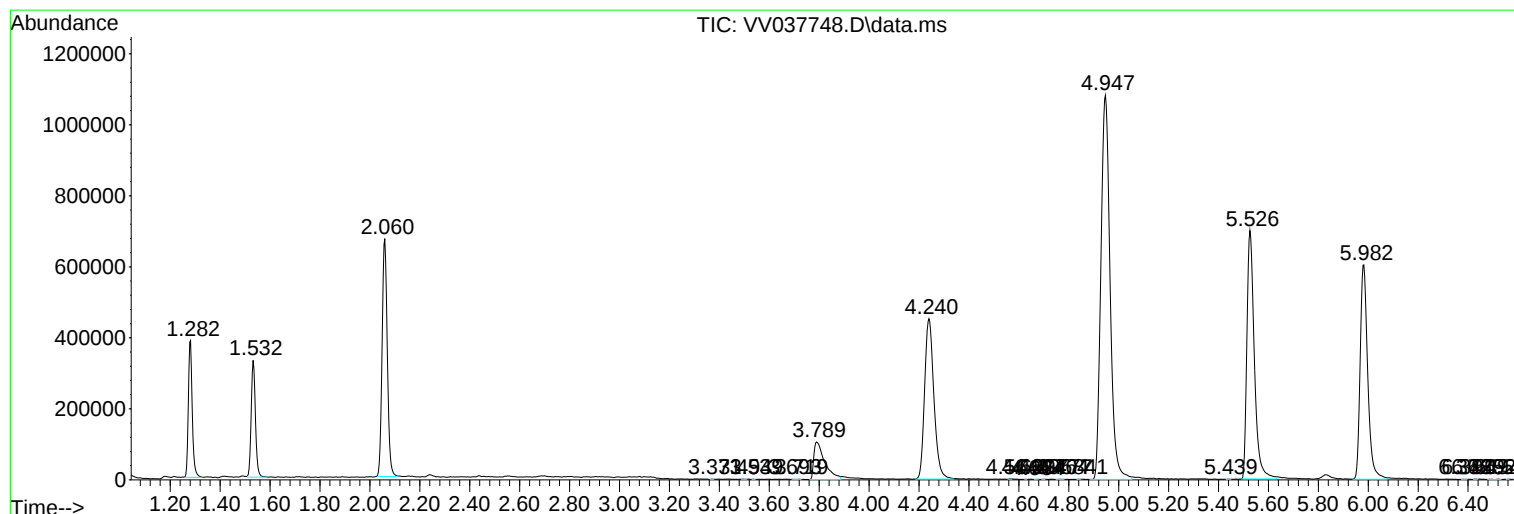

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037748.D
Acq On : 07 Oct 2024 09:35
Operator : SY/MD
Sample : VV1007MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037748.D
Acq On : 07 Oct 2024 09:35
Operator : SY/MD
Sample : VV1007MBL01
Misc : 5.00g/5mL/100ul/5ml/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc