

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037749.D
 Acq On : 07 Oct 2024 09:56
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037749.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	27	29	31	rBV2	827	477	0.02%	0.002%
2	1.182	37	44	47	rBV3	4945	6730	0.25%	0.035%
3	1.278	67	74	90	rBV	357743	389360	14.48%	2.007%
4	1.532	145	153	167	rVB	310975	365828	13.60%	1.886%
5	1.880	259	261	264	rBV3	1912	1116	0.04%	0.006%
6	2.060	307	317	338	rBV	645787	927050	34.47%	4.778%
7	2.317	395	397	402	rBV5	2233	1827	0.07%	0.009%
8	3.439	742	746	751	rBV6	498	453	0.02%	0.002%
9	3.529	770	774	776	rBV3	629	429	0.02%	0.002%
10	3.793	847	856	900	rBV	112199	339158	12.61%	1.748%
11	4.163	969	971	975	rVB	756	429	0.02%	0.002%
12	4.243	980	996	1025	rVV	438887	1110788	41.31%	5.725%
13	4.465	1063	1065	1069	rVB4	701	523	0.02%	0.003%
14	4.500	1075	1076	1082	rVB4	588	481	0.02%	0.002%
15	4.555	1090	1093	1096	rVV2	828	704	0.03%	0.004%
16	4.584	1100	1102	1108	rVB5	548	430	0.02%	0.002%
17	4.645	1117	1121	1125	rBV3	834	681	0.03%	0.004%
18	4.770	1154	1160	1165	rVB5	929	1224	0.05%	0.006%
19	4.835	1176	1180	1183	rVB4	576	461	0.02%	0.002%
20	4.950	1199	1216	1251	rBV2	1038446	2689130	100.00%	13.861%
21	5.294	1321	1323	1325	rBV3	822	554	0.02%	0.003%
22	5.330	1331	1334	1337	rBV5	827	636	0.02%	0.003%
23	5.429	1362	1365	1369	rVB5	755	620	0.02%	0.003%
24	5.529	1385	1396	1432	rBV	753400	1569339	58.36%	8.089%
25	5.835	1476	1491	1513	rVB4	12240	30285	1.13%	0.156%
26	5.982	1522	1537	1576	rBV	592611	1244466	46.28%	6.414%
27	6.481	1689	1692	1696	rVB3	938	634	0.02%	0.003%
28	6.516	1698	1703	1705	rBV5	657	476	0.02%	0.002%
29	6.545	1710	1712	1715	rVB2	778	449	0.02%	0.002%
30	6.571	1715	1720	1721	rBV3	741	453	0.02%	0.002%
31	6.609	1728	1732	1738	rBV4	612	674	0.03%	0.003%
32	6.642	1738	1742	1744	rVB2	728	572	0.02%	0.003%
33	6.667	1744	1750	1754	rBV4	713	869	0.03%	0.004%
34	6.741	1767	1773	1777	rBV5	1192	1200	0.04%	0.006%
35	6.767	1777	1781	1789	rVB7	1215	1554	0.06%	0.008%
36	6.825	1797	1799	1804	rVB3	640	432	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037749.D
 Acq On : 07 Oct 2024 09:56
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.851	1804	1807	1812	rVB2	843	764	0.03%	0.004%
38	6.908	1812	1825	1849	rBV	305271	585417	21.77%	3.017%
39	7.236	1916	1927	1967	rBV	1192047	2129282	79.18%	10.975%
40	7.548	2015	2024	2050	rBV	208683	379471	14.11%	1.956%
41	7.841	2112	2115	2119	rVB4	1053	675	0.03%	0.003%
42	7.860	2119	2121	2126	rBV5	585	429	0.02%	0.002%
43	7.912	2133	2137	2140	rBV6	989	968	0.04%	0.005%
44	7.969	2152	2155	2158	rVB2	869	558	0.02%	0.003%
45	8.024	2163	2172	2215	rBV2	317691	717624	26.69%	3.699%
46	8.384	2282	2284	2288	rVB2	984	525	0.02%	0.003%
47	8.622	2355	2358	2361	rBV3	889	569	0.02%	0.003%
48	8.674	2368	2374	2376	rBV4	955	1050	0.04%	0.005%
49	8.777	2391	2406	2439	rBV	1161656	1975193	73.45%	10.181%
50	9.050	2486	2491	2492	rBV4	1159	987	0.04%	0.005%
51	9.214	2536	2542	2545	rVB5	600	561	0.02%	0.003%
52	9.384	2592	2595	2600	rBV5	725	553	0.02%	0.003%
53	9.426	2603	2608	2610	rBV4	593	542	0.02%	0.003%
54	9.484	2623	2626	2629	rBV3	782	546	0.02%	0.003%
55	9.500	2629	2631	2634	rBV	682	444	0.02%	0.002%
56	9.551	2644	2647	2652	rVB5	1096	947	0.04%	0.005%
57	9.632	2670	2672	2677	rVB4	811	631	0.02%	0.003%
58	9.677	2684	2686	2692	rVB4	736	738	0.03%	0.004%
59	9.712	2692	2697	2699	rBV4	987	833	0.03%	0.004%
60	9.741	2703	2706	2709	rBV2	678	472	0.02%	0.002%
61	9.805	2721	2726	2727	rBV3	600	454	0.02%	0.002%
62	9.908	2756	2758	2761	rVB2	858	474	0.02%	0.002%
63	10.005	2784	2788	2791	rBV3	475	451	0.02%	0.002%
64	10.047	2796	2801	2806	rVB8	769	849	0.03%	0.004%
65	10.085	2810	2813	2816	rVB2	952	482	0.02%	0.002%
66	10.146	2819	2832	2861	rBV	678013	1089425	40.51%	5.615%
67	10.317	2882	2885	2889	rBV5	803	680	0.03%	0.004%
68	10.558	2958	2960	2965	rVV4	655	638	0.02%	0.003%
69	10.751	3015	3020	3024	rBV4	795	856	0.03%	0.004%
70	10.786	3027	3031	3036	rVB5	1785	1784	0.07%	0.009%
71	10.899	3065	3066	3072	rVB2	680	583	0.02%	0.003%
72	11.088	3123	3125	3128	rBV3	626	500	0.02%	0.003%
73	11.127	3130	3137	3142	rBV6	2648	3321	0.12%	0.017%
74	11.178	3142	3153	3180	rBV	1150379	1827043	67.94%	9.417%
75	11.448	3233	3237	3240	rBV5	500	531	0.02%	0.003%
76	11.551	3256	3269	3301	rBV	1170206	1931842	71.84%	9.957%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037749.D
 Acq On : 07 Oct 2024 09:56
 Operator : SY/MD
 Sample : VV1007WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK233

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.018	3411	3414	3417	rVB4	1003	636	0.02%	0.003%
78	12.056	3423	3426	3432	rBV5	1277	1284	0.05%	0.007%
79	12.117	3440	3445	3447	rBV4	803	704	0.03%	0.004%
80	12.275	3492	3494	3499	rVB4	802	544	0.02%	0.003%
81	12.378	3523	3526	3531	rVB3	713	572	0.02%	0.003%
82	12.455	3544	3550	3553	rVB5	865	904	0.03%	0.005%
83	12.519	3567	3570	3572	rVB3	845	423	0.02%	0.002%
84	12.593	3587	3593	3599	rVV8	2143	3124	0.12%	0.016%
85	12.673	3615	3618	3623	rVB2	989	749	0.03%	0.004%
86	12.696	3623	3625	3629	rBV2	709	634	0.02%	0.003%
87	12.863	3673	3677	3679	rBV5	619	441	0.02%	0.002%
88	13.069	3737	3741	3745	rBV2	708	707	0.03%	0.004%
89	13.210	3777	3785	3797	rBV8	4040	7738	0.29%	0.040%
90	13.268	3800	3803	3807	rVB4	1040	773	0.03%	0.004%
91	13.291	3808	3810	3814	rVB5	629	470	0.02%	0.002%
92	13.448	3850	3859	3874	rBV2	8766	18564	0.69%	0.096%
93	13.686	3925	3933	3944	rBV9	4892	8564	0.32%	0.044%
94	13.847	3980	3983	3988	rVB3	830	664	0.02%	0.003%
95	13.931	4006	4009	4012	rBV2	740	530	0.02%	0.003%
96	14.021	4035	4037	4041	rBV4	732	494	0.02%	0.003%
97	14.046	4041	4045	4047	rVV4	865	643	0.02%	0.003%
98	14.188	4086	4089	4090	rBV3	700	489	0.02%	0.003%
99	14.455	4169	4172	4173	rBV2	874	435	0.02%	0.002%
100	15.201	4401	4404	4406	rBV3	1128	715	0.03%	0.004%




Sum of corrected areas: 19400985

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037749.D
Acq On : 07 Oct 2024 09:56
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

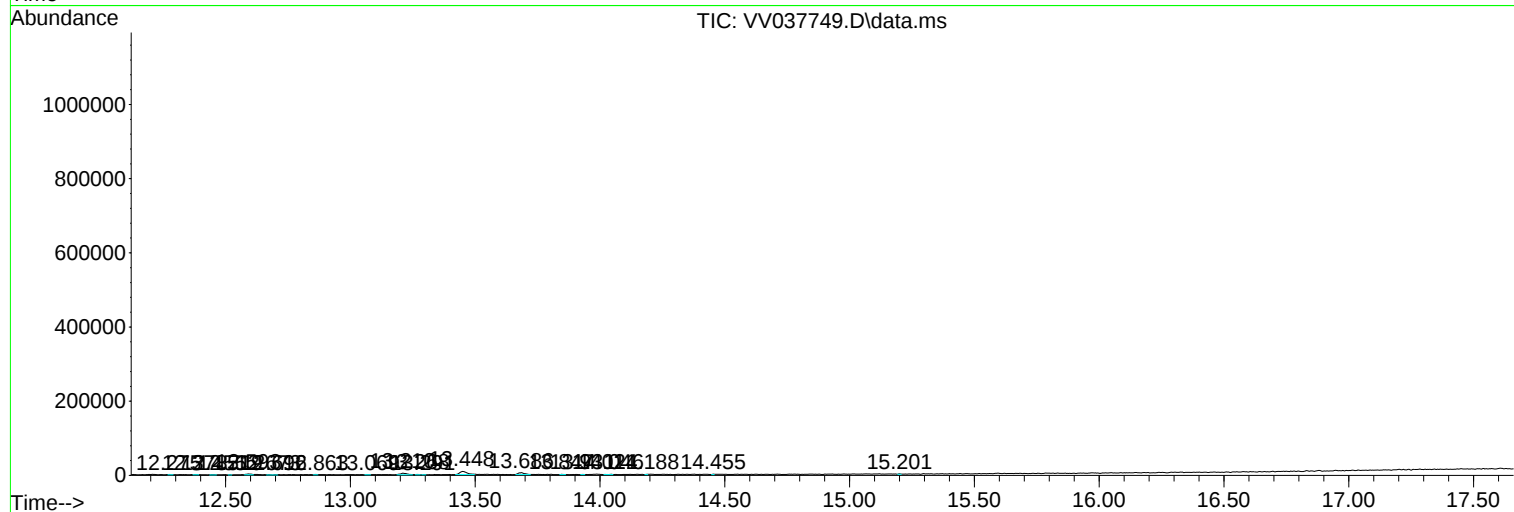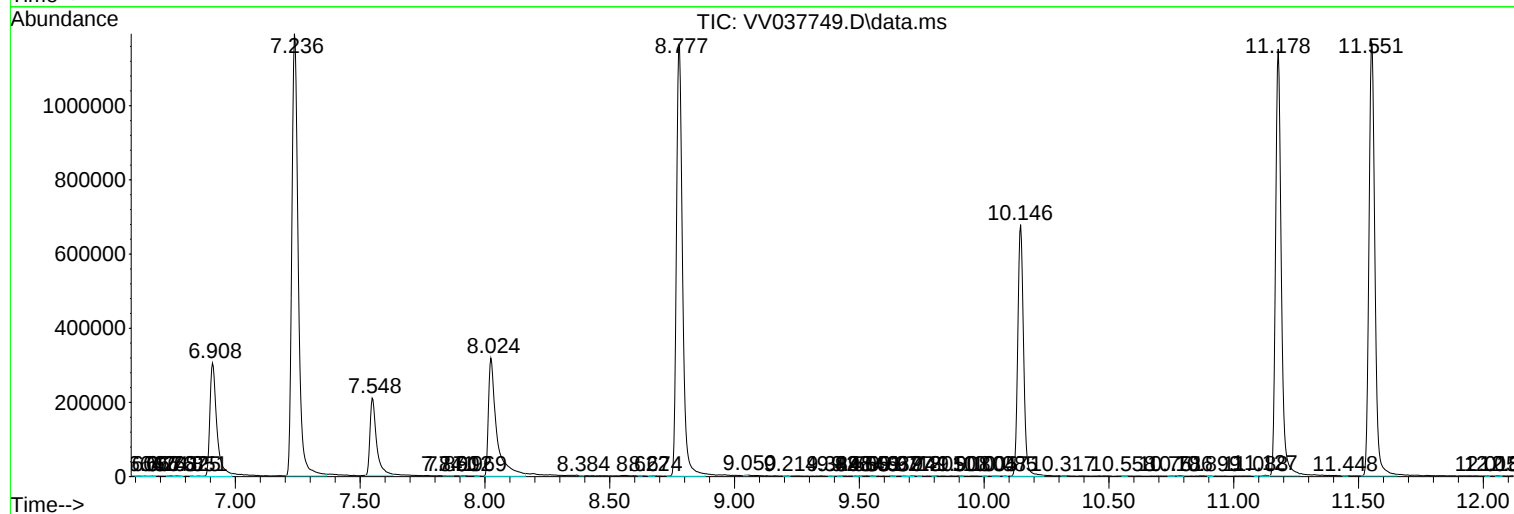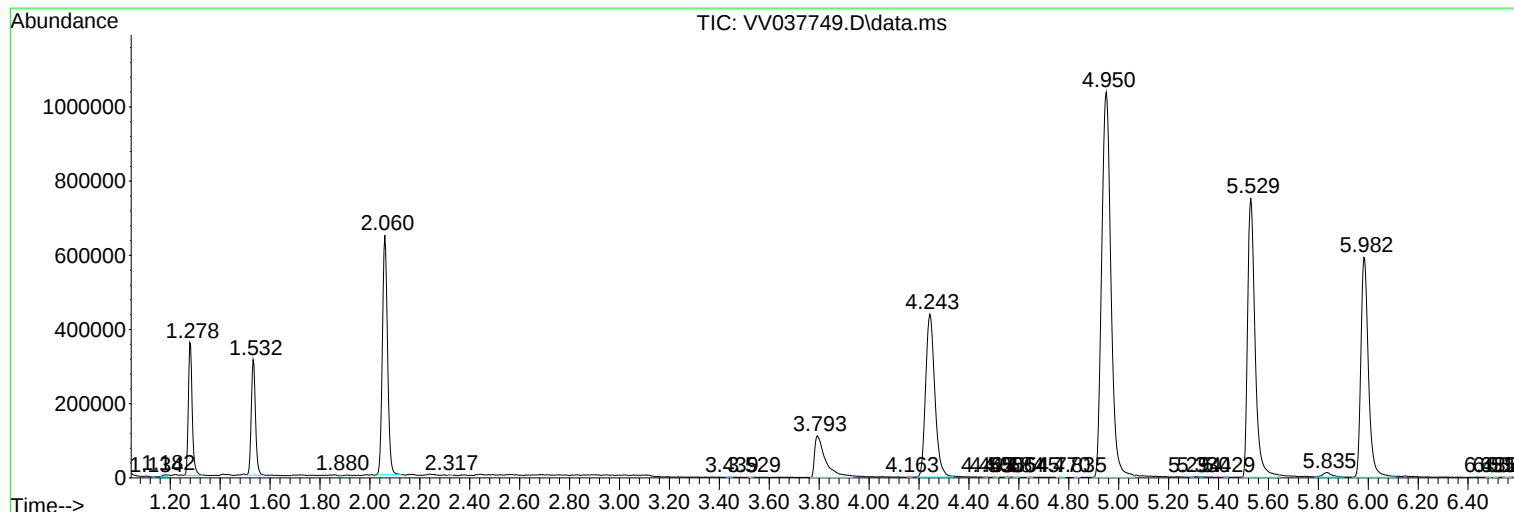

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037749.D
Acq On : 07 Oct 2024 09:56
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037749.D
Acq On : 07 Oct 2024 09:56
Operator : SY/MD
Sample : VV1007WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK233

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------