

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037754.D
 Acq On : 07 Oct 2024 13:48
 Operator : SY/MD
 Sample : P4239-11ME
 Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ET5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037754.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	95	rVB	162095	220464	10.84%	1.357%
2	2.043	303	312	330	rVB	354712	518206	25.48%	3.190%
3	3.439	744	746	749	rVB2	602	183	0.01%	0.001%
4	3.455	749	751	754	rBV2	529	329	0.02%	0.002%
5	3.487	759	761	762	rBV	435	114	0.01%	0.001%
6	3.580	786	790	792	rBV3	618	481	0.02%	0.003%
7	3.645	806	810	816	rVB5	921	887	0.04%	0.005%
8	3.674	816	819	822	rBV3	687	511	0.03%	0.003%
9	3.725	831	835	837	rVB3	424	278	0.01%	0.002%
10	3.738	837	839	840	rVB	169	57	0.00%	0.000%
11	3.748	840	842	844	rBV2	290	121	0.01%	0.001%
12	3.760	844	846	850	rBV3	441	358	0.02%	0.002%
13	3.802	850	859	876	rBV2	76203	220827	10.86%	1.359%
14	4.240	980	995	1019	rBV	353804	920909	45.28%	5.669%
15	4.551	1089	1092	1093	rBV2	655	339	0.02%	0.002%
16	4.580	1099	1101	1103	rBV3	483	226	0.01%	0.001%
17	4.670	1123	1129	1132	rBV5	1213	1056	0.05%	0.007%
18	4.738	1148	1150	1151	rBV2	325	168	0.01%	0.001%
19	4.793	1164	1167	1170	rVB2	399	242	0.01%	0.001%
20	4.809	1170	1172	1175	rBV3	622	373	0.02%	0.002%
21	4.831	1178	1179	1180	rBV	258	64	0.00%	0.000%
22	4.857	1185	1187	1191	rBV2	575	329	0.02%	0.002%
23	4.889	1194	1197	1199	rBV2	662	381	0.02%	0.002%
24	4.944	1199	1214	1264	rBV2	747738	2033593	100.00%	12.519%
25	5.526	1384	1395	1440	rBV	617114	1398903	68.79%	8.612%
26	5.982	1525	1537	1575	rBV	452315	1028051	50.55%	6.329%
27	6.320	1641	1642	1646	rBV4	779	363	0.02%	0.002%
28	6.339	1646	1648	1652	rBV3	433	338	0.02%	0.002%
29	6.362	1653	1655	1656	rVV2	489	150	0.01%	0.001%
30	6.448	1678	1682	1684	rBV4	625	518	0.03%	0.003%
31	6.513	1700	1702	1705	rVB3	702	401	0.02%	0.002%
32	6.535	1707	1709	1711	rVB2	511	194	0.01%	0.001%
33	6.545	1711	1712	1714	rBV2	336	161	0.01%	0.001%
34	6.574	1718	1721	1723	rBV4	773	572	0.03%	0.004%
35	6.632	1736	1739	1745	rVB4	934	939	0.05%	0.006%
36	6.661	1745	1748	1750	rBV3	1116	767	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037754.D
 Acq On : 07 Oct 2024 13:48
 Operator : SY/MD
 Sample : P4239-11ME
 Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ET5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.731	1768	1770	1772	rBV2	458	193	0.01%	0.001%
38	6.821	1794	1798	1802	rBV4	997	841	0.04%	0.005%
39	6.857	1806	1809	1811	rBV2	529	372	0.02%	0.002%
40	6.908	1814	1825	1864	rBV	231049	501269	24.65%	3.086%
41	7.149	1897	1900	1903	rBV5	856	635	0.03%	0.004%
42	7.236	1917	1927	1958	rBV	733092	1400160	68.85%	8.620%
43	7.516	2012	2014	2015	rBV	955	356	0.02%	0.002%
44	7.551	2016	2025	2051	rVV	158907	338126	16.63%	2.082%
45	7.905	2134	2135	2137	rBV2	582	244	0.01%	0.002%
46	8.034	2165	2175	2215	rBV3	271077	871532	42.86%	5.365%
47	8.693	2378	2380	2383	rBV3	635	388	0.02%	0.002%
48	8.712	2384	2386	2390	rVB4	1196	730	0.04%	0.004%
49	8.780	2395	2407	2437	rBV	1009586	1792766	88.16%	11.036%
50	9.246	2547	2552	2554	rBV4	784	610	0.03%	0.004%
51	9.349	2579	2584	2590	rVB7	524	652	0.03%	0.004%
52	9.374	2590	2592	2596	rVB4	350	188	0.01%	0.001%
53	9.394	2596	2598	2600	rBV	273	172	0.01%	0.001%
54	9.471	2620	2622	2624	rBV3	734	352	0.02%	0.002%
55	9.480	2624	2625	2627	rVB	654	144	0.01%	0.001%
56	9.564	2650	2651	2652	rVB	425	82	0.00%	0.001%
57	9.574	2652	2654	2658	rVB3	911	584	0.03%	0.004%
58	9.593	2658	2660	2661	rBV	286	102	0.01%	0.001%
59	9.603	2661	2663	2665	rBV2	409	162	0.01%	0.001%
60	9.619	2665	2668	2672	rBV4	823	554	0.03%	0.003%
61	9.670	2681	2684	2685	rBV	353	159	0.01%	0.001%
62	9.686	2685	2689	2694	rBV6	952	1164	0.06%	0.007%
63	9.709	2694	2696	2698	rVB2	563	201	0.01%	0.001%
64	9.725	2698	2701	2702	rBV	690	428	0.02%	0.003%
65	9.799	2721	2724	2727	rBV3	752	543	0.03%	0.003%
66	9.857	2740	2742	2744	rBV3	383	194	0.01%	0.001%
67	9.873	2744	2747	2748	rBV	665	325	0.02%	0.002%
68	9.937	2765	2767	2769	rVB	237	104	0.01%	0.001%
69	9.969	2771	2777	2779	rBV4	564	640	0.03%	0.004%
70	10.027	2792	2795	2796	rBV	447	273	0.01%	0.002%
71	10.146	2820	2832	2854	rBV	742211	1211468	59.57%	7.458%
72	10.458	2923	2929	2933	rBV3	1111	1223	0.06%	0.008%
73	10.480	2933	2936	2938	rBV3	720	436	0.02%	0.003%
74	10.670	2993	2995	3002	rBV5	550	593	0.03%	0.004%
75	10.725	3009	3012	3016	rVB4	689	566	0.03%	0.003%
76	10.754	3016	3021	3022	rBV3	637	516	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037754.D
 Acq On : 07 Oct 2024 13:48
 Operator : SY/MD
 Sample : P4239-11ME
 Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4ET5ME

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

77	10.937	3076	3078	3082	rVB3	571	346	0.02%	0.002%
78	10.979	3086	3091	3094	rVB3	853	676	0.03%	0.004%
79	10.998	3094	3097	3099	rBV3	624	399	0.02%	0.002%
80	11.021	3102	3104	3106	rBV2	336	199	0.01%	0.001%
81	11.056	3113	3115	3117	rBV3	682	365	0.02%	0.002%
82	11.114	3130	3133	3134	rBV3	501	299	0.01%	0.002%
83	11.178	3142	3153	3186	rBV	1088045	1754596	86.28%	10.801%
84	11.509	3254	3256	3257	rBV2	564	227	0.01%	0.001%
85	11.554	3258	3270	3294	rBV	1245385	1994736	98.09%	12.280%
86	12.162	3457	3459	3460	rBV	590	224	0.01%	0.001%
87	12.188	3461	3467	3476	rVB4	4463	6685	0.33%	0.041%
88	12.982	3711	3714	3719	rBV4	1117	967	0.05%	0.006%
89	13.091	3745	3748	3751	rBV2	675	527	0.03%	0.003%
90	13.831	3974	3978	3981	rBV4	1290	1228	0.06%	0.008%
91	14.223	4098	4100	4103	rBV2	1059	668	0.03%	0.004%




Sum of corrected areas: 16244042

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037754.D
Acq On : 07 Oct 2024 13:48
Operator : SY/MD
Sample : P4239-11ME
Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4ET5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

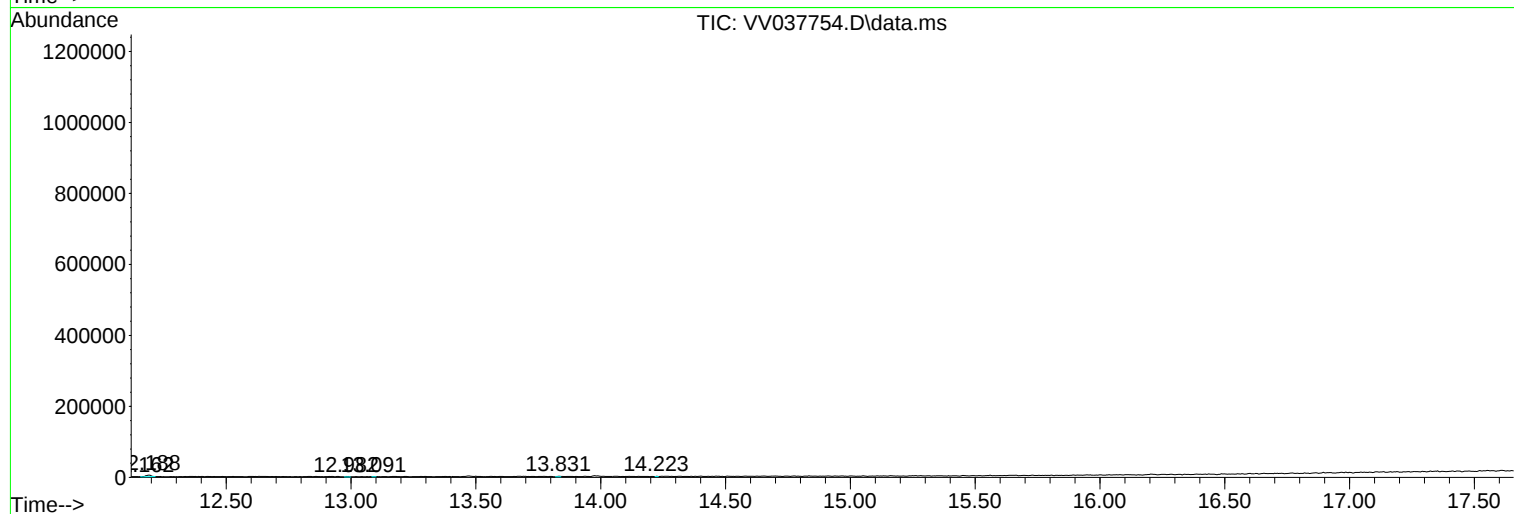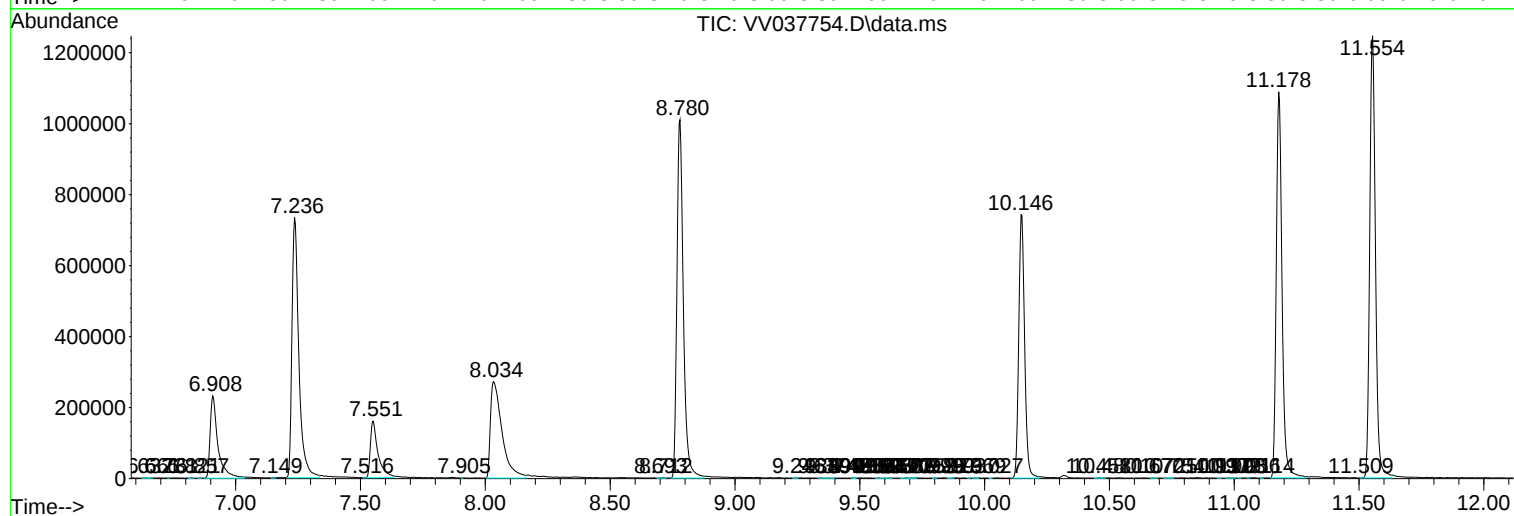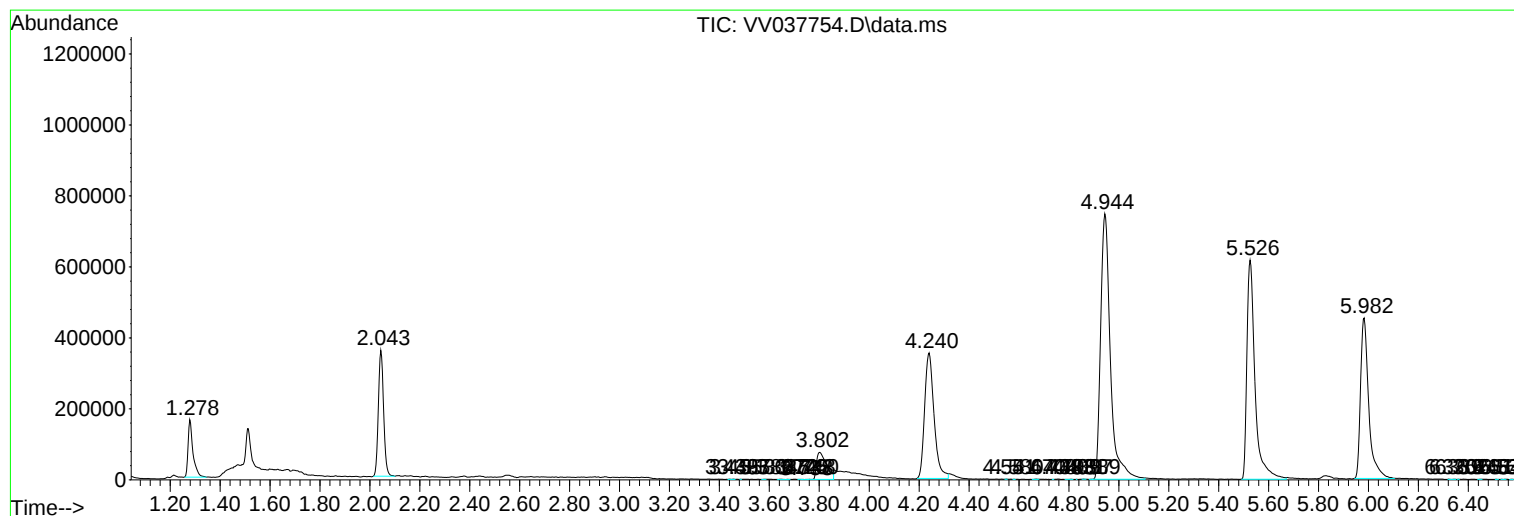

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037754.D
Acq On : 07 Oct 2024 13:48
Operator : SY/MD
Sample : P4239-11ME
Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4ET5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037754.D
Acq On : 07 Oct 2024 13:48
Operator : SY/MD
Sample : P4239-11ME
Misc : 4.19G/5.0mL/100uL/5mL/MSVOA_V/MEOH
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4ET5ME

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
