

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037755.D
 Acq On : 07 Oct 2024 14:23
 Operator : SY/MD
 Sample : VIBLK201
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037755.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	51	rBV3	7184	12782	0.50%	0.071%
2	1.281	67	75	92	rVB	359541	389010	15.33%	2.173%
3	1.532	145	153	166	rVB	297659	346581	13.65%	1.936%
4	2.060	306	317	340	rBV	622338	908295	35.78%	5.073%
5	2.796	544	546	550	rVB4	2372	1005	0.04%	0.006%
6	3.243	683	685	688	rVB3	961	498	0.02%	0.003%
7	3.365	720	723	728	rVB3	749	685	0.03%	0.004%
8	3.407	734	736	742	rBV6	699	570	0.02%	0.003%
9	3.523	768	772	774	rBV2	941	718	0.03%	0.004%
10	3.645	807	810	812	rBV	728	523	0.02%	0.003%
11	3.696	822	826	831	rVB4	795	659	0.03%	0.004%
12	3.793	847	856	891	rBV	98406	300764	11.85%	1.680%
13	4.240	978	995	1024	rBV	411556	1041652	41.04%	5.818%
14	4.728	1140	1147	1151	rBV6	1021	1196	0.05%	0.007%
15	4.773	1159	1161	1166	rBV4	817	567	0.02%	0.003%
16	4.870	1188	1191	1193	rBV3	678	469	0.02%	0.003%
17	4.947	1198	1215	1246	rBV2	1001383	2538329	100.00%	14.177%
18	5.159	1278	1281	1285	rBV4	981	614	0.02%	0.003%
19	5.236	1301	1305	1308	rBV4	819	696	0.03%	0.004%
20	5.307	1323	1327	1328	rBV3	946	672	0.03%	0.004%
21	5.358	1340	1343	1347	rVB4	1213	915	0.04%	0.005%
22	5.413	1356	1360	1363	rBV4	1110	1030	0.04%	0.006%
23	5.455	1371	1373	1378	rBV3	803	675	0.03%	0.004%
24	5.526	1384	1395	1429	rBV	655841	1371658	54.04%	7.661%
25	5.780	1472	1474	1478	rVB4	927	495	0.02%	0.003%
26	5.831	1478	1490	1505	rBV4	10325	24513	0.97%	0.137%
27	5.982	1523	1537	1567	rBV	552139	1157315	45.59%	6.464%
28	6.246	1615	1619	1621	rBV5	779	737	0.03%	0.004%
29	6.329	1639	1645	1653	rVV8	1070	1873	0.07%	0.010%
30	6.419	1671	1673	1674	rBV	1163	498	0.02%	0.003%
31	6.600	1725	1729	1731	rVV3	731	538	0.02%	0.003%
32	6.674	1749	1752	1756	rBV3	786	640	0.03%	0.004%
33	6.905	1814	1824	1852	rBV	277463	541272	21.32%	3.023%
34	7.236	1915	1927	1963	rBV	1144157	2040629	80.39%	11.397%
35	7.400	1976	1978	1980	rBV3	1462	628	0.02%	0.004%
36	7.548	2014	2024	2049	rBV	188818	358523	14.12%	2.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037755.D
 Acq On : 07 Oct 2024 14:23
 Operator : SY/MD
 Sample : VIBLK201
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.712	2072	2075	2078	rBV3	1041	755	0.03%	0.004%
38	7.744	2081	2085	2089	rBV5	1115	953	0.04%	0.005%
39	7.773	2092	2094	2097	rVB4	1053	555	0.02%	0.003%
40	7.812	2101	2106	2112	rVB5	1147	1441	0.06%	0.008%
41	7.847	2114	2117	2120	rVB3	832	526	0.02%	0.003%
42	7.963	2151	2153	2156	rVB2	1098	604	0.02%	0.003%
43	8.024	2163	2172	2222	rBV2	270687	636986	25.09%	3.558%
44	8.484	2310	2315	2320	rBV5	1232	1101	0.04%	0.006%
45	8.542	2329	2333	2337	rBV6	935	992	0.04%	0.006%
46	8.619	2352	2357	2361	rBV5	1237	1090	0.04%	0.006%
47	8.693	2377	2380	2382	rBV3	881	462	0.02%	0.003%
48	8.776	2394	2406	2440	rBV	1052198	1757037	69.22%	9.813%
49	8.995	2473	2474	2477	rVB3	1185	565	0.02%	0.003%
50	9.117	2509	2512	2516	rVV4	887	732	0.03%	0.004%
51	9.423	2605	2607	2610	rVB2	1065	496	0.02%	0.003%
52	9.487	2624	2627	2632	rVV4	624	588	0.02%	0.003%
53	9.535	2634	2642	2646	rVV6	801	911	0.04%	0.005%
54	9.619	2660	2668	2670	rBV3	778	911	0.04%	0.005%
55	9.648	2673	2677	2680	rVB2	560	492	0.02%	0.003%
56	9.686	2686	2689	2696	rVB4	529	505	0.02%	0.003%
57	9.722	2696	2700	2702	rBV3	600	519	0.02%	0.003%
58	9.760	2709	2712	2715	rBV5	729	517	0.02%	0.003%
59	10.053	2797	2803	2807	rBV3	778	916	0.04%	0.005%
60	10.146	2820	2832	2856	rBV	603102	960500	37.84%	5.365%
61	10.342	2891	2893	2898	rVB3	818	509	0.02%	0.003%
62	10.374	2898	2903	2908	rVB4	897	983	0.04%	0.005%
63	10.423	2916	2918	2921	rBV3	1016	566	0.02%	0.003%
64	10.554	2953	2959	2962	rVB4	689	542	0.02%	0.003%
65	10.689	2997	3001	3006	rBV3	792	739	0.03%	0.004%
66	10.905	3066	3068	3074	rVV4	670	537	0.02%	0.003%
67	10.934	3074	3077	3080	rVB3	754	512	0.02%	0.003%
68	11.075	3118	3121	3128	rBV5	631	627	0.02%	0.004%
69	11.140	3137	3141	3142	rBV3	773	540	0.02%	0.003%
70	11.178	3142	3153	3188	rVV	1026170	1655122	65.21%	9.244%
71	11.551	3257	3269	3300	rVV	1110761	1804850	71.10%	10.080%
72	11.789	3340	3343	3344	rBV3	1147	612	0.02%	0.003%
73	11.831	3354	3356	3362	rVB3	912	691	0.03%	0.004%
74	11.863	3362	3366	3368	rBV4	944	666	0.03%	0.004%
75	12.004	3407	3410	3413	rBV2	672	488	0.02%	0.003%
76	12.037	3417	3420	3423	rBV3	624	464	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
 Data File : VV037755.D
 Acq On : 07 Oct 2024 14:23
 Operator : SY/MD
 Sample : VIBLK201
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VIBLK201

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.082	3432	3434	3439	rVB5	749	648	0.03%	0.004%
78	12.201	3465	3471	3476	rVB7	1191	1369	0.05%	0.008%
79	12.358	3517	3520	3521	rVV2	955	600	0.02%	0.003%
80	12.387	3525	3529	3531	rBV2	992	793	0.03%	0.004%
81	12.490	3556	3561	3563	rBV4	762	615	0.02%	0.003%
82	12.635	3602	3606	3609	rVB3	1339	849	0.03%	0.005%
83	12.673	3615	3618	3621	rBV2	627	535	0.02%	0.003%
84	12.975	3708	3712	3716	rBV3	941	635	0.03%	0.004%
85	13.152	3763	3767	3770	rBV3	1012	925	0.04%	0.005%
86	13.390	3837	3841	3846	rVB3	1118	1034	0.04%	0.006%
87	13.458	3860	3862	3866	rBV3	689	472	0.02%	0.003%
88	13.506	3874	3877	3881	rBV4	971	866	0.03%	0.005%
89	13.529	3882	3884	3887	rBV4	991	665	0.03%	0.004%
90	13.644	3916	3920	3924	rBV4	788	690	0.03%	0.004%
91	13.776	3957	3961	3964	rBV4	1206	857	0.03%	0.005%
92	13.850	3980	3984	3986	rBV3	962	766	0.03%	0.004%
93	13.988	4024	4027	4029	rVB3	1241	670	0.03%	0.004%
94	14.059	4046	4049	4053	rVB4	683	503	0.02%	0.003%
95	14.220	4096	4099	4101	rBV3	829	567	0.02%	0.003%
96	14.329	4131	4133	4136	rVB2	1114	606	0.02%	0.003%
97	14.458	4170	4173	4178	rBV3	1255	921	0.04%	0.005%
98	14.500	4183	4186	4188	rBV4	800	496	0.02%	0.003%
99	14.770	4268	4270	4273	rBV4	827	573	0.02%	0.003%
100	15.059	4357	4360	4364	rBV3	1179	1135	0.04%	0.006%




Sum of corrected areas: 17904616

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037755.D
Acq On : 07 Oct 2024 14:23
Operator : SY/MD
Sample : VIBLK201
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

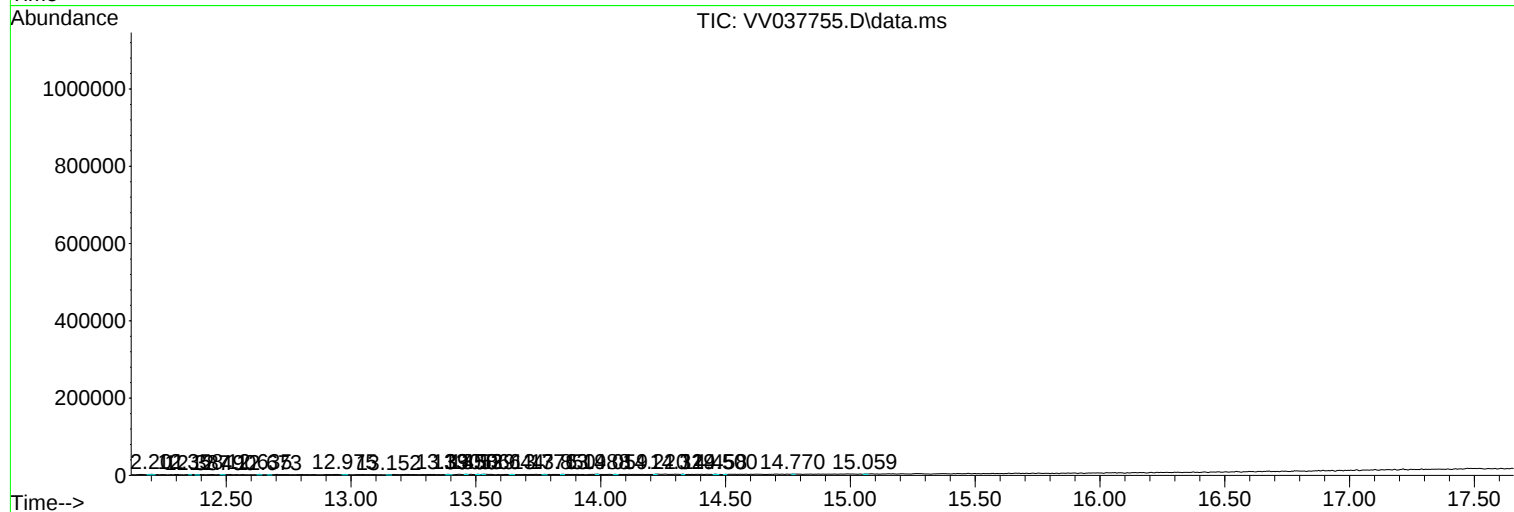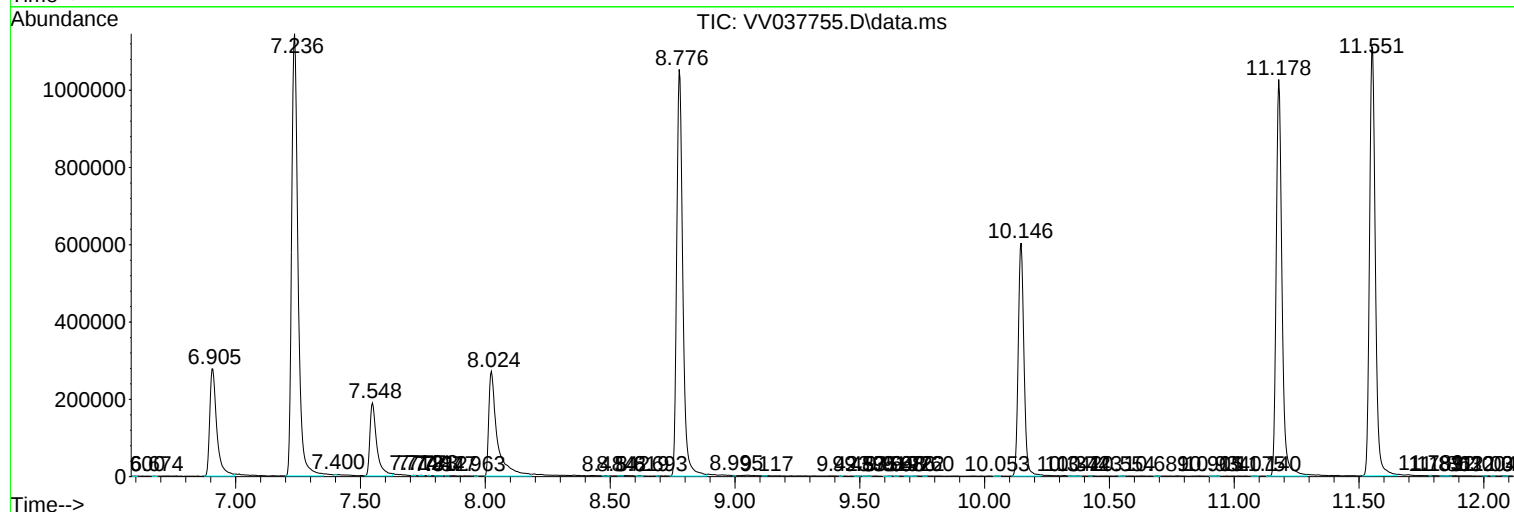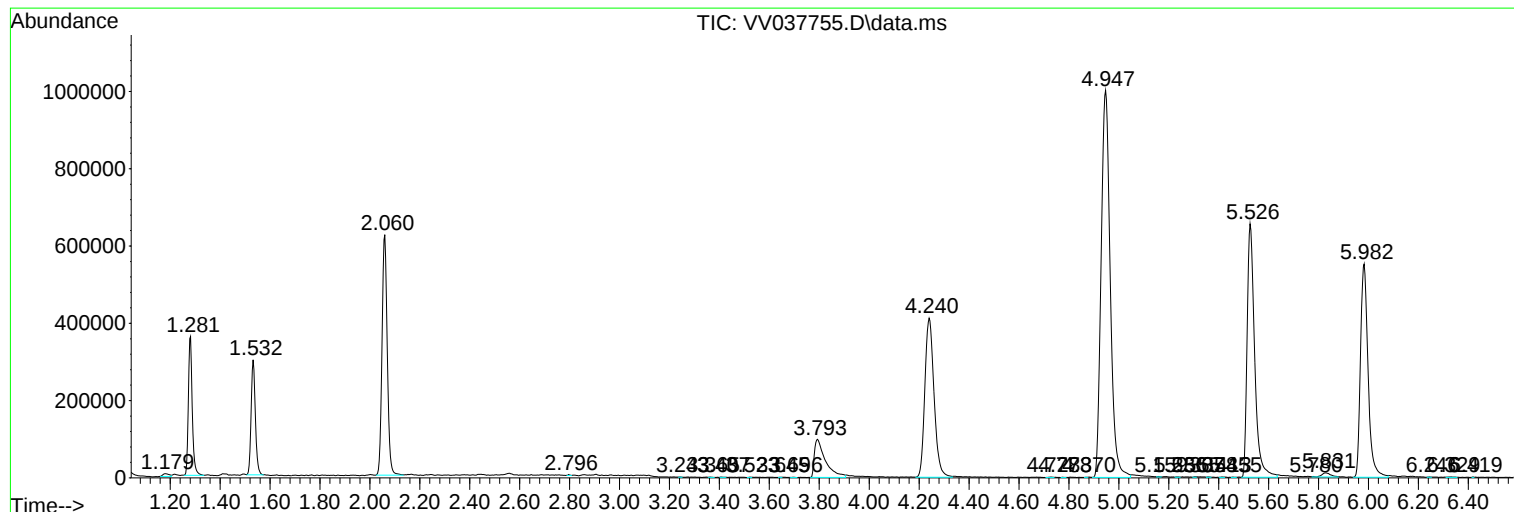

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037755.D
Acq On : 07 Oct 2024 14:23
Operator : SY/MD
Sample : VIBLK201
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037755.D
Acq On : 07 Oct 2024 14:23
Operator : SY/MD
Sample : VIBLK201
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VIBLK201

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc