
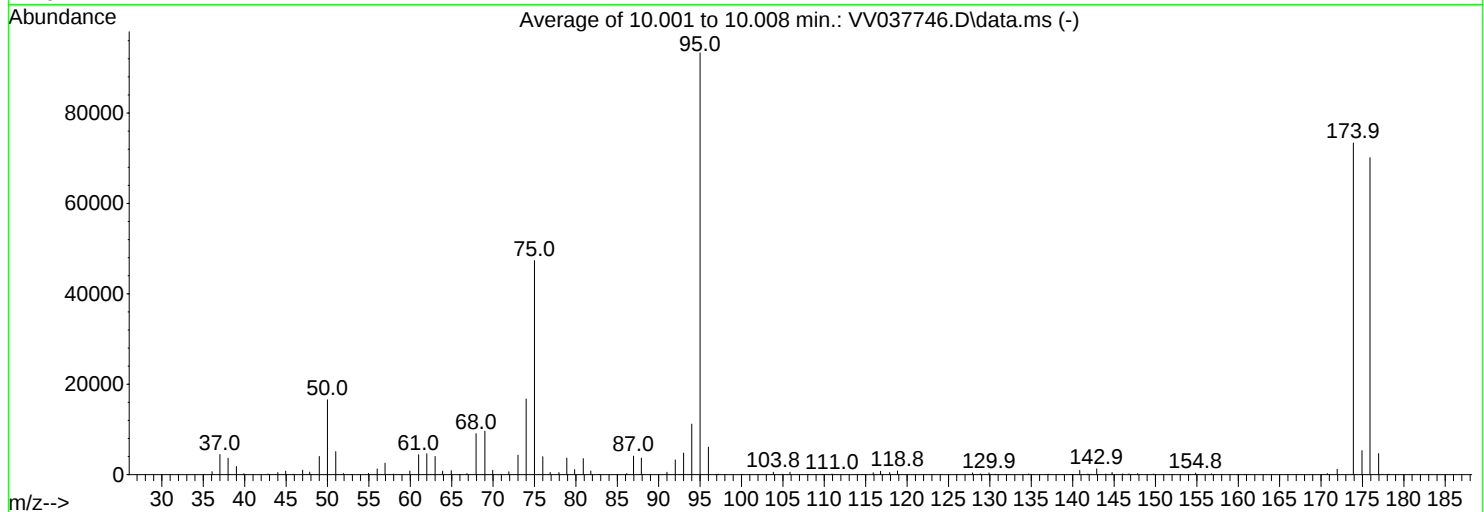


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100724\
Data File : VV037746.D
Acq On : 07 Oct 2024 08:37
Operator : SY/MD
Sample : BFB388
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB388

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Tue Oct 08 04:30:01 2024

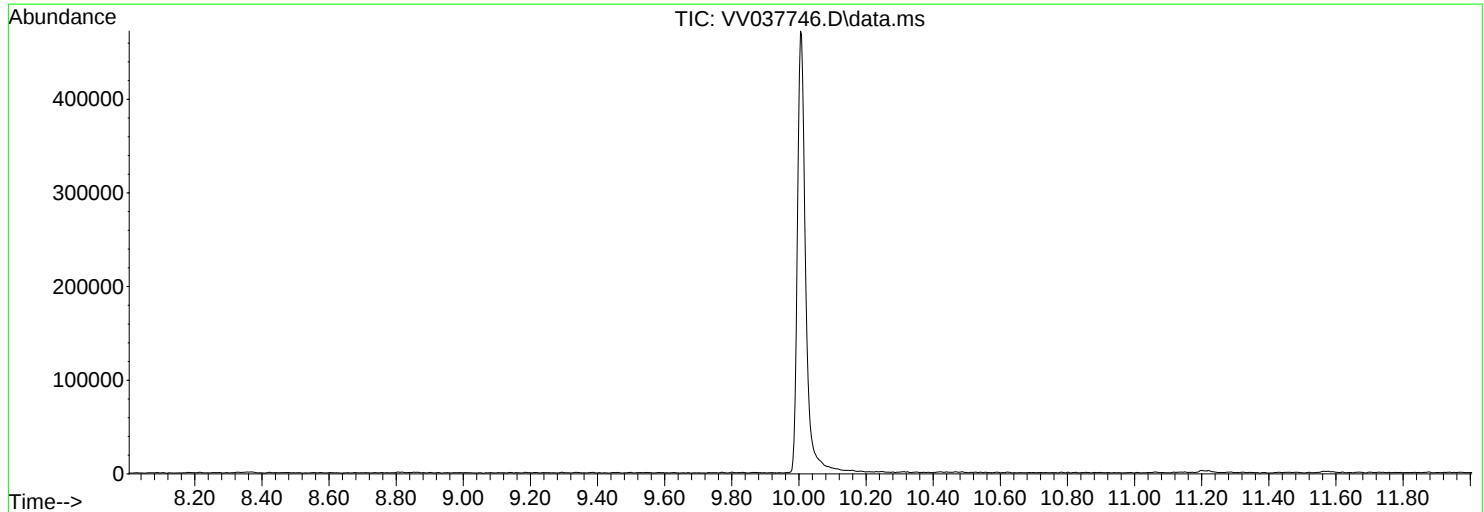

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2776

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	16554	PASS
75	95	30	80	50.7	47355	PASS
95	95	100	100	100.0	93320	PASS
96	95	5	9	6.5	6079	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	78.6	73371	PASS
175	174	5	9	7.2	5304	PASS
176	174	95	105	95.6	70117	PASS
177	176	5	10	6.7	4685	PASS

m/z	Abundance
38.20	128.0
39.90	345.0
44.00	595.0
53.00	112.0
76.90	105.0
206.80	118.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
36.00	607.0
37.00	4051.0
38.00	3574.0
39.00	1652.0
39.90	506.0
42.80	124.0
44.00	1037.0
45.00	716.0
46.00	109.0
46.90	871.0
47.80	555.0
49.00	3693.0
50.00	16005.0
51.00	5222.0
52.00	251.0
52.80	157.0
55.00	253.0
56.00	1177.0
56.90	2372.0
57.90	158.0
59.90	849.0
61.00	4087.0
62.00	4461.0
63.00	3949.0
63.90	806.0
65.00	876.0
66.80	228.0
67.90	8672.0
69.00	9262.0
70.00	1004.0
71.90	615.0
73.00	4024.0
74.00	15596.0
75.00	44624.0
76.00	3731.0
76.90	536.0
78.00	383.0
78.90	3658.0
79.90	1010.0
80.90	3421.0
81.80	707.0
82.80	101.0
86.10	230.0
87.00	3900.0
87.90	3764.0
91.00	558.0
92.00	3022.0
93.00	4628.0
94.00	10841.0
95.00	87720.0
96.00	5783.0
97.20	131.0
103.90	480.0
105.80	478.0
109.80	110.0
111.00	154.0
114.50	117.0
115.90	371.0
116.80	759.0
117.80	446.0
118.90	746.0
127.90	407.0
128.90	156.0
129.90	367.0
130.60	111.0
131.10	116.0
134.70	278.0
140.90	834.0
141.90	118.0
142.90	1201.0
144.00	131.0
144.80	453.0
146.10	123.0
146.80	128.0
147.80	283.0
149.80	123.0
154.90	270.0
156.80	137.0
170.80	231.0
171.90	1143.0
173.90	67888.0
175.00	4998.0
175.90	64768.0
176.90	4252.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
36.00	649.0
37.00	4767.0
38.00	3887.0
39.00	1876.0
39.90	598.0
42.80	152.0
44.00	1090.0
44.90	729.0
45.80	112.0
47.00	1026.0
47.80	589.0
49.00	4159.0
50.00	17224.0
51.00	5256.0
52.00	246.0
52.90	146.0
54.90	306.0
56.00	1351.0
56.90	2653.0
58.00	130.0
59.90	851.0
61.00	4536.0
62.00	4890.0
63.00	4271.0
63.90	809.0
65.00	912.0
65.90	121.0
66.80	251.0
68.00	9232.0
69.00	9976.0
70.00	1005.0
71.90	680.0
73.00	4461.0
74.00	17368.0
75.00	49064.0
76.00	4075.0
76.90	615.0
78.00	488.0
78.90	3800.0
79.80	1123.0
80.90	3604.0
81.80	814.0
82.80	111.0
86.20	256.0
86.90	4244.0
87.90	3794.0
91.00	546.0
92.00	3452.0
93.00	5005.0
94.00	11580.0
95.00	96560.0
96.00	6294.0
97.20	163.0
103.90	569.0
104.90	142.0
105.90	538.0
106.80	112.0
109.80	128.0
111.00	168.0
114.60	137.0
115.90	427.0
116.80	765.0
117.90	472.0
118.80	832.0
127.90	404.0
128.80	179.0
129.90	426.0
130.70	124.0
131.10	117.0
134.70	297.0
136.70	120.0
137.10	118.0
140.90	957.0
141.80	142.0
142.90	1280.0
144.00	153.0
144.80	489.0
146.00	183.0
146.80	183.0
147.90	260.0
149.80	169.0
154.80	390.0
156.70	188.0
160.70	121.0
170.70	257.0
172.00	1201.0
173.90	75800.0
174.90	5513.0
175.90	72696.0
177.00	4801.0
178.20	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388

m/z	Abundance
36.10	764.0
37.00	4611.0
38.00	3923.0
39.00	1886.0
39.90	548.0
42.80	136.0
44.00	1042.0
44.90	869.0
45.80	133.0
47.10	1099.0
47.90	610.0
49.00	4226.0
50.00	16432.0
51.00	4864.0
51.90	220.0
52.90	170.0
54.90	322.0
56.00	1306.0
57.00	2647.0
58.00	104.0
60.00	798.0
61.00	4620.0
62.00	4620.0
63.00	3844.0
63.90	716.0
64.90	898.0
65.90	128.0
66.90	275.0
68.00	9287.0
69.00	9637.0
69.90	886.0
71.90	606.0
73.00	4488.0
74.00	17312.0
75.00	48376.0
76.00	4083.0
76.90	666.0
77.90	537.0
78.90	3618.0
79.90	1245.0
80.90	3566.0
81.80	892.0
86.20	221.0
87.00	4156.0
87.90	3460.0
91.00	506.0
92.00	3343.0
93.00	4659.0
94.00	11108.0
95.00	95680.0
96.00	6160.0
96.90	158.0
103.80	582.0
104.90	208.0
105.90	559.0
108.10	108.0
110.90	146.0
114.80	146.0
115.90	453.0
116.80	745.0
118.00	488.0
118.80	885.0
127.90	332.0
128.80	167.0
129.90	397.0
130.70	145.0
135.00	256.0
137.00	193.0
138.80	122.0
139.80	145.0
140.80	1043.0
141.90	123.0
142.90	1358.0
144.00	134.0
144.70	519.0
146.00	230.0
146.80	180.0
147.90	247.0
149.80	189.0
154.80	427.0
156.70	199.0
160.70	153.0
170.70	264.0
172.00	1265.0
173.90	76424.0
174.90	5400.0
175.90	72888.0
176.90	5003.0
178.20	148.0

Instrument :
MSVOA_V
ClientSampleId :
BFB388