

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037760.D
 Acq On : 08 Oct 2024 09:19
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 09 05:08:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 09 05:07:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	605473	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	597482	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	274983	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	233687	43.967	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	87.940%		
7) Chloroethane-d5	1.532	69	202413	49.062	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.120%		
11) 1,1-Dichloroethene-d2	2.060	65	105594	47.552	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.100%		
21) 2-Butanone-d5	3.793	46	194928	102.966	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	102.970%		
24) Chloroform-d	4.243	84	472296	49.946	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.900%		
26) 1,2-Dichloroethane-d4	4.937	65	285928	51.659	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	103.320%		
32) Benzene-d6	4.953	84	925442	49.498	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	99.000%		
36) 1,2-Dichloropropane-d6	5.982	67	299358	50.283	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	100.560%		
41) Toluene-d8	7.236	98	804246	47.439	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.880%		
43) trans-1,3-Dichloroprop...	7.548	79	131636	47.597	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	95.200%		
47) 2-Hexanone-d5	8.024	63	112445	89.446	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	89.450%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	341317	49.341	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	98.680%		
66) 1,2-Dichlorobenzene-d4	11.554	152	319288	55.102	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	110.200%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3240	0.751	ug/L	# 25


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037760.D
Acq On : 08 Oct 2024 09:19
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 09 05:08:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 09 05:07:27 2024
Response via : Initial Calibration

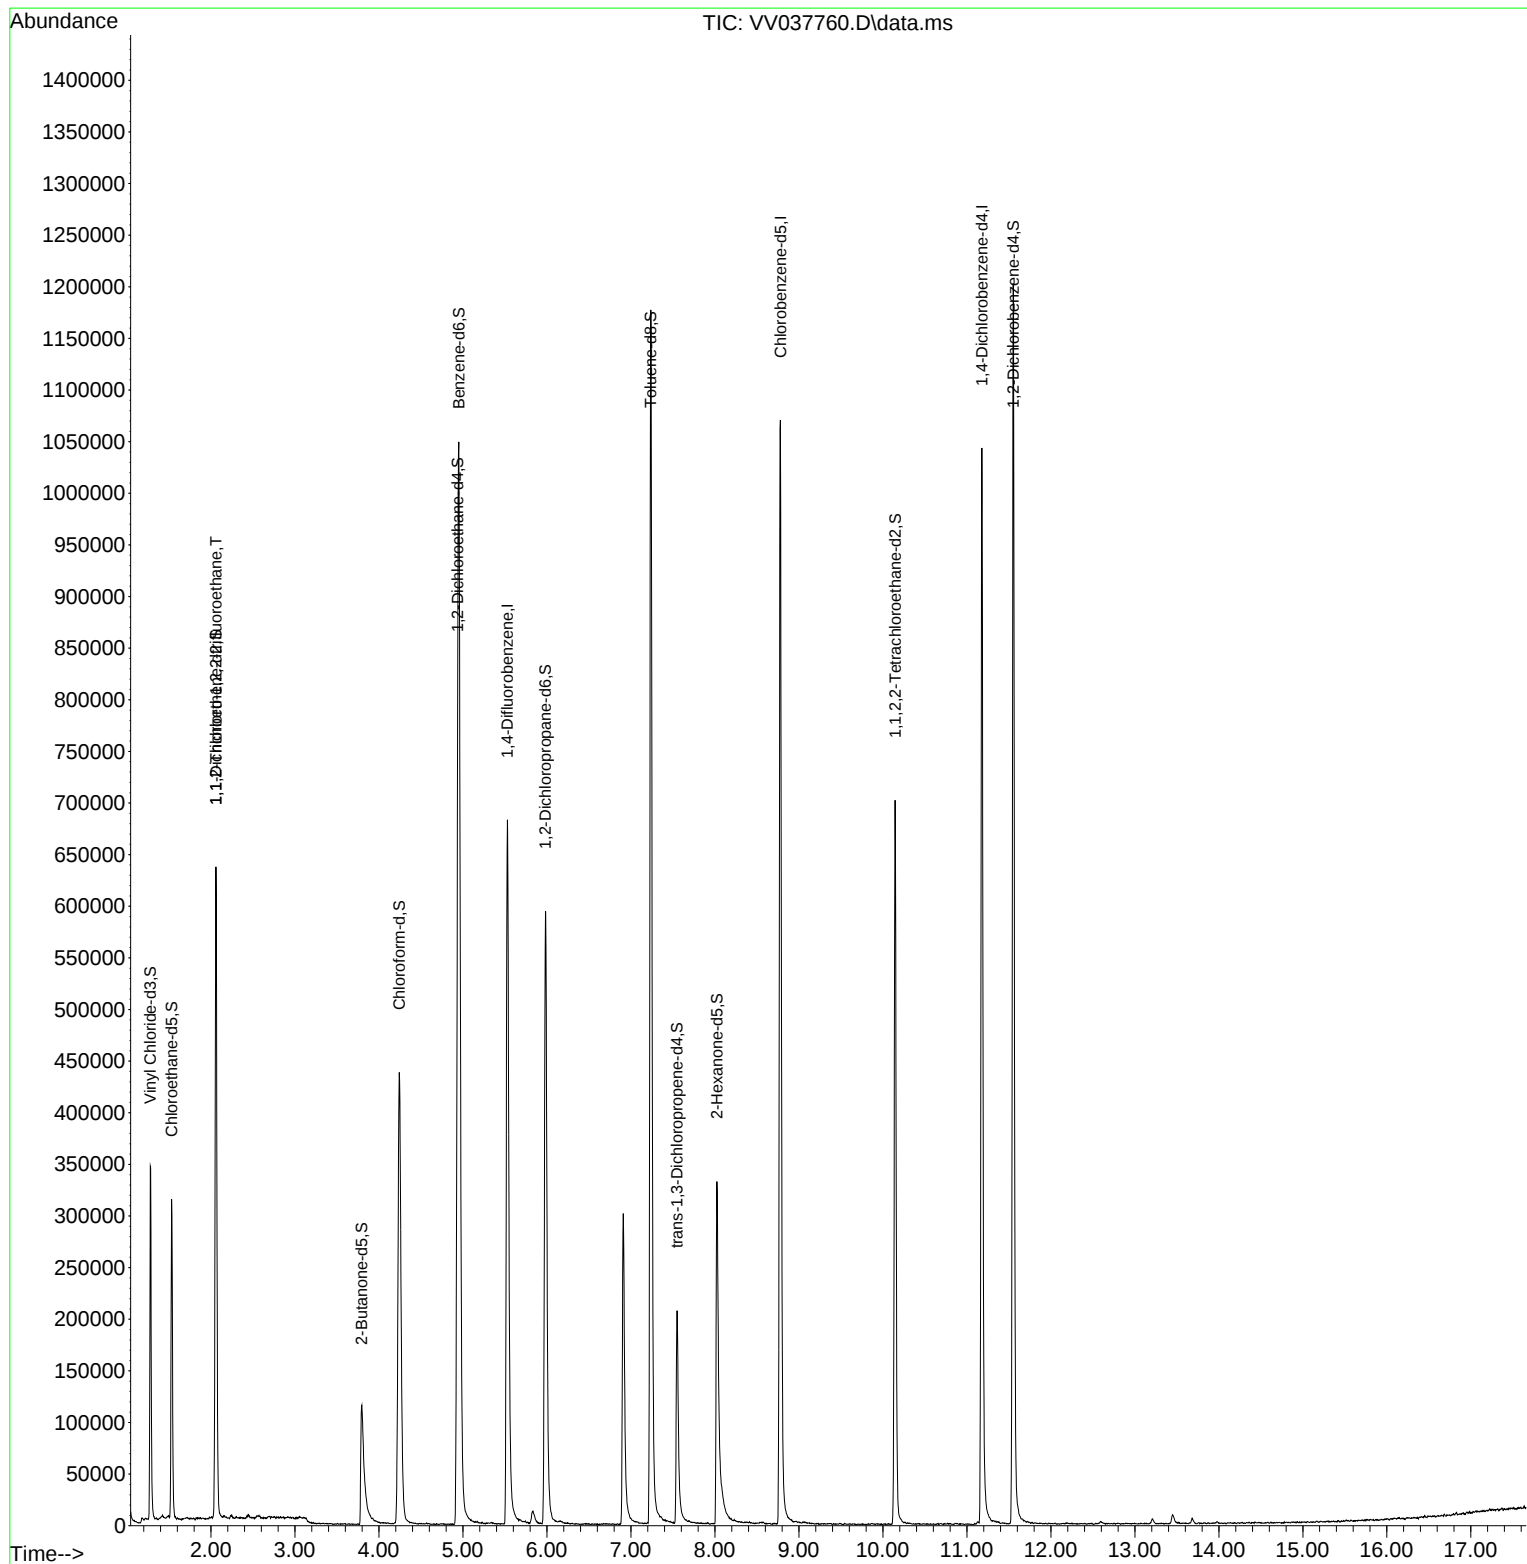

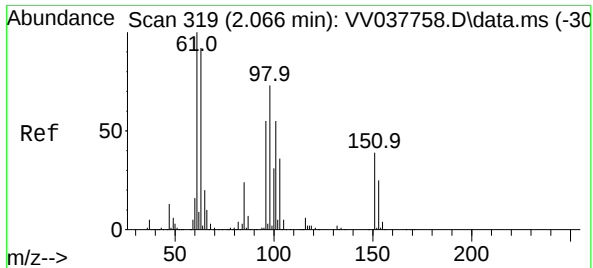

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.751 ug/L
 RT: 2.060 min Scan# 31
 Delta R.T. -0.006 min
 Lab File: VV037760.D
 Acq: 08 Oct 2024 09:19

Instrument :
 MSVOA_V
 ClientSampleId :

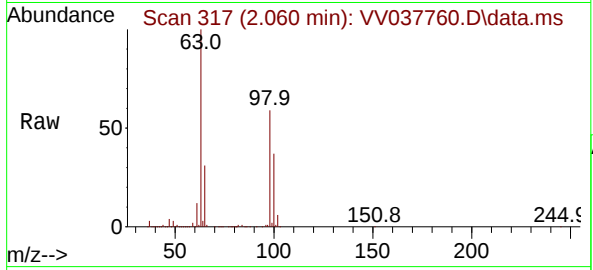

Tgt Ion:	101	Resp:	3240
Ion	Ratio	Lower	Upper
101	100		
85	2.1	34.6	52.0#
151	4.3	57.5	86.3#

