

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037762.D
 Acq On : 08 Oct 2024 12:54
 Operator : SY/MD
 Sample : P4346-01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 09 05:08:49 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 09 05:07:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.526	114	587029	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.776	117	579350	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	270960	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	241485	46.861	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	93.720%		
7) Chloroethane-d5	1.532	69	197648	49.413	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	98.820%		
11) 1,1-Dichloroethene-d2	2.056	65	105576	49.038	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	98.080%		
21) 2-Butanone-d5	3.793	46	154779	84.327	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.330%		
24) Chloroform-d	4.236	84	447178	48.775	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	97.560%		
26) 1,2-Dichloroethane-d4	4.931	65	272686	50.814	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	101.620%		
32) Benzene-d6	4.947	84	893587	49.290	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.580%		
36) 1,2-Dichloropropane-d6	5.979	67	283427	49.097	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	98.200%		
41) Toluene-d8	7.233	98	777311	47.285	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	94.580%		
43) trans-1,3-Dichloroprop...	7.545	79	119327	44.497	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	89.000%		
47) 2-Hexanone-d5	8.021	63	86019	70.566	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	70.570%		
56) 1,1,2,2-Tetrachloroeth...	10.143	84	290265	43.274	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	86.540%		
66) 1,2-Dichlorobenzene-d4	11.551	152	291441	51.043	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	102.080%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.060	101	3125	0.747	ug/L	# 26


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037762.D
Acq On : 08 Oct 2024 12:54
Operator : SY/MD
Sample : P4346-01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 09 05:08:49 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 09 05:07:27 2024
Response via : Initial Calibration

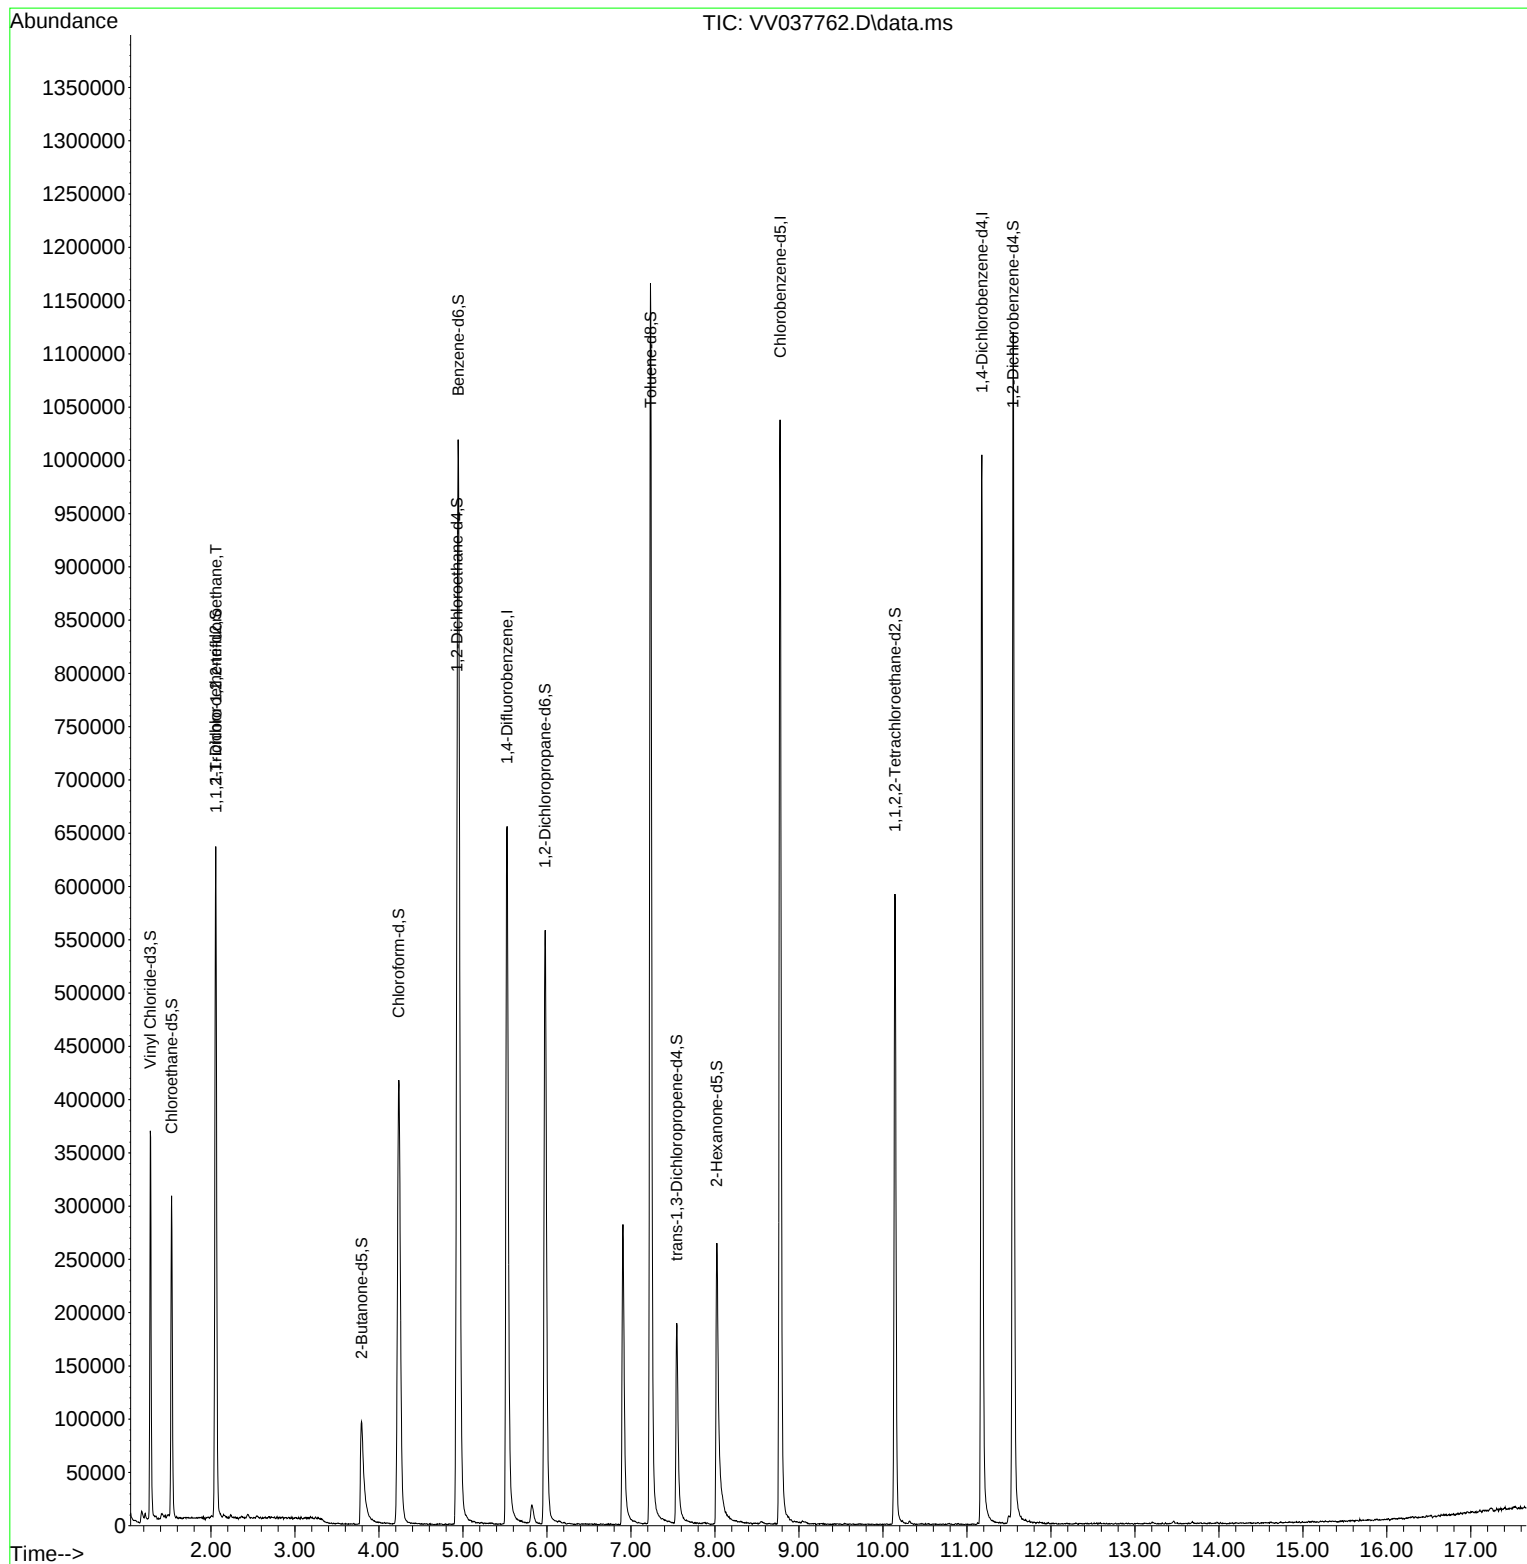

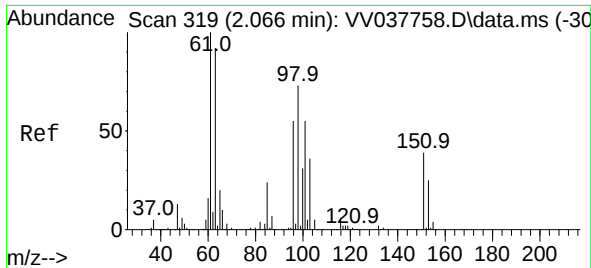

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.747 ug/L
 RT: 2.060 min Scan# 317
 Delta R.T. -0.006 min
 Lab File: VV037762.D
 Acq: 08 Oct 2024 12:54

Instrument :
 MSVOA_V
 ClientSampleId :

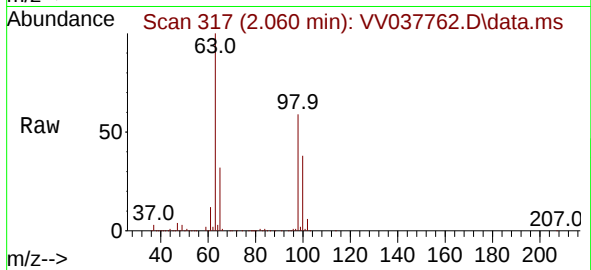

Tgt Ion:101 Resp: 3125
 Ion Ratio Lower Upper
 101 100
 85 2.2 34.6 52.0#
 151 5.1 57.5 86.3#

