

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037771.D
 Acq On : 08 Oct 2024 16:14
 Operator : SY/MD
 Sample : P4329-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 09 05:10:51 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 09 05:07:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	505602	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	525095	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	243083	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	211360	47.621	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 95.240%			
7) Chloroethane-d5	1.532	69	177045	51.390	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 102.780%			
11) 1,1-Dichloroethene-d2	2.056	65	94376	50.895	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 101.800%			
21) 2-Butanone-d5	3.799	46	147039	93.012	ug/L	0.01
Spiked Amount 100.000	Range 40 - 130		Recovery = 93.010%			
24) Chloroform-d	4.243	84	411508	52.113	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 104.220%			
26) 1,2-Dichloroethane-d4	4.937	65	251223	54.354	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 108.700%			
32) Benzene-d6	4.950	84	809358	49.257	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 98.520%			
36) 1,2-Dichloropropane-d6	5.982	67	261263	49.934	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 99.860%			
41) Toluene-d8	7.236	98	711899	47.780	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 95.560%			
43) trans-1,3-Dichloroprop...	7.551	79	108404	44.600	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 89.200%			
47) 2-Hexanone-d5	8.024	63	93571	84.693	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 84.690%			
56) 1,1,2,2-Tetrachloroeth...	10.146	84	291395	47.931	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 95.860%			
66) 1,2-Dichlorobenzene-d4	11.555	152	270524	52.814	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 105.620%			
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.053	101	3012	0.836	ug/L	# 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037771.D
Acq On : 08 Oct 2024 16:14
Operator : SY/MD
Sample : P4329-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 09 05:10:51 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 09 05:07:27 2024
Response via : Initial Calibration

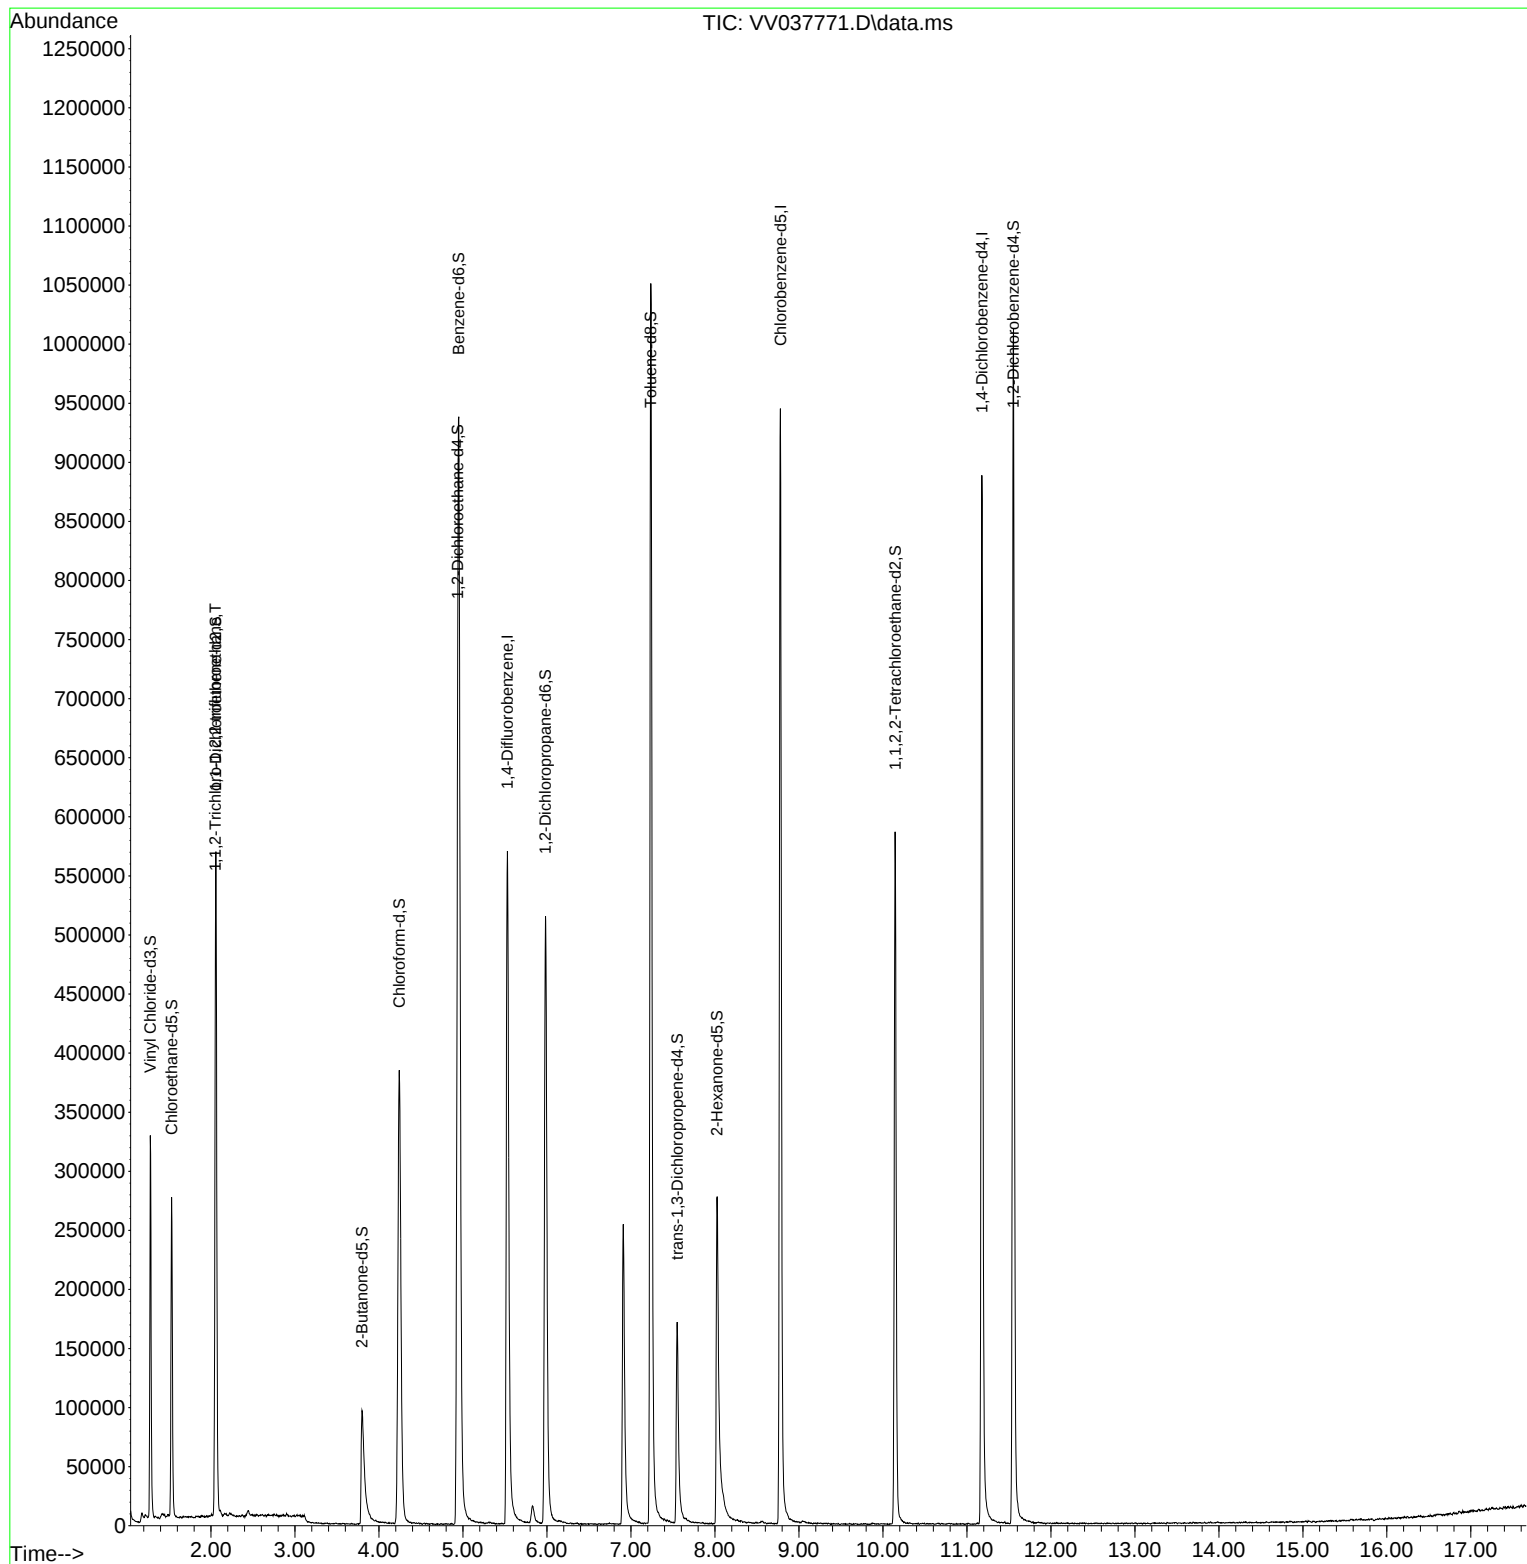

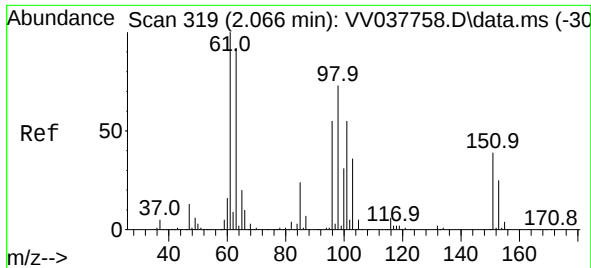

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.836 ug/L
 RT: 2.053 min Scan# 31
 Delta R.T. -0.013 min
 Lab File: VV037771.D
 Acq: 08 Oct 2024 16:14

Instrument :
 MSVOA_V
 ClientSampleId :

Tgt Ion:101 Resp: 3012
 Ion Ratio Lower Upper
 101 100
 85 1.3 34.6 52.0#
 151 1.3 57.5 86.3#

