

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037764.D
 Acq On : 08 Oct 2024 13:43
 Operator : SY/MD
 Sample : P4329-23
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 A4FD9

Quant Time: Oct 09 05:09:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Oct 09 05:07:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	460782	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	470271	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	219006	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	222196	54.932	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery = 109.860%			
7) Chloroethane-d5	1.532	69	185993	59.239	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery = 118.480%			
11) 1,1-Dichloroethene-d2	2.056	65	98796	58.462	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 116.920%			
21) 2-Butanone-d5	3.796	46	148745	103.243	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery = 103.240%			
24) Chloroform-d	4.240	84	431009	59.892	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 119.780%			
26) 1,2-Dichloroethane-d4	4.934	65	261964	62.191	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 124.380%			
32) Benzene-d6	4.950	84	851162	57.840	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery = 115.680%			
36) 1,2-Dichloropropane-d6	5.982	67	269557	57.525	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery = 115.040%			
41) Toluene-d8	7.236	98	743181	55.695	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 111.400%			
43) trans-1,3-Dichloroprop...	7.548	79	114357	52.535	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery = 105.060%			
47) 2-Hexanone-d5	8.024	63	88444	89.385	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery = 89.380%			
56) 1,1,2,2-Tetrachloroeth...	10.146	84	283933	52.149	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery = 104.300%			
66) 1,2-Dichlorobenzene-d4	11.554	152	284280	61.601	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery = 123.200%#			
Target Compounds					Qvalue	
13) Acetone	2.114	43	64474	45.650	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037764.D
Acq On : 08 Oct 2024 13:43
Operator : SY/MD
Sample : P4329-23
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
A4FD9

Quant Time: Oct 09 05:09:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Oct 09 05:07:27 2024
Response via : Initial Calibration

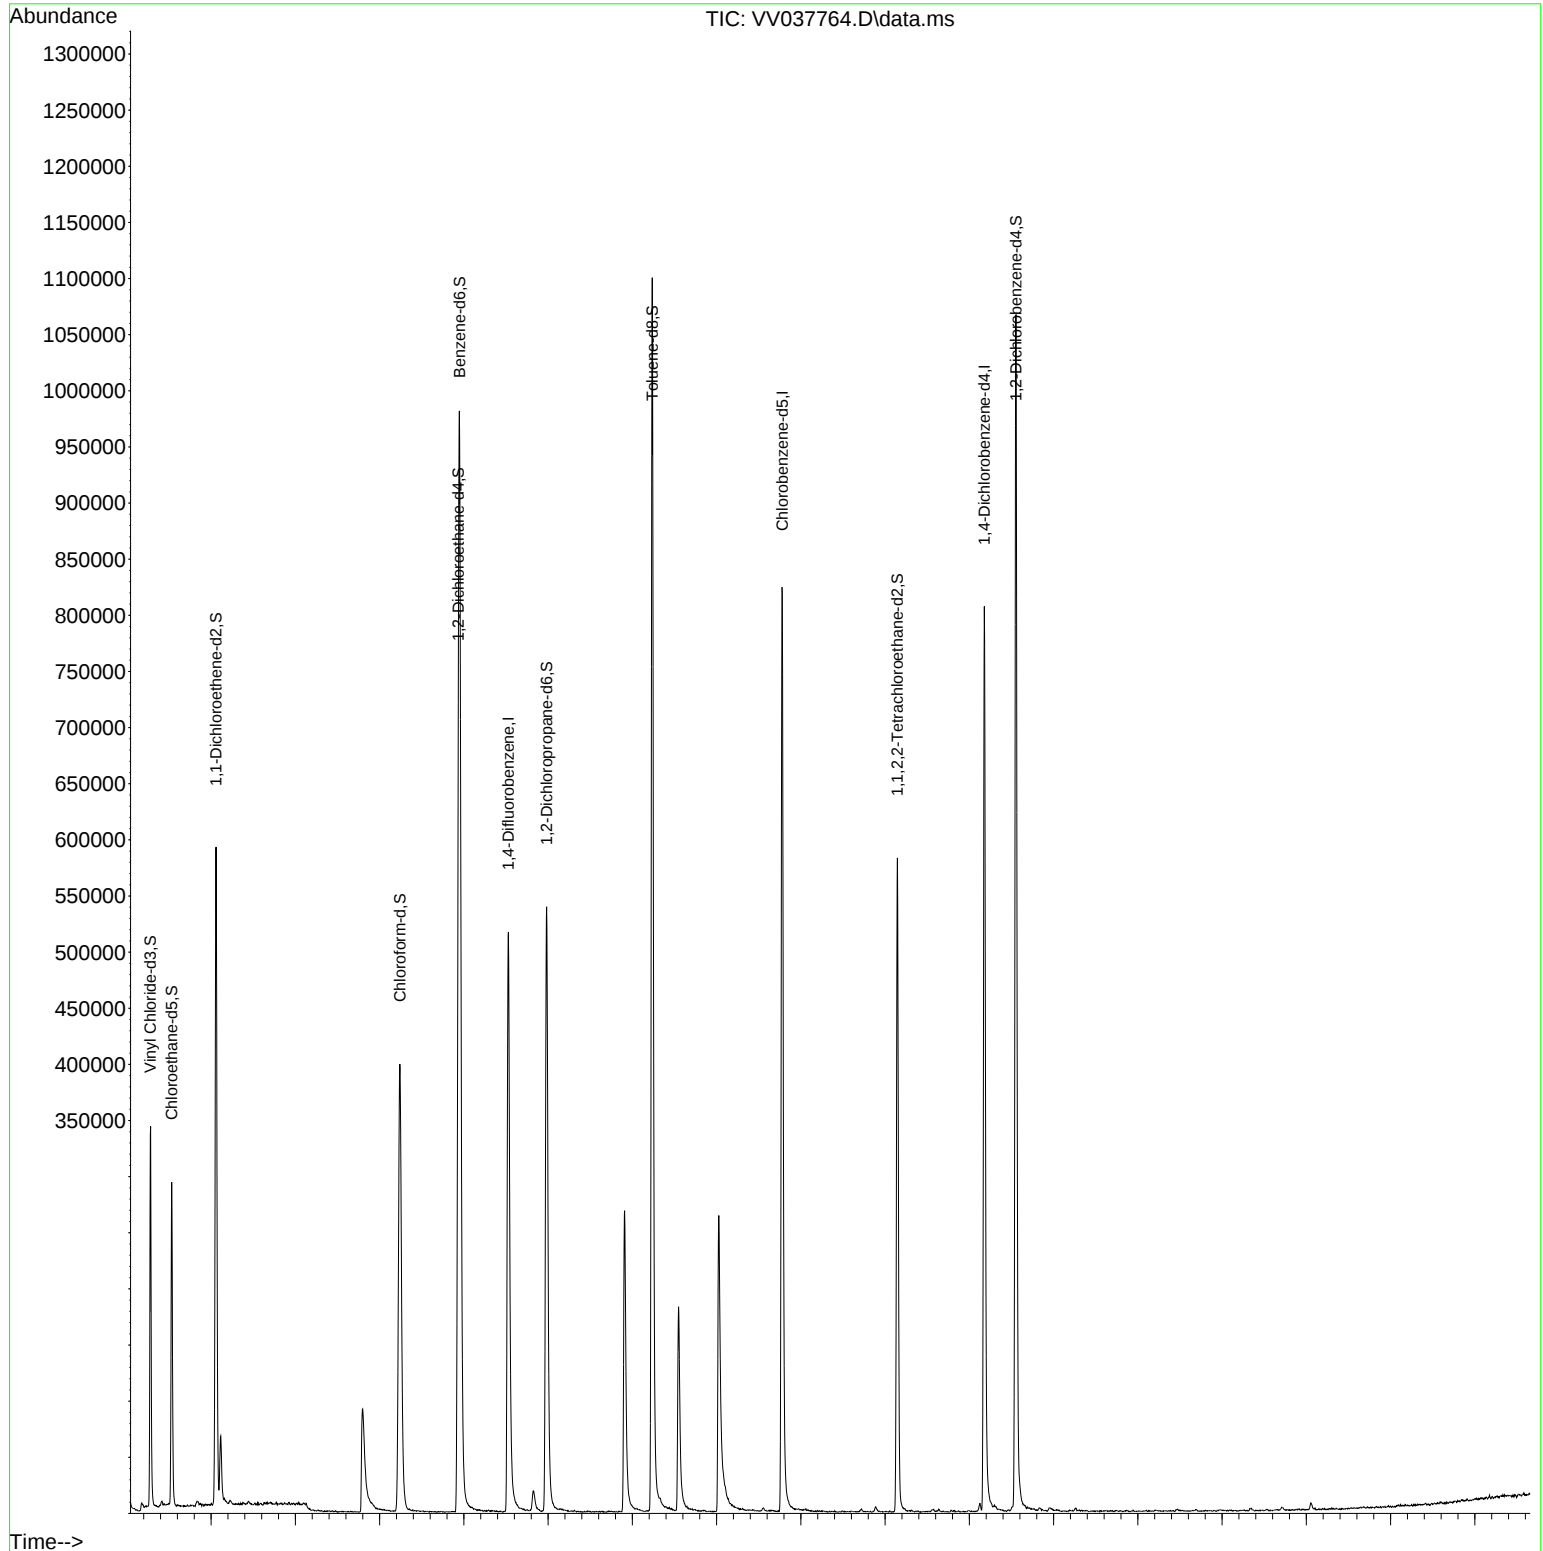

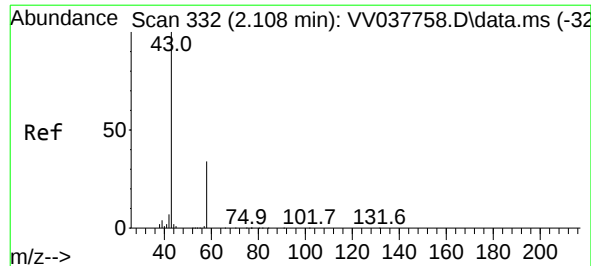

#13

Acetone

Concen: 45.650 ug/L

RT: 2.114 min Scan# 33

Delta R.T. 0.006 min

Lab File: VV037764.D

Acq: 08 Oct 2024 13:43

Instrument :

MSVOA_V

ClientSampleId :

A4FD9

Tgt Ion: 43 Resp: 64474

Ion Ratio Lower Upper

43 100

58 32.4 0.0 66.6

