

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037760.D
 Acq On : 08 Oct 2024 09:19
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037760.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	341717	373148	13.91%	1.986%
2	1.532	146	153	170	rVB	309475	367848	13.71%	1.957%
3	2.060	308	317	334	rVB	628353	899085	33.51%	4.784%
4	3.507	765	767	771	rVB3	834	474	0.02%	0.003%
5	3.571	784	787	790	rBV3	477	364	0.01%	0.002%
6	3.622	801	803	805	rBV	410	258	0.01%	0.001%
7	3.796	848	857	894	rBV	115407	346560	12.91%	1.844%
8	4.243	981	996	1029	rBV	436307	1108871	41.32%	5.901%
9	4.484	1067	1071	1075	rBV4	779	764	0.03%	0.004%
10	4.648	1120	1122	1124	rBV2	630	286	0.01%	0.002%
11	4.677	1128	1131	1132	rBV2	455	169	0.01%	0.001%
12	4.687	1132	1134	1140	rVB4	667	417	0.02%	0.002%
13	4.735	1145	1149	1150	rBV2	487	306	0.01%	0.002%
14	4.773	1159	1161	1164	rVB	726	372	0.01%	0.002%
15	4.854	1184	1186	1189	rVB2	696	361	0.01%	0.002%
16	4.870	1189	1191	1193	rBV2	445	245	0.01%	0.001%
17	4.950	1198	1216	1259	rBV2	1048687	2683403	100.00%	14.280%
18	5.529	1385	1396	1435	rBV	681881	1418298	52.85%	7.547%
19	5.834	1479	1491	1504	rBV5	12017	30636	1.14%	0.163%
20	5.982	1524	1537	1566	rBV	593614	1230526	45.86%	6.548%
21	6.407	1665	1669	1671	rBV3	492	346	0.01%	0.002%
22	6.429	1673	1676	1677	rBV2	534	221	0.01%	0.001%
23	6.468	1686	1688	1691	rBV3	721	338	0.01%	0.002%
24	6.490	1692	1695	1699	rVB3	810	486	0.02%	0.003%
25	6.535	1704	1709	1710	rBV3	786	553	0.02%	0.003%
26	6.603	1728	1730	1733	rVB2	787	405	0.02%	0.002%
27	6.622	1733	1736	1737	rBV2	570	247	0.01%	0.001%
28	6.632	1737	1739	1741	rBV2	413	224	0.01%	0.001%
29	6.674	1749	1752	1754	rBV2	733	406	0.02%	0.002%
30	6.741	1770	1773	1776	rBV5	638	426	0.02%	0.002%
31	6.777	1781	1784	1785	rBV2	387	231	0.01%	0.001%
32	6.822	1794	1798	1800	rBV3	456	296	0.01%	0.002%
33	6.857	1807	1809	1811	rVB2	588	259	0.01%	0.001%
34	6.870	1811	1813	1815	rBV3	1010	529	0.02%	0.003%
35	6.908	1815	1825	1852	rBV	300791	579137	21.58%	3.082%
36	7.236	1917	1927	1961	rBV	1174923	2098619	78.21%	11.168%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037760.D
 Acq On : 08 Oct 2024 09:19
 Operator : SY/MD
 Sample : VV1008WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK235

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.548	2015	2024	2056	rBV	205860	387350	14.44%	2.061%
38	8.024	2163	2172	2221	rBV2	331526	753556	28.08%	4.010%
39	8.616	2354	2356	2358	rBV	645	244	0.01%	0.001%
40	8.696	2379	2381	2383	rBV3	912	526	0.02%	0.003%
41	8.780	2395	2407	2435	rBV	1069306	1786339	66.57%	9.506%
42	9.156	2523	2524	2527	rBV2	767	435	0.02%	0.002%
43	9.246	2549	2552	2554	rBV3	512	309	0.01%	0.002%
44	9.259	2554	2556	2558	rBV	557	364	0.01%	0.002%
45	9.416	2601	2605	2610	rBV4	918	739	0.03%	0.004%
46	9.439	2610	2612	2614	rVB2	708	302	0.01%	0.002%
47	9.487	2622	2627	2630	rBV4	988	975	0.04%	0.005%
48	9.545	2640	2645	2648	rBV3	1122	871	0.03%	0.005%
49	9.587	2656	2658	2660	rBV2	338	194	0.01%	0.001%
50	9.638	2672	2674	2678	rBV4	555	538	0.02%	0.003%
51	9.677	2685	2686	2688	rBV4	280	113	0.00%	0.001%
52	9.696	2689	2692	2694	rVV2	239	163	0.01%	0.001%
53	9.738	2702	2705	2706	rBV	412	220	0.01%	0.001%
54	9.764	2711	2713	2717	rVB2	612	343	0.01%	0.002%
55	9.908	2757	2758	2759	rVB	201	39	0.00%	0.000%
56	9.921	2759	2762	2767	rBV4	744	789	0.03%	0.004%
57	9.982	2779	2781	2786	rVB3	749	548	0.02%	0.003%
58	10.014	2786	2791	2794	rBV3	777	804	0.03%	0.004%
59	10.030	2794	2796	2798	rVB	670	249	0.01%	0.001%
60	10.098	2813	2817	2819	rBV2	677	429	0.02%	0.002%
61	10.146	2819	2832	2866	rVV	701298	1113706	41.50%	5.927%
62	10.439	2921	2923	2926	rVB3	648	258	0.01%	0.001%
63	10.519	2946	2948	2950	rBV2	537	278	0.01%	0.001%
64	10.545	2954	2956	2960	rBV4	440	214	0.01%	0.001%
65	10.571	2960	2964	2966	rVB2	468	253	0.01%	0.001%
66	10.641	2984	2986	2987	rBV2	355	123	0.00%	0.001%
67	10.683	2994	2999	3002	rBV3	1013	1094	0.04%	0.006%
68	10.725	3010	3012	3013	rBV3	374	108	0.00%	0.001%
69	10.735	3013	3015	3018	rVB3	770	339	0.01%	0.002%
70	10.770	3024	3026	3029	rBV4	695	353	0.01%	0.002%
71	10.850	3049	3051	3052	rBV	833	391	0.01%	0.002%
72	10.985	3089	3093	3096	rBV4	757	714	0.03%	0.004%
73	11.075	3118	3121	3122	rBV4	149	93	0.00%	0.000%
74	11.091	3122	3126	3128	rBV3	953	549	0.02%	0.003%
75	11.127	3132	3137	3143	rBV6	2313	3321	0.12%	0.018%
76	11.178	3143	3153	3180	rBV	1041301	1649160	61.46%	8.776%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037760.D
Acq On : 08 Oct 2024 09:19
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	11.551	3258	3269	3298	rBV	1200606	1934539	72.09%	10.295%
78	11.976	3398	3401	3406	rBV5	1000	761	0.03%	0.004%
79	12.085	3432	3435	3441	rVB4	670	602	0.02%	0.003%
80	12.111	3441	3443	3447	rBV2	552	503	0.02%	0.003%
81	12.435	3541	3544	3545	rBV2	584	359	0.01%	0.002%
82	12.487	3558	3560	3567	rVB3	1267	1006	0.04%	0.005%
83	12.664	3610	3615	3616	rBV4	815	674	0.03%	0.004%
84	12.789	3647	3654	3655	rBV5	993	957	0.04%	0.005%

Sum of corrected areas: 18791908




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037760.D
Acq On : 08 Oct 2024 09:19
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

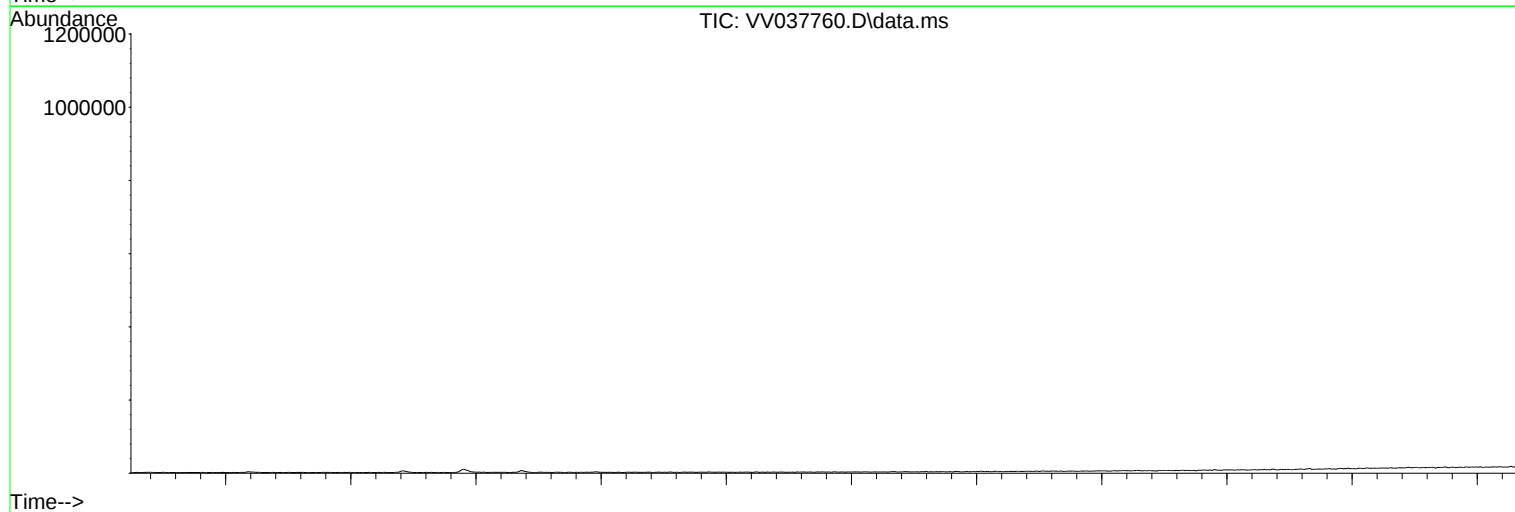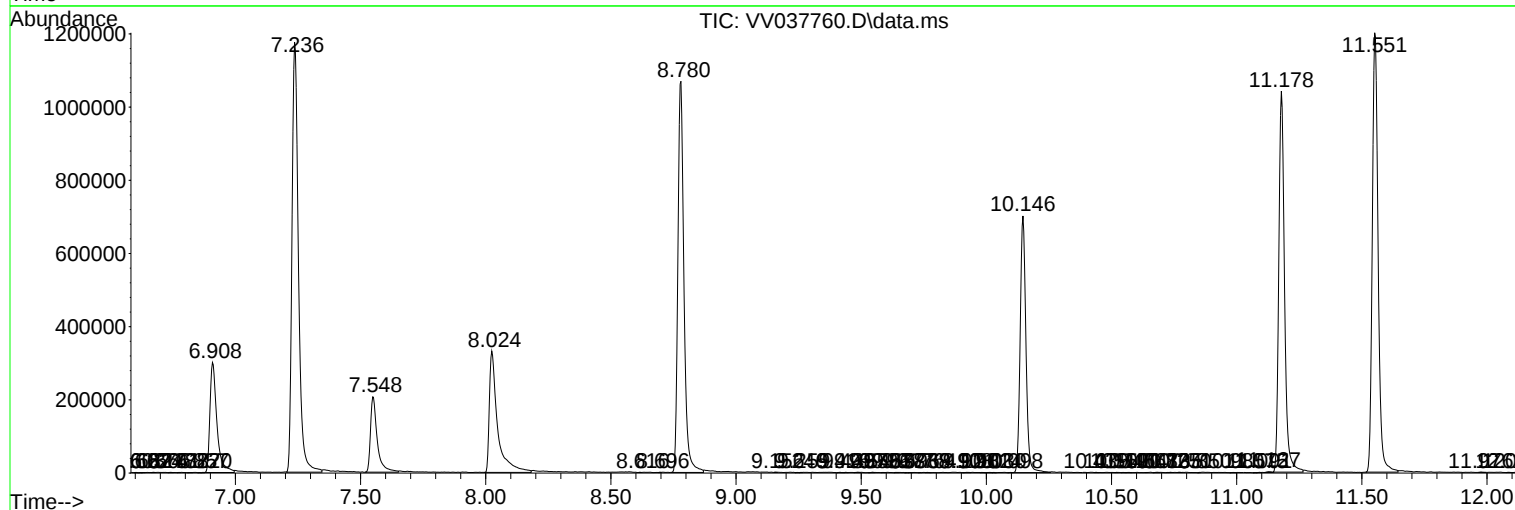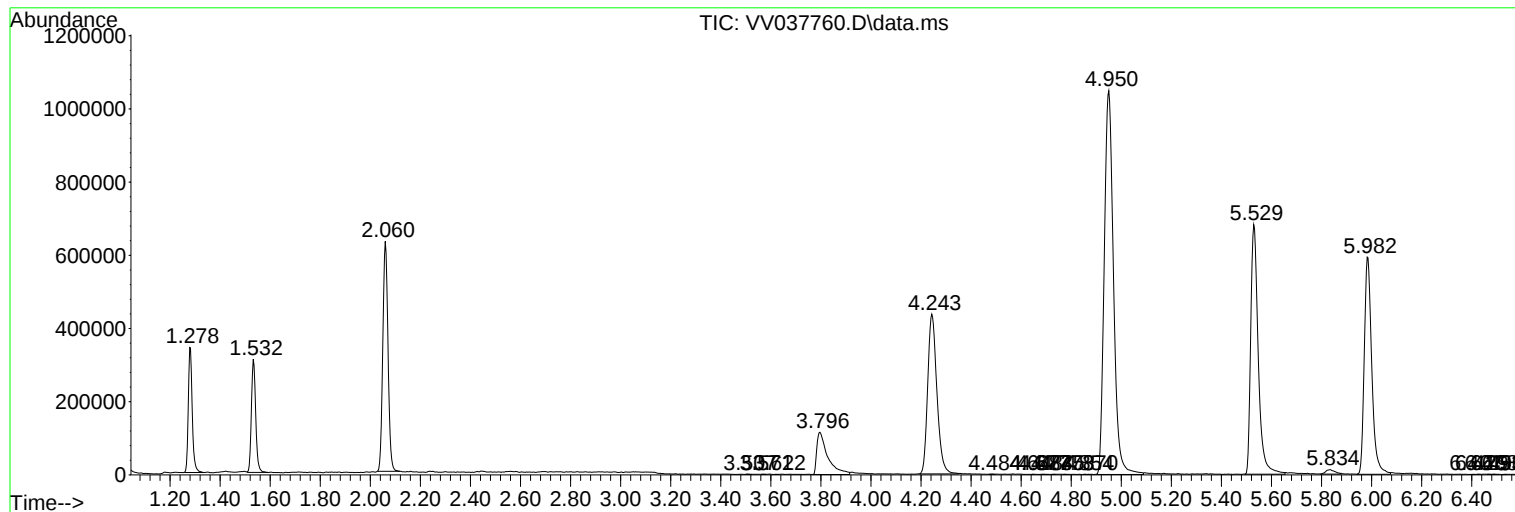

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037760.D
Acq On : 08 Oct 2024 09:19
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037760.D
Acq On : 08 Oct 2024 09:19
Operator : SY/MD
Sample : VV1008WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK235

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc