

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037766.D
 Acq On : 08 Oct 2024 14:26
 Operator : SY/MD
 Sample : P4349-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037766.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	35	42	51	rBV	14544	24511	1.00%	0.144%
2	1.278	66	74	90	rBV	330514	363220	14.88%	2.133%
3	1.532	145	153	166	rBV	278020	326554	13.38%	1.917%
4	2.060	307	317	330	rBV	588105	845893	34.66%	4.967%
5	3.317	705	708	710	rBV	936	560	0.02%	0.003%
6	3.471	754	756	762	rVB2	982	606	0.02%	0.004%
7	3.593	792	794	799	rVB2	743	527	0.02%	0.003%
8	3.625	799	804	806	rBV3	725	523	0.02%	0.003%
9	3.667	812	817	821	rBV4	1183	982	0.04%	0.006%
10	3.703	821	828	833	rBV4	853	1027	0.04%	0.006%
11	3.799	850	858	889	rBV	98669	291852	11.96%	1.714%
12	4.243	980	996	1027	rVV	397637	1003465	41.11%	5.892%
13	4.490	1070	1073	1078	rVB3	1503	1116	0.05%	0.007%
14	4.519	1078	1082	1083	rBV	918	509	0.02%	0.003%
15	4.564	1092	1096	1100	rVV5	942	834	0.03%	0.005%
16	4.670	1125	1129	1131	rBV3	895	638	0.03%	0.004%
17	4.883	1192	1195	1200	rBV3	533	643	0.03%	0.004%
18	4.950	1201	1216	1252	rBV2	973395	2440691	100.00%	14.330%
19	5.178	1285	1287	1291	rVV4	860	621	0.03%	0.004%
20	5.198	1291	1293	1297	rVB4	956	681	0.03%	0.004%
21	5.436	1365	1367	1372	rVB5	740	508	0.02%	0.003%
22	5.529	1385	1396	1431	rBV	604139	1248716	51.16%	7.332%
23	5.831	1479	1490	1502	rVV5	15878	35888	1.47%	0.211%
24	5.985	1525	1538	1570	rBV	536823	1116494	45.74%	6.555%
25	6.326	1640	1644	1647	rBV	721	604	0.02%	0.004%
26	6.497	1694	1697	1700	rBV4	2229	1061	0.04%	0.006%
27	6.522	1702	1705	1709	rVB3	889	692	0.03%	0.004%
28	6.670	1749	1751	1757	rVB3	807	604	0.02%	0.004%
29	6.706	1757	1762	1764	rVB3	636	512	0.02%	0.003%
30	6.834	1798	1802	1804	rBV3	642	539	0.02%	0.003%
31	6.857	1806	1809	1813	rBV3	964	738	0.03%	0.004%
32	6.908	1813	1825	1848	rBV	267839	513715	21.05%	3.016%
33	7.156	1899	1902	1909	rVB5	769	636	0.03%	0.004%
34	7.236	1912	1927	1947	rBV	1104040	1921895	78.74%	11.284%
35	7.439	1988	1990	1991	rBV2	1230	514	0.02%	0.003%
36	7.551	2015	2025	2050	rBV	178890	342872	14.05%	2.013%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037766.D
 Acq On : 08 Oct 2024 14:26
 Operator : SY/MD
 Sample : P4349-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.863	2120	2122	2129	rVB6	1240	1396	0.06%	0.008%
38	7.915	2134	2138	2139	rBV3	865	577	0.02%	0.003%
39	7.976	2153	2157	2159	rBV3	826	506	0.02%	0.003%
40	8.027	2164	2173	2211	rBV3	283492	663921	27.20%	3.898%
41	8.297	2255	2257	2260	rBV3	936	606	0.02%	0.004%
42	8.551	2332	2336	2338	rBV5	1557	1324	0.05%	0.008%
43	8.632	2358	2361	2365	rVB4	1405	824	0.03%	0.005%
44	8.722	2383	2389	2390	rBV3	1175	1071	0.04%	0.006%
45	8.780	2396	2407	2437	rBV	948641	1604618	65.74%	9.421%
46	9.040	2486	2488	2489	rBV2	1096	526	0.02%	0.003%
47	9.082	2494	2501	2514	rVB4	11495	20371	0.83%	0.120%
48	9.217	2541	2543	2548	rVB4	1397	1130	0.05%	0.007%
49	9.294	2564	2567	2570	rVB4	1138	754	0.03%	0.004%
50	9.339	2577	2581	2583	rBV5	931	751	0.03%	0.004%
51	9.374	2588	2592	2599	rBV6	943	935	0.04%	0.005%
52	9.487	2618	2627	2633	rBV6	4970	8224	0.34%	0.048%
53	9.564	2647	2651	2655	rVB6	710	550	0.02%	0.003%
54	9.651	2676	2678	2683	rVB2	905	615	0.03%	0.004%
55	9.715	2693	2698	2700	rBV2	779	739	0.03%	0.004%
56	9.792	2719	2722	2724	rBV2	823	537	0.02%	0.003%
57	9.857	2736	2742	2744	rVB5	937	756	0.03%	0.004%
58	9.988	2779	2783	2786	rVV4	708	563	0.02%	0.003%
59	10.008	2786	2789	2791	rVV2	844	554	0.02%	0.003%
60	10.079	2808	2811	2813	rBV	883	503	0.02%	0.003%
61	10.146	2818	2832	2855	rBV	610862	960418	39.35%	5.639%
62	10.320	2881	2886	2891	rVB7	1968	2139	0.09%	0.013%
63	10.384	2904	2906	2910	rVB5	898	682	0.03%	0.004%
64	10.516	2943	2947	2949	rBV4	951	608	0.02%	0.004%
65	10.635	2979	2984	2987	rBV3	800	651	0.03%	0.004%
66	10.779	3025	3029	3030	rBV3	1086	710	0.03%	0.004%
67	10.799	3033	3035	3038	rVB2	1051	616	0.03%	0.004%
68	10.863	3046	3055	3061	rBV3	2329	3657	0.15%	0.021%
69	10.937	3073	3078	3082	rBV4	709	690	0.03%	0.004%
70	11.024	3100	3105	3107	rBV4	724	635	0.03%	0.004%
71	11.040	3107	3110	3114	rVV2	704	597	0.02%	0.004%
72	11.117	3130	3134	3136	rBV3	1209	815	0.03%	0.005%
73	11.178	3142	3153	3193	rBV	926382	1505447	61.68%	8.839%
74	11.496	3243	3252	3253	rBV7	7667	8579	0.35%	0.050%
75	11.554	3259	3270	3299	rVB	1068378	1720485	70.49%	10.102%
76	11.757	3331	3333	3336	rBV3	1432	674	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037766.D
 Acq On : 08 Oct 2024 14:26
 Operator : SY/MD
 Sample : P4349-02
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.853	3359	3363	3366	rBV5	1253	1231	0.05%	0.007%
78	11.972	3396	3400	3403	rVB5	1325	945	0.04%	0.006%
79	12.004	3408	3410	3415	rVB4	1238	730	0.03%	0.004%
80	12.149	3450	3455	3459	rBV4	893	967	0.04%	0.006%
81	12.175	3459	3463	3465	rVV2	636	509	0.02%	0.003%
82	12.191	3465	3468	3472	rVB3	1198	997	0.04%	0.006%
83	12.275	3492	3494	3499	rVB3	900	656	0.03%	0.004%
84	12.567	3582	3585	3589	rVB4	1259	1028	0.04%	0.006%
85	12.599	3592	3595	3600	rVB3	1073	989	0.04%	0.006%
86	12.657	3610	3613	3616	rBV4	710	568	0.02%	0.003%
87	12.821	3658	3664	3666	rBV4	1208	1031	0.04%	0.006%
88	12.895	3680	3687	3688	rBV5	745	665	0.03%	0.004%
89	12.969	3705	3710	3712	rBV3	722	593	0.02%	0.003%
90	13.085	3743	3746	3749	rVB3	783	569	0.02%	0.003%
91	13.165	3768	3771	3775	rVB2	1135	891	0.04%	0.005%
92	13.194	3775	3780	3781	rBV2	693	515	0.02%	0.003%
93	13.210	3781	3785	3786	rBV2	1087	647	0.03%	0.004%
94	13.220	3786	3788	3799	rVB7	1697	1511	0.06%	0.009%
95	13.458	3859	3862	3864	rBV2	1533	963	0.04%	0.006%
96	13.686	3930	3933	3934	rBV2	1139	613	0.03%	0.004%
97	13.779	3959	3962	3963	rBV2	1075	624	0.03%	0.004%
98	13.975	4017	4023	4024	rBV3	1336	1267	0.05%	0.007%
99	14.670	4235	4239	4242	rBV5	1530	1122	0.05%	0.007%
100	15.364	4453	4455	4457	rBV3	1442	774	0.03%	0.005%




Sum of corrected areas: 17031600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037766.D
Acq On : 08 Oct 2024 14:26
Operator : SY/MD
Sample : P4349-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

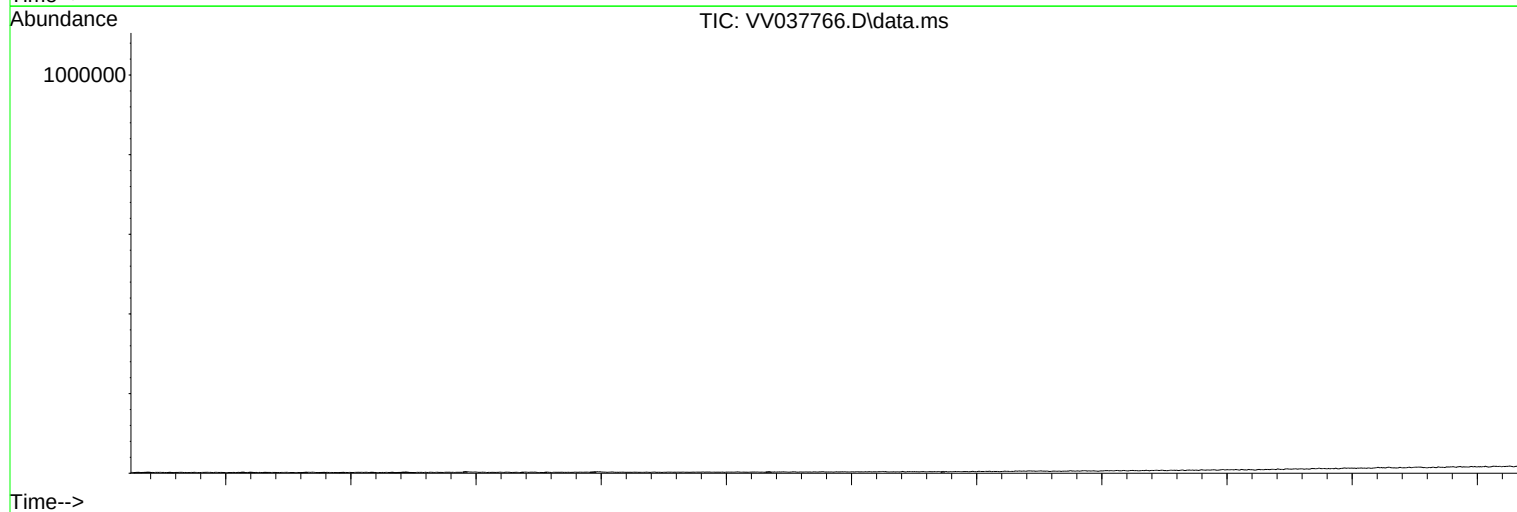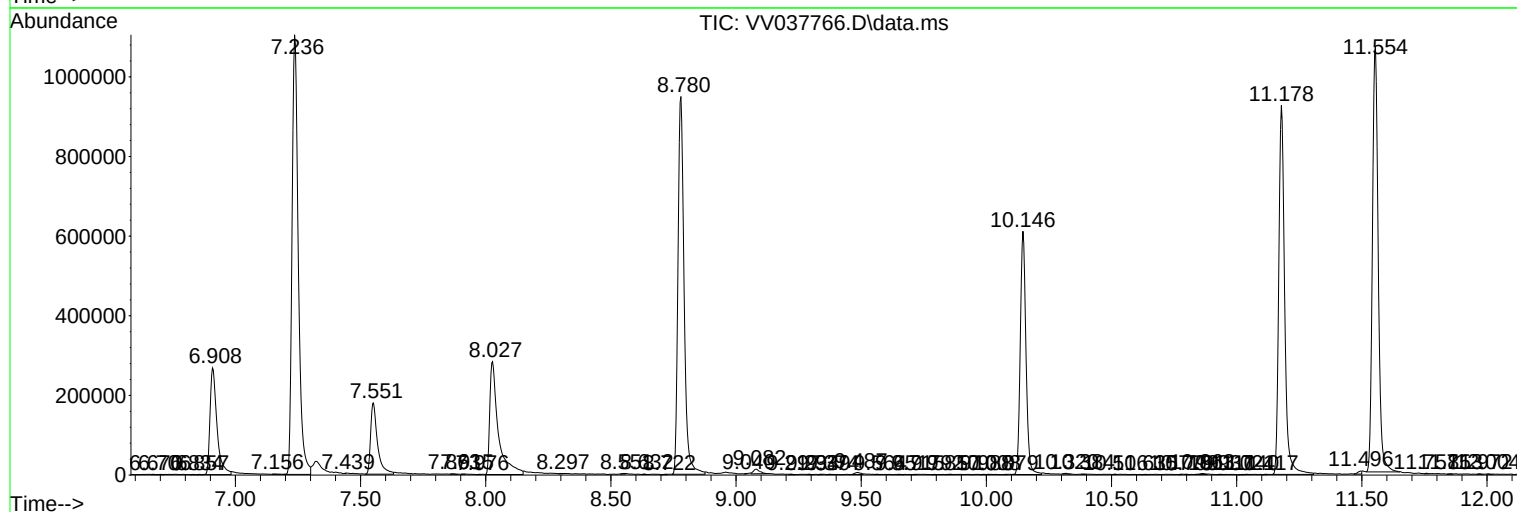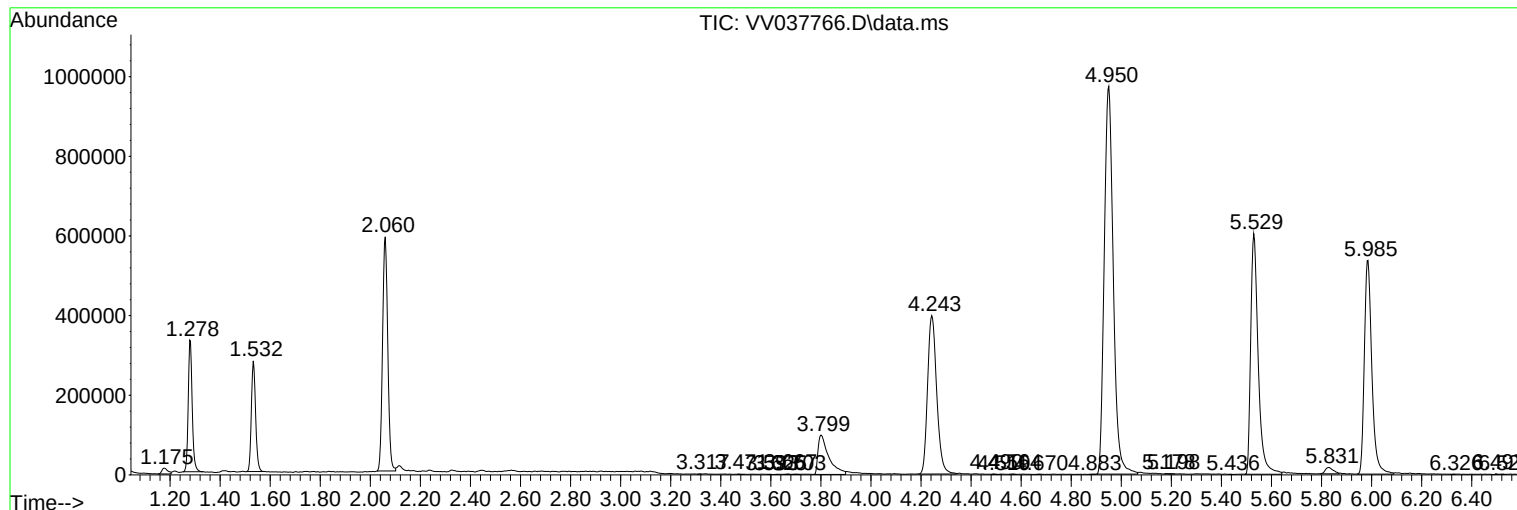

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037766.D
Acq On : 08 Oct 2024 14:26
Operator : SY/MD
Sample : P4349-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037766.D
Acq On : 08 Oct 2024 14:26
Operator : SY/MD
Sample : P4349-02
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------