

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037767.D
 Acq On : 08 Oct 2024 14:47
 Operator : SY/MD
 Sample : P4349-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037767.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.179	37	43	52	rBV	9170	16013	0.64%	0.093%
2	1.282	67	75	92	rVB	340747	379884	15.27%	2.216%
3	1.532	146	153	171	rVB	282159	332953	13.38%	1.942%
4	2.060	308	317	329	rBV	593203	842110	33.84%	4.912%
5	3.323	706	710	719	rVB	19043	16790	0.67%	0.098%
6	3.468	750	755	760	rBV3	967	1119	0.04%	0.007%
7	3.577	785	789	790	rBV3	601	314	0.01%	0.002%
8	3.613	797	800	801	rBV	454	196	0.01%	0.001%
9	3.638	805	808	809	rBV2	626	331	0.01%	0.002%
10	3.674	814	819	821	rBV2	747	539	0.02%	0.003%
11	3.716	828	832	834	rBV3	678	453	0.02%	0.003%
12	3.745	837	841	844	rBV3	738	488	0.02%	0.003%
13	3.761	844	846	848	rBV	285	179	0.01%	0.001%
14	3.799	850	858	894	rBV	102661	305588	12.28%	1.782%
15	4.243	982	996	1023	rBV	401040	995695	40.02%	5.808%
16	4.519	1081	1082	1085	rBV2	395	225	0.01%	0.001%
17	4.603	1106	1108	1115	rVB4	428	323	0.01%	0.002%
18	4.645	1118	1121	1126	rVB4	892	830	0.03%	0.005%
19	4.671	1126	1129	1134	rBV3	882	712	0.03%	0.004%
20	4.693	1134	1136	1138	rBV	469	226	0.01%	0.001%
21	4.725	1144	1146	1149	rBV2	740	517	0.02%	0.003%
22	4.751	1151	1154	1157	rBV3	420	301	0.01%	0.002%
23	4.806	1167	1171	1173	rBV2	323	248	0.01%	0.001%
24	4.822	1173	1176	1177	rBV2	396	277	0.01%	0.002%
25	4.950	1201	1216	1251	rVV2	988309	2488221	100.00%	14.513%
26	5.529	1386	1396	1439	rBV	583138	1229514	49.41%	7.171%
27	5.828	1480	1489	1512	rVB3	17773	41743	1.68%	0.243%
28	5.982	1524	1537	1573	rBV	536574	1136714	45.68%	6.630%
29	6.314	1637	1640	1641	rBV2	465	325	0.01%	0.002%
30	6.343	1647	1649	1651	rBV2	390	170	0.01%	0.001%
31	6.397	1663	1666	1667	rBV2	394	217	0.01%	0.001%
32	6.410	1668	1670	1672	rVB2	695	296	0.01%	0.002%
33	6.426	1672	1675	1678	rBV2	427	289	0.01%	0.002%
34	6.442	1678	1680	1684	rBV2	833	524	0.02%	0.003%
35	6.519	1696	1704	1706	rBV5	1011	1124	0.05%	0.007%
36	6.603	1725	1730	1734	rBV4	620	624	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037767.D
 Acq On : 08 Oct 2024 14:47
 Operator : SY/MD
 Sample : P4349-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.651	1743	1745	1747	rBV2	544	290	0.01%	0.002%
38	6.696	1755	1759	1761	rBV3	684	375	0.02%	0.002%
39	6.722	1765	1767	1768	rVV2	671	282	0.01%	0.002%
40	6.732	1768	1770	1772	rVV3	994	561	0.02%	0.003%
41	6.760	1775	1779	1782	rBV4	533	524	0.02%	0.003%
42	6.857	1806	1809	1814	rBV4	388	276	0.01%	0.002%
43	6.908	1814	1825	1853	rBV	266681	521646	20.96%	3.043%
44	7.236	1916	1927	1947	rBV	1103597	1956459	78.63%	11.412%
45	7.548	2016	2024	2055	rBV	180809	346296	13.92%	2.020%
46	7.912	2134	2137	2141	rVB5	1104	674	0.03%	0.004%
47	7.992	2160	2162	2164	rBV2	762	461	0.02%	0.003%
48	8.027	2164	2173	2214	rBV2	293783	679228	27.30%	3.962%
49	8.722	2386	2389	2392	rVB3	1080	576	0.02%	0.003%
50	8.780	2395	2407	2442	rBV	949996	1594893	64.10%	9.303%
51	9.265	2555	2558	2563	rBV6	824	865	0.03%	0.005%
52	9.291	2563	2566	2569	rVV2	1030	682	0.03%	0.004%
53	9.317	2572	2574	2576	rBV	429	209	0.01%	0.001%
54	9.333	2576	2579	2581	rBV3	787	375	0.02%	0.002%
55	9.365	2587	2589	2590	rBV	451	199	0.01%	0.001%
56	9.452	2612	2616	2617	rBV2	709	470	0.02%	0.003%
57	9.487	2620	2627	2637	rVV6	5135	8441	0.34%	0.049%
58	9.603	2657	2663	2664	rBV4	795	597	0.02%	0.003%
59	9.622	2668	2669	2671	rBV	796	306	0.01%	0.002%
60	9.683	2685	2688	2691	rVB3	925	535	0.02%	0.003%
61	9.706	2691	2695	2699	rBV3	1020	1090	0.04%	0.006%
62	9.760	2709	2712	2715	rBV3	557	328	0.01%	0.002%
63	9.783	2715	2719	2720	rBV3	844	583	0.02%	0.003%
64	9.825	2729	2732	2735	rBV2	746	377	0.02%	0.002%
65	9.866	2740	2745	2746	rBV	705	594	0.02%	0.003%
66	9.905	2755	2757	2760	rVB	517	212	0.01%	0.001%
67	9.921	2760	2762	2763	rBV	616	292	0.01%	0.002%
68	9.957	2771	2773	2778	rVB2	577	448	0.02%	0.003%
69	9.979	2778	2780	2782	rVB2	433	173	0.01%	0.001%
70	9.995	2782	2785	2787	rBV3	642	530	0.02%	0.003%
71	10.066	2804	2807	2810	rBV3	592	433	0.02%	0.003%
72	10.146	2820	2832	2857	rBV	612729	976168	39.23%	5.694%
73	10.468	2927	2932	2933	rBV4	612	478	0.02%	0.003%
74	10.481	2933	2936	2938	rBV2	633	443	0.02%	0.003%
75	10.522	2946	2949	2950	rBV2	808	427	0.02%	0.002%
76	10.612	2973	2977	2980	rBV2	959	760	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037767.D
 Acq On : 08 Oct 2024 14:47
 Operator : SY/MD
 Sample : P4349-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH5

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.625	2980	2981	2984	rBV3	469	296	0.01%	0.002%
78	10.719	3008	3010	3014	rVB2	595	361	0.01%	0.002%
79	10.744	3014	3018	3021	rBV2	704	501	0.02%	0.003%
80	10.860	3046	3054	3058	rBV8	2441	3562	0.14%	0.021%
81	10.953	3080	3083	3085	rBV	628	432	0.02%	0.003%
82	11.027	3104	3106	3108	rBV2	287	188	0.01%	0.001%
83	11.085	3121	3124	3125	rBV	582	283	0.01%	0.002%
84	11.095	3125	3127	3130	rVB2	730	319	0.01%	0.002%
85	11.124	3133	3136	3137	rBV	561	270	0.01%	0.002%
86	11.178	3142	3153	3186	rBV	927577	1484337	59.65%	8.658%
87	11.555	3259	3270	3298	rBV	1078198	1752318	70.42%	10.221%
88	12.108	3440	3442	3446	rBV3	608	262	0.01%	0.002%
89	12.490	3559	3561	3565	rVB3	777	326	0.01%	0.002%
90	12.513	3565	3568	3573	rBV4	1083	905	0.04%	0.005%
91	12.622	3600	3602	3604	rBV	361	201	0.01%	0.001%
92	12.712	3627	3630	3633	rBV4	875	488	0.02%	0.003%
93	12.792	3653	3655	3657	rBV	605	371	0.01%	0.002%
94	12.947	3701	3703	3706	rBV	664	260	0.01%	0.002%
95	12.963	3706	3708	3710	rBV2	842	454	0.02%	0.003%
96	13.056	3734	3737	3740	rBV3	866	679	0.03%	0.004%
97	13.271	3799	3804	3806	rBV3	1084	1002	0.04%	0.006%
98	13.297	3810	3812	3815	rBV4	790	555	0.02%	0.003%
99	13.339	3819	3825	3826	rBV4	836	837	0.03%	0.005%
100	13.860	3984	3987	3989	rBV	1083	682	0.03%	0.004%

Sum of corrected areas: 17144517




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037767.D
Acq On : 08 Oct 2024 14:47
Operator : SY/MD
Sample : P4349-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L

TIC Integration Parameters: LSCINT.P

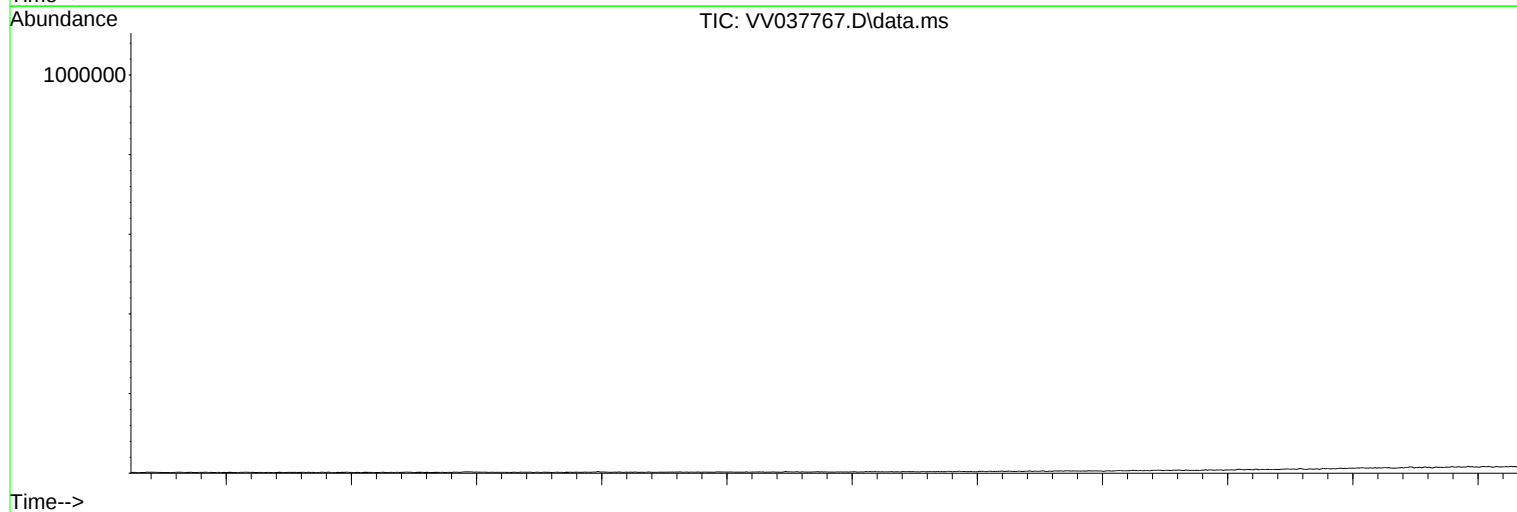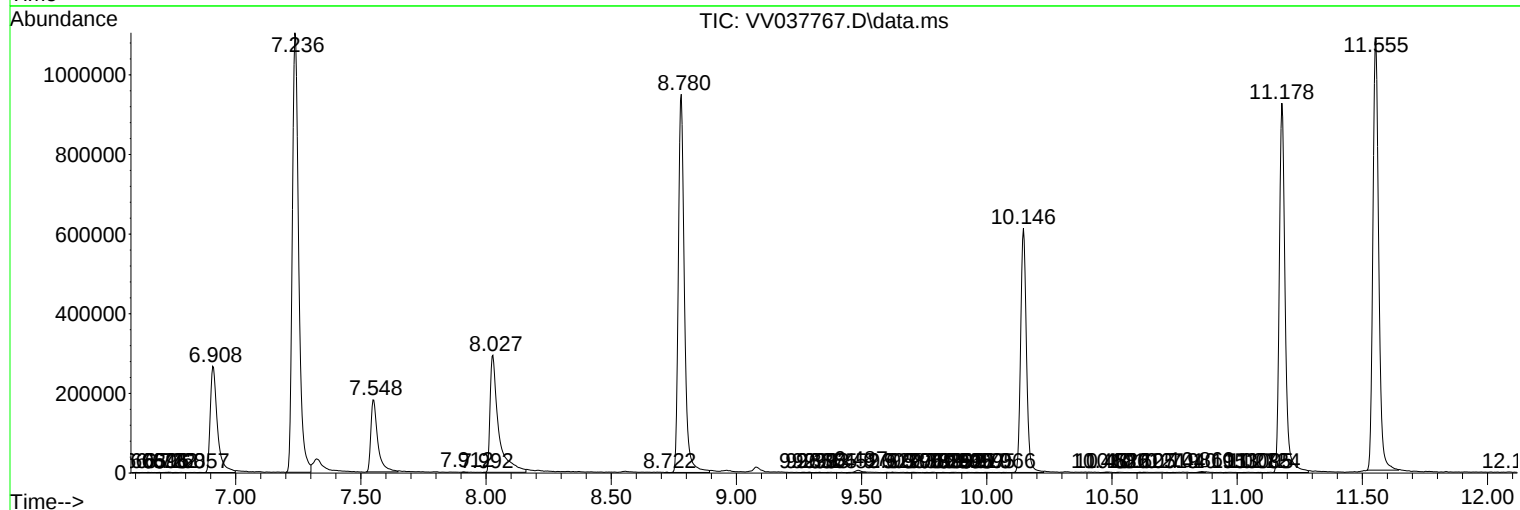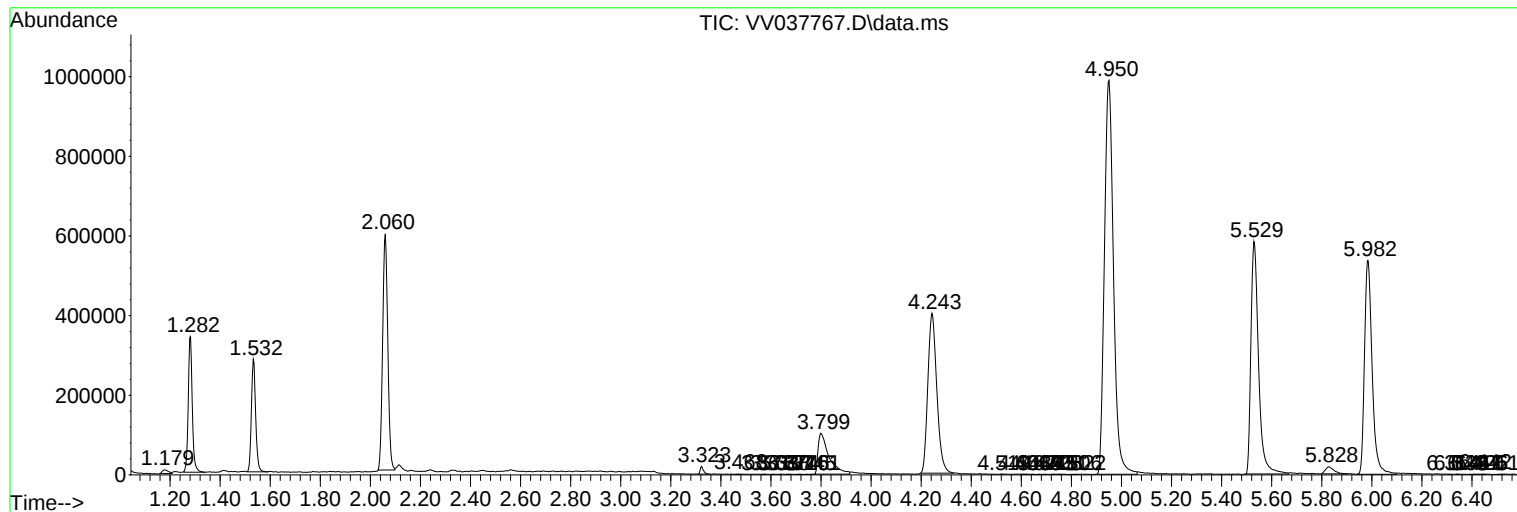

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037767.D
Acq On : 08 Oct 2024 14:47
Operator : SY/MD
Sample : P4349-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037767.D
Acq On : 08 Oct 2024 14:47
Operator : SY/MD
Sample : P4349-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------