

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037770.D
 Acq On : 08 Oct 2024 15:52
 Operator : SY/MD
 Sample : P4346-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037770.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	51	rBV2	6876	12578	0.51%	0.074%
2	1.282	68	75	90	rBV	331317	350661	14.31%	2.057%
3	1.532	146	153	166	rVB	270875	323776	13.22%	1.899%
4	2.060	307	317	332	rBV	589835	841707	34.36%	4.938%
5	3.237	680	683	686	rBV3	900	548	0.02%	0.003%
6	3.375	724	726	729	rVB2	965	562	0.02%	0.003%
7	3.397	729	733	735	rBV2	915	793	0.03%	0.005%
8	3.542	775	778	783	rVB4	764	538	0.02%	0.003%
9	3.635	806	807	811	rBV3	762	431	0.02%	0.003%
10	3.799	850	858	897	rBV	103623	304244	12.42%	1.785%
11	4.243	977	996	1023	rBV2	394922	1003774	40.97%	5.888%
12	4.407	1045	1047	1051	rVB3	920	469	0.02%	0.003%
13	4.555	1089	1093	1096	rVB4	516	448	0.02%	0.003%
14	4.606	1107	1109	1113	rBV2	510	500	0.02%	0.003%
15	4.638	1115	1119	1122	rVV4	830	676	0.03%	0.004%
16	4.709	1137	1141	1142	rBV	1042	636	0.03%	0.004%
17	4.719	1142	1144	1149	rVV4	797	637	0.03%	0.004%
18	4.764	1152	1158	1162	rVB5	1200	1377	0.06%	0.008%
19	4.789	1162	1166	1172	rBV3	946	1140	0.05%	0.007%
20	4.844	1180	1183	1185	rBV3	699	446	0.02%	0.003%
21	4.950	1198	1216	1250	rBV2	974772	2449748	100.00%	14.371%
22	5.217	1293	1299	1301	rBV5	1415	1461	0.06%	0.009%
23	5.397	1352	1355	1357	rVV4	906	527	0.02%	0.003%
24	5.529	1383	1396	1427	rBV	587771	1226471	50.07%	7.195%
25	5.828	1480	1489	1508	rVB5	14269	32385	1.32%	0.190%
26	5.986	1525	1538	1566	rBV	540100	1113369	45.45%	6.531%
27	6.333	1645	1646	1649	rVB2	1020	423	0.02%	0.002%
28	6.355	1649	1653	1655	rBV2	695	493	0.02%	0.003%
29	6.368	1655	1657	1660	rBV3	683	417	0.02%	0.002%
30	6.423	1669	1674	1675	rBV3	586	422	0.02%	0.002%
31	6.433	1675	1677	1682	rVB3	1109	618	0.03%	0.004%
32	6.461	1682	1686	1688	rBV3	970	611	0.02%	0.004%
33	6.503	1697	1699	1704	rVB4	701	478	0.02%	0.003%
34	6.632	1737	1739	1745	rBV4	936	889	0.04%	0.005%
35	6.783	1782	1786	1791	rBV5	604	554	0.02%	0.003%
36	6.908	1815	1825	1860	rBV	266695	527631	21.54%	3.095%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037770.D
 Acq On : 08 Oct 2024 15:52
 Operator : SY/MD
 Sample : P4346-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.185	1909	1911	1914	rBV3	987	549	0.02%	0.003%
38	7.236	1916	1927	1961	rBV	1087306	1950687	79.63%	11.443%
39	7.551	2016	2025	2046	rBV	177120	333871	13.63%	1.959%
40	7.799	2097	2102	2107	rVB6	1203	981	0.04%	0.006%
41	7.915	2136	2138	2144	rVB4	867	725	0.03%	0.004%
42	7.969	2152	2155	2157	rBV3	775	494	0.02%	0.003%
43	8.027	2164	2173	2210	rBV2	309876	702524	28.68%	4.121%
44	8.500	2318	2320	2324	rBV5	607	457	0.02%	0.003%
45	8.558	2333	2338	2343	rBV7	2081	1738	0.07%	0.010%
46	8.622	2355	2358	2363	rVB6	775	554	0.02%	0.003%
47	8.780	2396	2407	2438	rBV	956501	1589026	64.86%	9.322%
48	9.149	2519	2522	2526	rBV4	1016	818	0.03%	0.005%
49	9.288	2564	2565	2569	rVV2	845	436	0.02%	0.003%
50	9.310	2569	2572	2578	rVB4	1290	1108	0.05%	0.006%
51	9.545	2643	2645	2651	rVB4	847	565	0.02%	0.003%
52	9.632	2665	2672	2674	rBV5	908	782	0.03%	0.005%
53	9.738	2699	2705	2708	rBV4	1155	990	0.04%	0.006%
54	9.870	2743	2746	2748	rBV3	775	475	0.02%	0.003%
55	9.892	2748	2753	2756	rBV5	590	667	0.03%	0.004%
56	9.937	2765	2767	2770	rVB3	847	410	0.02%	0.002%
57	9.989	2779	2783	2784	rBV3	751	480	0.02%	0.003%
58	10.088	2810	2814	2820	rVB4	636	643	0.03%	0.004%
59	10.146	2820	2832	2861	rBV	619376	995285	40.63%	5.839%
60	10.313	2880	2884	2886	rBV5	1185	822	0.03%	0.005%
61	10.333	2886	2890	2896	rVV6	1105	1315	0.05%	0.008%
62	10.381	2902	2905	2908	rBV3	527	517	0.02%	0.003%
63	10.497	2938	2941	2944	rBV4	747	480	0.02%	0.003%
64	10.786	3023	3031	3034	rBV4	729	817	0.03%	0.005%
65	10.825	3039	3043	3046	rBV3	835	712	0.03%	0.004%
66	10.882	3056	3061	3065	rVB3	641	664	0.03%	0.004%
67	10.960	3078	3085	3086	rBV3	735	554	0.02%	0.003%
68	11.120	3133	3135	3137	rBV2	854	475	0.02%	0.003%
69	11.178	3142	3153	3190	rBV	907035	1478773	60.36%	8.675%
70	11.426	3227	3230	3233	rBV4	1279	823	0.03%	0.005%
71	11.445	3234	3236	3239	rVB3	1321	586	0.02%	0.003%
72	11.554	3258	3270	3302	rBV	1062605	1752322	71.53%	10.280%
73	11.956	3391	3395	3398	rBV4	1226	1130	0.05%	0.007%
74	11.982	3401	3403	3405	rVV3	928	424	0.02%	0.002%
75	12.030	3416	3418	3429	rVB8	1636	2259	0.09%	0.013%
76	12.079	3430	3433	3435	rBV	778	515	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037770.D
 Acq On : 08 Oct 2024 15:52
 Operator : SY/MD
 Sample : P4346-22
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.390	3528	3530	3537	rVB5	833	672	0.03%	0.004%
78	12.426	3537	3541	3543	rBV4	552	416	0.02%	0.002%
79	12.497	3558	3563	3567	rVB3	890	772	0.03%	0.005%
80	12.529	3567	3573	3574	rBV3	1017	831	0.03%	0.005%
81	12.628	3600	3604	3606	rBV2	781	558	0.02%	0.003%
82	12.792	3651	3655	3657	rVB3	666	441	0.02%	0.003%
83	12.850	3670	3673	3678	rBV4	1119	1025	0.04%	0.006%
84	13.043	3728	3733	3734	rBV3	621	551	0.02%	0.003%
85	13.169	3770	3772	3778	rVB3	808	604	0.02%	0.004%
86	13.217	3783	3787	3792	rBV6	960	792	0.03%	0.005%
87	13.390	3837	3841	3846	rBV2	797	762	0.03%	0.004%
88	13.429	3846	3853	3854	rBV4	795	804	0.03%	0.005%
89	13.471	3863	3866	3870	rVB4	972	586	0.02%	0.003%
90	13.542	3886	3888	3892	rBV2	520	433	0.02%	0.003%
91	13.779	3960	3962	3966	rBV2	663	469	0.02%	0.003%
92	13.934	4007	4010	4012	rVB3	1136	668	0.03%	0.004%
93	13.953	4012	4016	4017	rBV3	684	451	0.02%	0.003%
94	14.014	4032	4035	4038	rBV3	600	441	0.02%	0.003%
95	14.056	4046	4048	4052	rBV3	635	477	0.02%	0.003%
96	14.130	4067	4071	4074	rBV4	988	952	0.04%	0.006%
97	14.545	4196	4200	4202	rBV3	895	587	0.02%	0.003%
98	14.677	4238	4241	4244	rVB4	1431	792	0.03%	0.005%
99	14.696	4244	4247	4251	rBV4	907	611	0.02%	0.004%
100	14.924	4315	4318	4325	rBV5	1221	1835	0.07%	0.011%




Sum of corrected areas: 17046421

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037770.D
Acq On : 08 Oct 2024 15:52
Operator : SY/MD
Sample : P4346-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

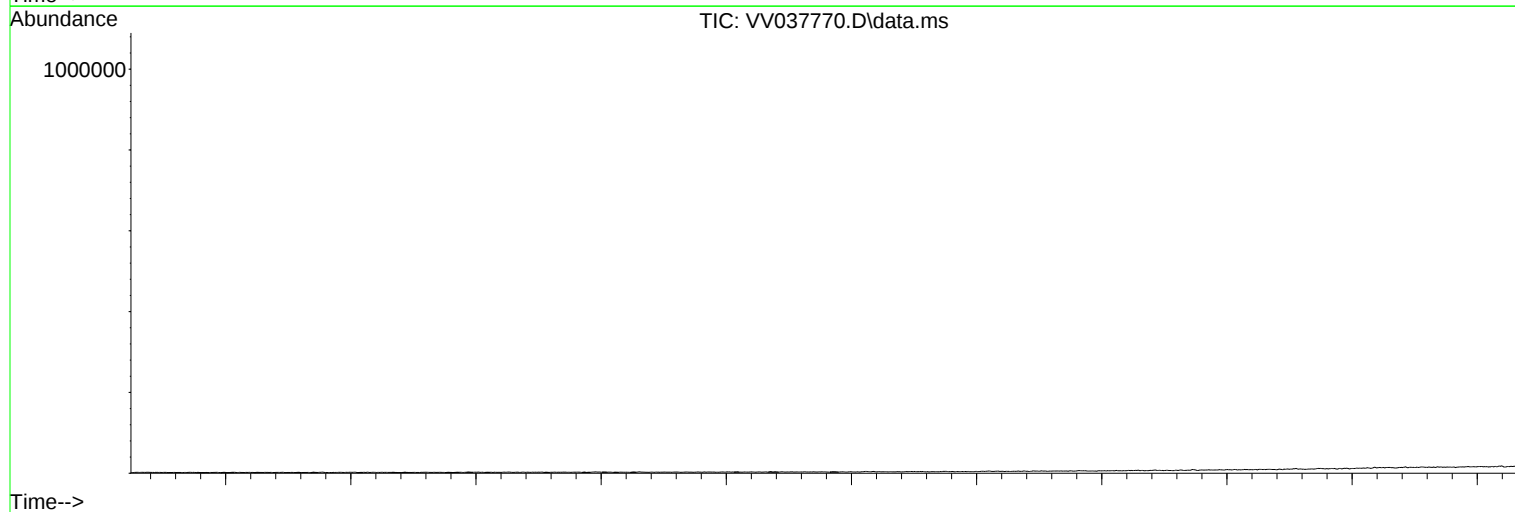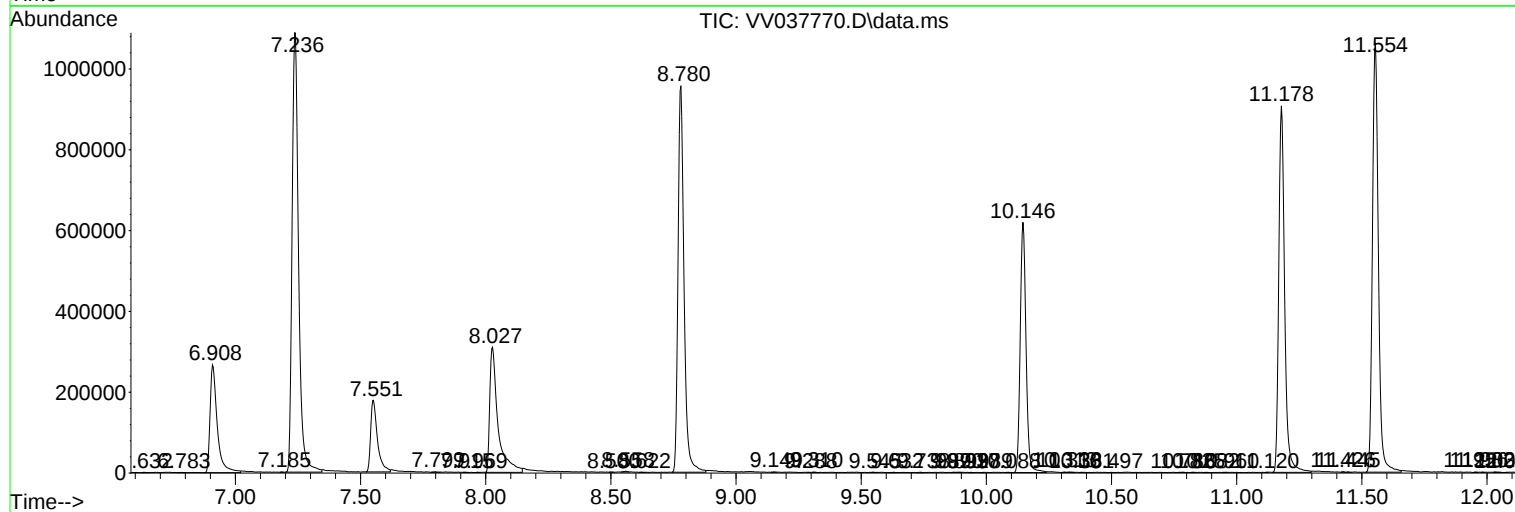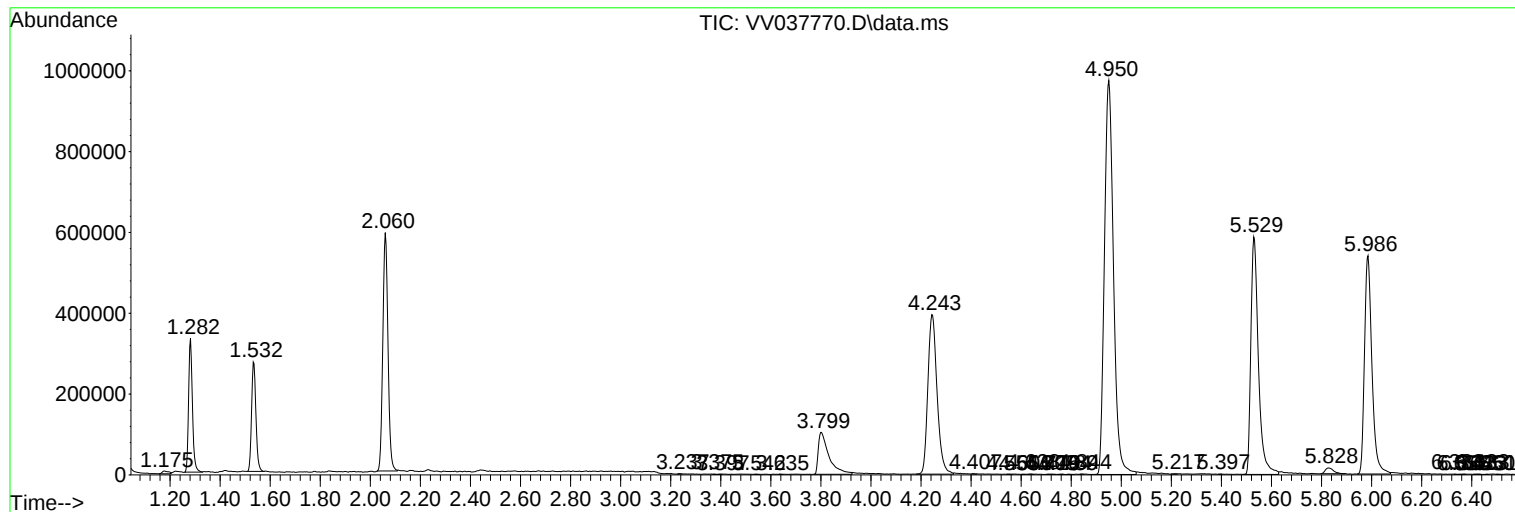

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037770.D
Acq On : 08 Oct 2024 15:52
Operator : SY/MD
Sample : P4346-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037770.D
Acq On : 08 Oct 2024 15:52
Operator : SY/MD
Sample : P4346-22
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc