

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037771.D
 Acq On : 08 Oct 2024 16:14
 Operator : SY/MD
 Sample : P4329-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037771.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	88	rVB	323419	340193	14.59%	2.096%
2	1.532	146	153	169	rVB	270438	318159	13.65%	1.961%
3	2.060	307	317	330	rBV	560760	810340	34.76%	4.994%
4	3.333	710	713	717	rBV4	620	371	0.02%	0.002%
5	3.539	776	777	778	rBV4	432	142	0.01%	0.001%
6	3.671	814	818	821	rBV3	664	383	0.02%	0.002%
7	3.728	834	836	837	rBV2	233	79	0.00%	0.000%
8	3.741	838	840	844	rBV3	535	382	0.02%	0.002%
9	3.770	846	849	850	rBV	663	389	0.02%	0.002%
10	3.799	850	858	892	rBV	95630	271936	11.66%	1.676%
11	4.243	978	996	1023	rBV	383880	970327	41.62%	5.980%
12	4.494	1071	1074	1081	rVB4	961	1033	0.04%	0.006%
13	4.545	1081	1090	1092	rBV4	961	1372	0.06%	0.008%
14	4.564	1092	1096	1100	rBV5	829	752	0.03%	0.005%
15	4.616	1109	1112	1113	rBV2	359	235	0.01%	0.001%
16	4.651	1120	1123	1126	rBV3	496	356	0.02%	0.002%
17	4.683	1130	1133	1134	rBV	767	423	0.02%	0.003%
18	4.738	1145	1150	1151	rBV	663	596	0.03%	0.004%
19	4.767	1157	1159	1161	rBV	339	160	0.01%	0.001%
20	4.793	1165	1167	1169	rBV2	468	248	0.01%	0.002%
21	4.825	1174	1177	1181	rVB2	413	281	0.01%	0.002%
22	4.863	1185	1189	1190	rBV4	661	405	0.02%	0.002%
23	4.950	1201	1216	1248	rBV2	936875	2331223	100.00%	14.366%
24	5.397	1353	1355	1357	rBV2	477	220	0.01%	0.001%
25	5.529	1385	1396	1425	rBV	569088	1188655	50.99%	7.325%
26	5.931	1519	1521	1522	rBV2	583	145	0.01%	0.001%
27	5.982	1525	1537	1569	rVV	513439	1068459	45.83%	6.584%
28	6.397	1662	1666	1667	rBV2	732	468	0.02%	0.003%
29	6.420	1671	1673	1677	rBV3	787	489	0.02%	0.003%
30	6.439	1677	1679	1682	rBV3	533	351	0.02%	0.002%
31	6.478	1688	1691	1692	rBV	409	226	0.01%	0.001%
32	6.574	1718	1721	1724	rVB3	539	267	0.01%	0.002%
33	6.609	1729	1732	1733	rBV2	547	260	0.01%	0.002%
34	6.642	1741	1742	1744	rBV2	352	161	0.01%	0.001%
35	6.654	1744	1746	1752	rVB3	472	424	0.02%	0.003%
36	6.680	1752	1754	1755	rBV2	590	230	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037771.D
 Acq On : 08 Oct 2024 16:14
 Operator : SY/MD
 Sample : P4329-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.744	1772	1774	1777	rBV4	844	375	0.02%	0.002%
38	6.822	1795	1798	1800	rBV2	445	335	0.01%	0.002%
39	6.867	1809	1812	1815	rBV4	646	447	0.02%	0.003%
40	6.908	1815	1825	1853	rBV	253845	495479	21.25%	3.053%
41	7.162	1899	1904	1907	rBV3	937	914	0.04%	0.006%
42	7.236	1916	1927	1954	rBV	1049201	1848295	79.28%	11.390%
43	7.551	2015	2025	2053	rBV	169735	326221	13.99%	2.010%
44	7.957	2149	2151	2156	rVB3	1026	512	0.02%	0.003%
45	7.979	2156	2158	2159	rBV2	514	192	0.01%	0.001%
46	8.027	2164	2173	2221	rBV2	276409	653199	28.02%	4.025%
47	8.625	2357	2359	2363	rBV3	714	608	0.03%	0.004%
48	8.715	2385	2387	2389	rBV3	601	337	0.01%	0.002%
49	8.780	2396	2407	2440	rBV	943333	1556687	66.78%	9.593%
50	9.178	2528	2531	2533	rBV4	857	472	0.02%	0.003%
51	9.384	2594	2595	2596	rBV	517	132	0.01%	0.001%
52	9.410	2601	2603	2606	rBV3	574	324	0.01%	0.002%
53	9.468	2619	2621	2625	rVB2	864	480	0.02%	0.003%
54	9.506	2629	2633	2637	rBV4	661	704	0.03%	0.004%
55	9.561	2648	2650	2655	rBV2	424	334	0.01%	0.002%
56	9.641	2672	2675	2676	rBV	249	149	0.01%	0.001%
57	9.651	2676	2678	2681	rVB2	479	235	0.01%	0.001%
58	9.773	2712	2716	2719	rBV3	739	505	0.02%	0.003%
59	9.789	2719	2721	2725	rVB3	590	404	0.02%	0.002%
60	9.870	2743	2746	2747	rBV2	894	442	0.02%	0.003%
61	9.963	2774	2775	2776	rBV	198	64	0.00%	0.000%
62	10.082	2810	2812	2814	rBV2	626	329	0.01%	0.002%
63	10.146	2821	2832	2854	rBV	585358	931886	39.97%	5.743%
64	10.362	2897	2899	2901	rBV2	459	245	0.01%	0.002%
65	10.448	2921	2926	2928	rBV4	806	740	0.03%	0.005%
66	10.493	2938	2940	2944	rVB3	685	244	0.01%	0.002%
67	10.702	3000	3005	3008	rBV3	830	819	0.04%	0.005%
68	10.751	3018	3020	3022	rBV3	384	204	0.01%	0.001%
69	10.847	3047	3050	3053	rVB2	456	275	0.01%	0.002%
70	10.876	3053	3059	3063	rBV5	733	630	0.03%	0.004%
71	10.892	3063	3064	3065	rBV	315	102	0.00%	0.001%
72	10.973	3087	3089	3091	rVB2	512	208	0.01%	0.001%
73	10.985	3091	3093	3094	rBV	524	208	0.01%	0.001%
74	10.995	3094	3096	3099	rVB3	485	297	0.01%	0.002%
75	11.053	3112	3114	3115	rBV3	260	107	0.00%	0.001%
76	11.085	3121	3124	3129	rBV3	623	398	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
 Data File : VV037771.D
 Acq On : 08 Oct 2024 16:14
 Operator : SY/MD
 Sample : P4329-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK002

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.130	3135	3138	3141	rVB5	1063	637	0.03%	0.004%
78	11.178	3142	3153	3182	rBV	887307	1435796	61.59%	8.848%
79	11.555	3258	3270	3301	rBV	1011709	1648792	70.73%	10.161%
80	11.956	3389	3395	3396	rBV3	922	840	0.04%	0.005%
81	12.024	3414	3416	3420	rBV3	713	350	0.02%	0.002%
82	12.046	3421	3423	3426	rVB3	872	411	0.02%	0.003%
83	12.127	3443	3448	3451	rVB2	819	629	0.03%	0.004%
84	12.281	3494	3496	3499	rBV2	841	585	0.03%	0.004%
85	12.448	3547	3548	3552	rBV2	512	370	0.02%	0.002%
86	12.667	3612	3616	3618	rBV5	716	493	0.02%	0.003%
87	12.882	3678	3683	3684	rBV2	885	717	0.03%	0.004%
88	12.953	3704	3705	3707	rBV2	633	341	0.01%	0.002%
89	13.207	3778	3784	3787	rBV3	837	986	0.04%	0.006%
90	13.239	3792	3794	3797	rVB2	677	322	0.01%	0.002%
91	13.384	3836	3839	3844	rBV4	1354	1298	0.06%	0.008%




Sum of corrected areas: 16227245

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037771.D
Acq On : 08 Oct 2024 16:14
Operator : SY/MD
Sample : P4329-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

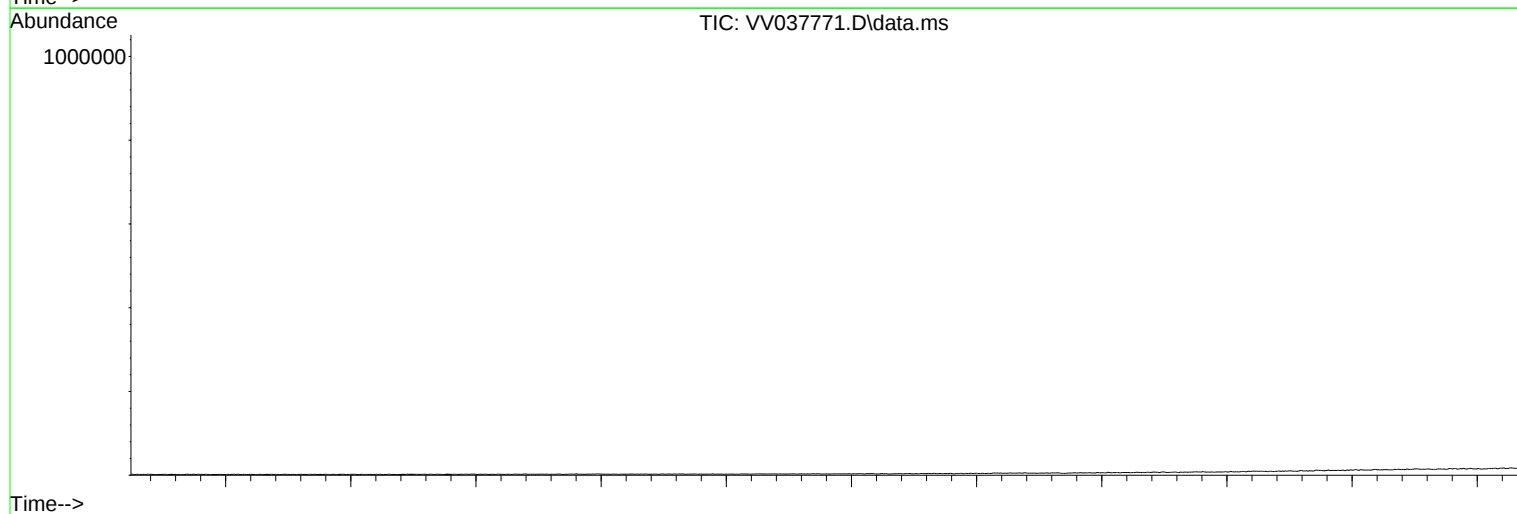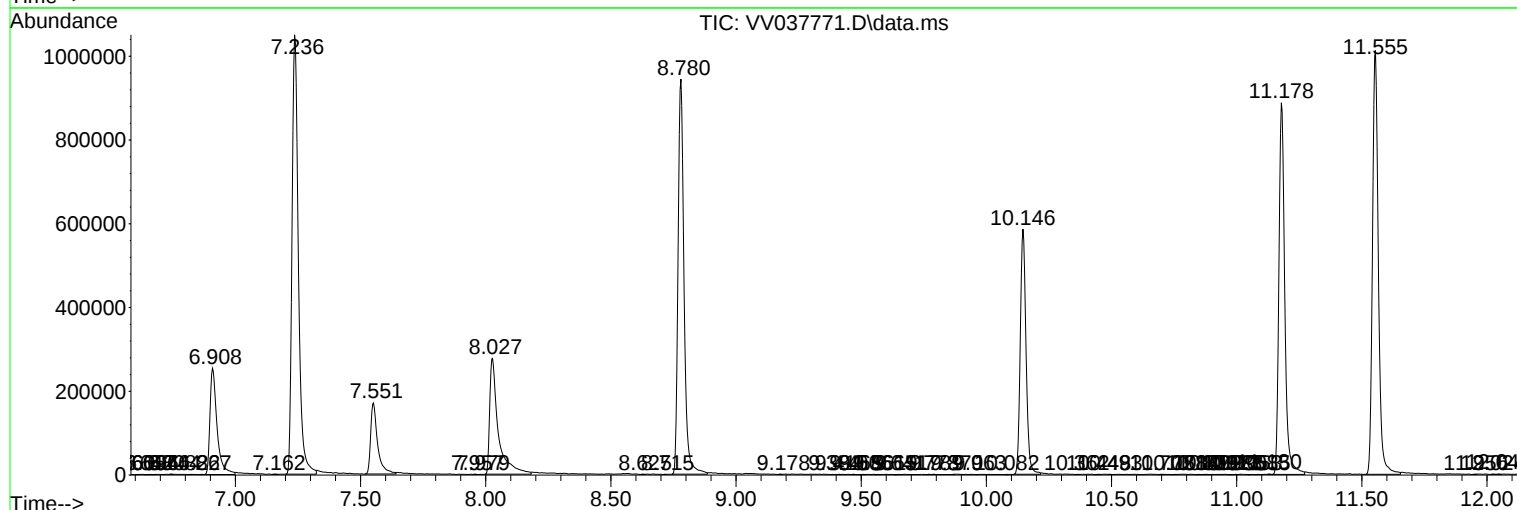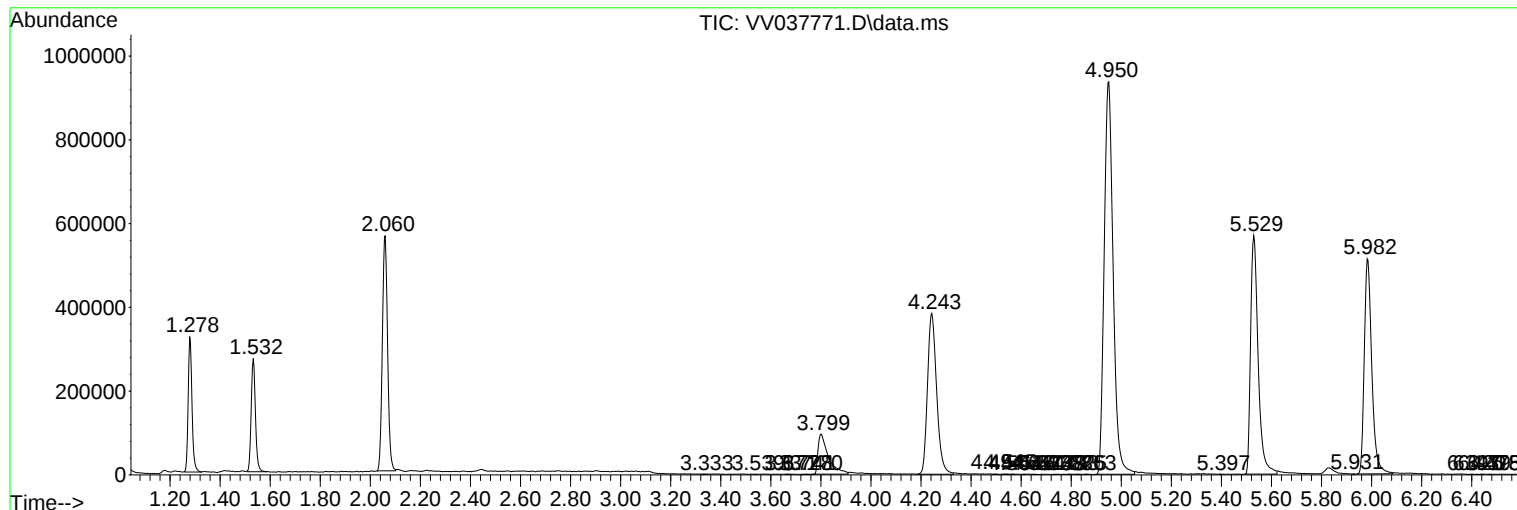

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037771.D
Acq On : 08 Oct 2024 16:14
Operator : SY/MD
Sample : P4329-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037771.D
Acq On : 08 Oct 2024 16:14
Operator : SY/MD
Sample : P4329-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK002

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------