
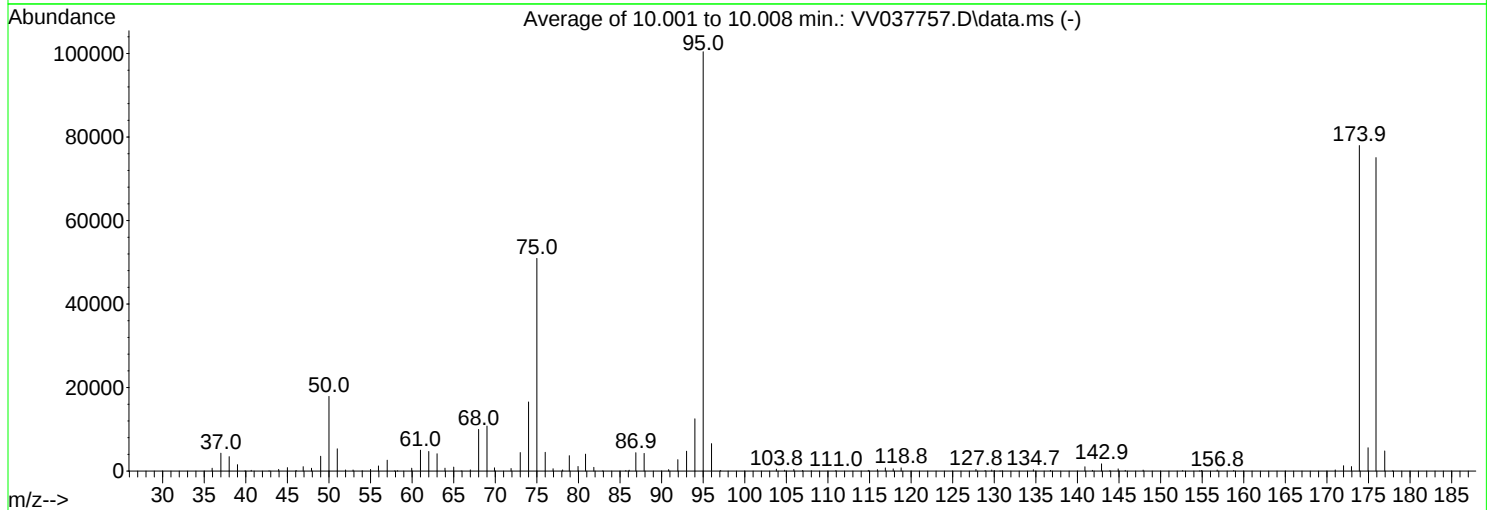


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100824\
Data File : VV037757.D
Acq On : 08 Oct 2024 08:00
Operator : SY/MD
Sample : BFB389
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB389

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Wed Oct 09 05:07:27 2024

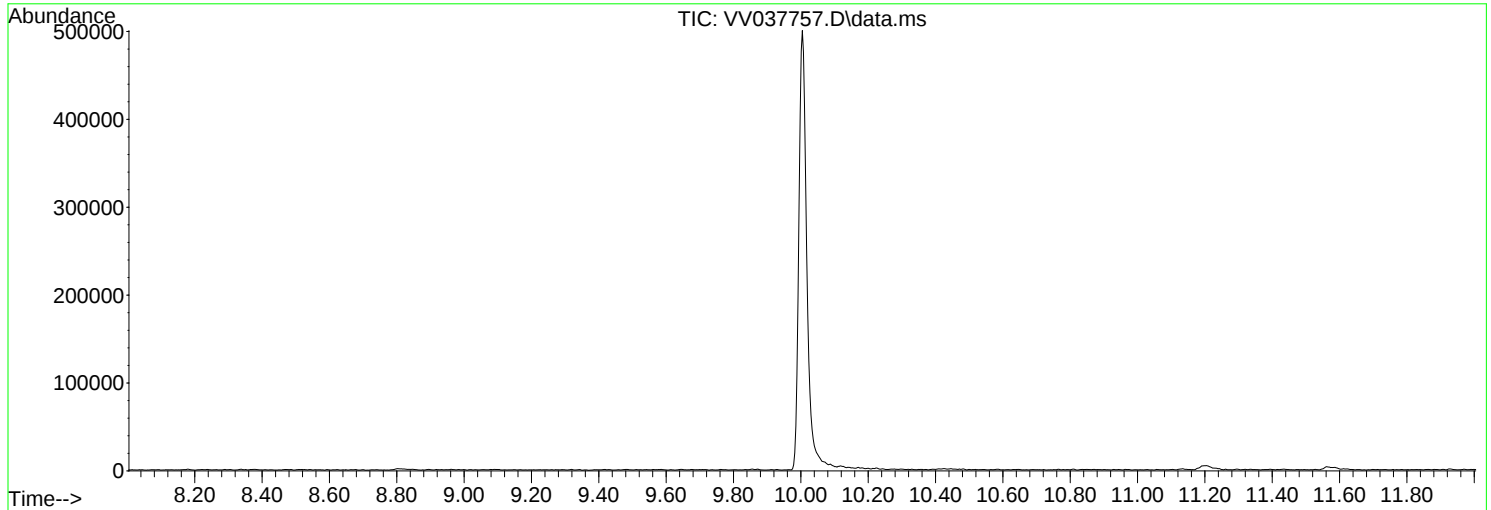

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	17891	PASS
75	95	30	80	50.7	50941	PASS
95	95	100	100	100.0	100429	PASS
96	95	5	9	6.6	6580	PASS
173	174	0.00	2	1.4	1078	PASS
174	95	50	120	77.6	77968	PASS
175	174	5	9	7.2	5595	PASS
176	174	95	105	96.3	75075	PASS
177	176	5	10	6.4	4813	PASS

m/z	Abundance
40.00	387.0
43.90	716.0
77.10	107.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
35.90	718.0
37.00	4260.0
38.00	3350.0
39.00	1640.0
39.90	407.0
40.70	147.0
42.80	110.0
44.00	1256.0
45.00	890.0
46.00	181.0
46.90	1000.0
47.90	708.0
49.00	3499.0
50.00	18136.0
51.00	5333.0
52.10	247.0
52.90	217.0
55.00	317.0
56.00	1361.0
57.00	2611.0
57.90	140.0
59.90	645.0
61.00	5268.0
62.00	4652.0
63.00	4181.0
63.90	683.0
65.00	896.0
65.90	114.0
67.00	337.0
68.00	9847.0
69.00	11249.0
69.90	749.0
71.90	558.0
73.00	4560.0
74.00	16480.0
75.00	50864.0
76.00	4674.0
77.00	629.0
78.90	3659.0
79.90	1074.0
80.90	4075.0
81.90	744.0
82.90	112.0
86.10	237.0
86.90	4242.0
87.90	4279.0
90.90	344.0
92.00	2990.0
93.00	4668.0
94.00	12188.0
95.00	99256.0
96.00	6644.0
97.10	137.0
103.80	477.0
104.90	218.0
105.80	384.0
107.00	116.0
111.00	119.0
114.80	133.0
115.90	417.0
116.90	793.0
117.80	589.0
118.80	744.0
127.80	341.0
128.90	132.0
130.00	343.0
130.70	145.0
134.70	341.0
136.80	124.0
140.90	1051.0
141.80	117.0
142.90	1589.0
143.90	122.0
144.90	502.0
145.70	171.0
147.90	247.0
152.70	130.0
154.70	179.0
156.80	301.0
158.80	178.0
171.00	283.0
172.00	1284.0
173.00	990.0
173.90	75456.0
174.90	5538.0
175.90	71288.0
176.90	5009.0
177.90	133.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
35.90	710.0
37.00	4454.0
38.00	3642.0
39.00	1556.0
39.90	432.0
40.60	180.0
42.80	112.0
44.00	1127.0
45.00	862.0
46.00	142.0
46.90	1066.0
47.90	744.0
49.00	3645.0
50.00	18528.0
51.00	5475.0
52.00	241.0
52.90	286.0
55.00	441.0
56.00	1260.0
57.00	2641.0
58.20	121.0
60.00	689.0
61.00	5193.0
62.00	4770.0
63.00	4293.0
63.90	720.0
65.00	994.0
67.00	275.0
68.00	10421.0
69.00	11088.0
69.90	807.0
71.90	674.0
73.00	4556.0
74.00	17128.0
75.00	52544.0
76.00	4661.0
76.90	711.0
78.10	429.0
78.90	3740.0
80.00	1147.0
80.90	4133.0
81.80	918.0
85.70	192.0
86.10	252.0
86.90	4552.0
87.90	4338.0
90.80	363.0
91.90	2853.0
93.00	4988.0
94.00	13022.0
95.00	103592.0
96.00	6764.0
97.10	133.0
103.80	508.0
104.80	230.0
105.90	403.0
106.90	147.0
108.00	102.0
110.90	111.0
114.80	171.0
116.00	362.0
116.90	809.0
117.80	560.0
118.80	804.0
127.80	399.0
128.90	155.0
129.70	373.0
131.00	125.0
134.70	363.0
136.80	164.0
140.90	1080.0
141.80	174.0
142.90	1755.0
143.90	107.0
144.90	547.0
145.70	162.0
147.90	253.0
152.70	121.0
154.90	198.0
156.80	274.0
158.80	177.0
171.00	308.0
172.00	1293.0
172.90	1118.0
173.90	80416.0
174.90	5746.0
175.90	77880.0
177.00	4995.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389

m/z	Abundance
36.00	645.0
37.00	4170.0
38.00	3387.0
39.00	1440.0
39.90	433.0
40.60	227.0
44.00	971.0
45.00	754.0
46.10	139.0
46.90	1112.0
47.90	599.0
49.00	3527.0
50.00	17008.0
51.00	5187.0
51.90	303.0
52.90	298.0
54.00	138.0
55.00	429.0
55.90	1087.0
57.00	2583.0
58.30	133.0
60.00	750.0
61.00	4573.0
62.00	4663.0
63.00	3975.0
64.00	684.0
65.00	999.0
67.00	264.0
68.00	9664.0
69.00	10034.0
69.90	790.0
71.90	616.0
73.00	4179.0
74.00	16059.0
75.00	49416.0
76.00	4169.0
76.90	669.0
78.10	392.0
78.90	3692.0
80.00	1089.0
80.80	3970.0
81.80	1048.0
85.70	185.0
86.10	177.0
86.90	4438.0
87.90	4093.0
90.80	380.0
91.90	2385.0
93.00	4632.0
94.00	12369.0
95.00	98440.0
96.00	6331.0
97.10	157.0
103.80	441.0
104.70	212.0
106.00	407.0
106.90	156.0
111.00	112.0
114.90	215.0
115.90	275.0
116.90	667.0
117.90	488.0
118.80	785.0
127.80	440.0
128.90	151.0
129.70	391.0
130.90	137.0
134.70	314.0
136.70	178.0
140.90	969.0
141.80	221.0
142.90	1851.0
144.90	550.0
145.80	161.0
147.90	227.0
152.60	104.0
154.90	224.0
156.80	186.0
158.70	117.0
171.00	252.0
172.00	1279.0
172.90	1126.0
173.90	78032.0
175.00	5502.0
175.90	76056.0
177.00	4435.0

Instrument :
MSVOA_V
ClientSampleId :
BFB389