

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037780.D
 Acq On : 09 Oct 2024 15:06
 Operator : SY/MD
 Sample : P4349-08
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 10 03:13:04 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 10 03:11:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	568883	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	560221	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	249629	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	209197	41.891	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	83.780%		
7) Chloroethane-d5	1.532	69	177875	45.888	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.780%		
11) 1,1-Dichloroethene-d2	2.060	65	94090	45.097	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	90.200%		
21) 2-Butanone-d5	3.799	46	155565	87.459	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	87.460%		
24) Chloroform-d	4.243	84	417459	46.986	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.980%		
26) 1,2-Dichloroethane-d4	4.937	65	257348	49.486	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.980%		
32) Benzene-d6	4.953	84	830254	47.361	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.720%		
36) 1,2-Dichloropropane-d6	5.986	67	267724	47.960	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	95.920%		
41) Toluene-d8	7.236	98	728468	45.827	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.660%		
43) trans-1,3-Dichloroprop...	7.551	79	110495	42.610	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.220%		
47) 2-Hexanone-d5	8.024	63	94771	80.401	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	80.400%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	293025	45.177	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	90.360%		
66) 1,2-Dichlorobenzene-d4	11.554	152	280996	53.419	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	106.840%		
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	6.908	75	7029	1.009	ug/L	# 58


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037780.D
Acq On : 09 Oct 2024 15:06
Operator : SY/MD
Sample : P4349-08
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 10 03:13:04 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 03:11:31 2024
Response via : Initial Calibration

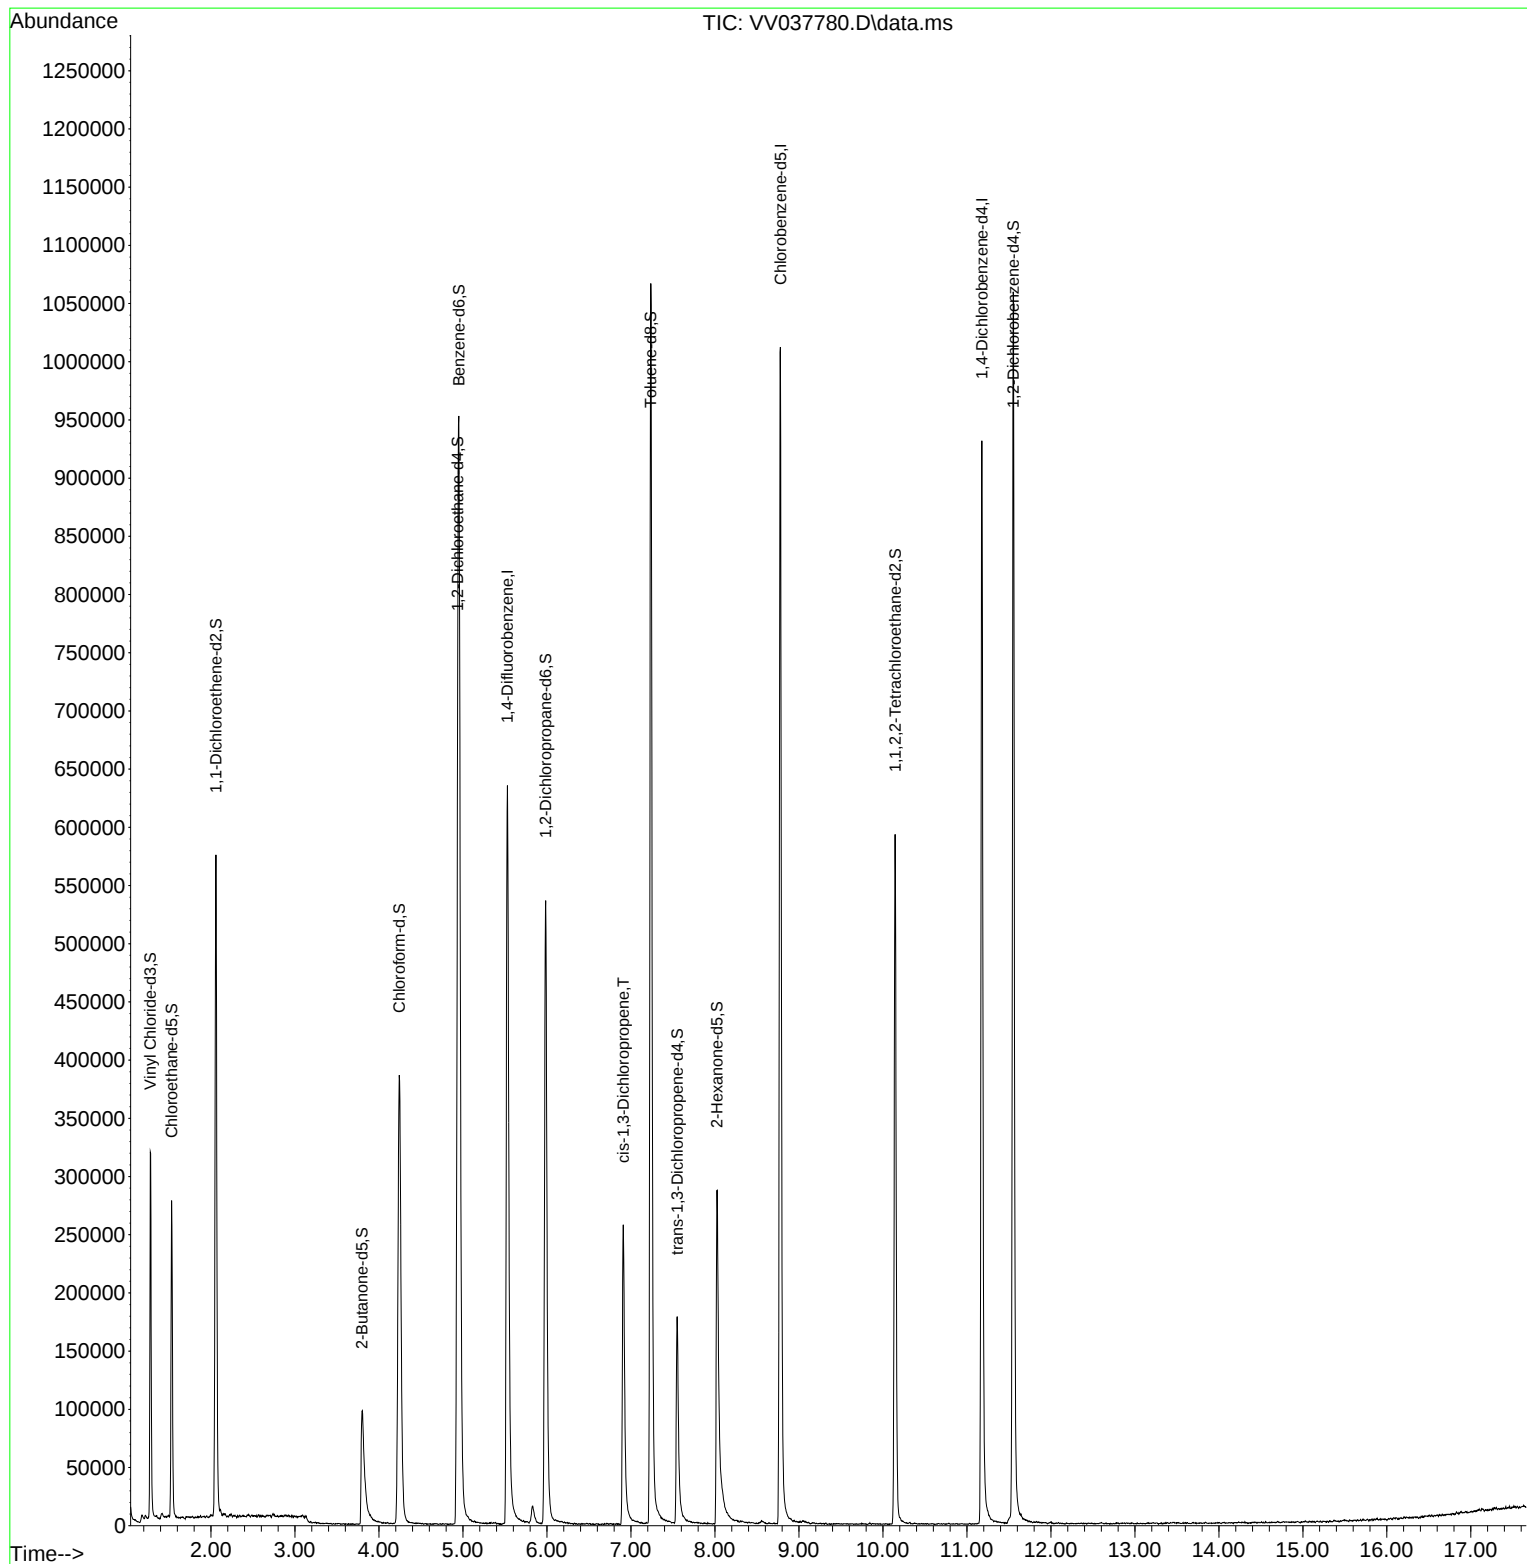

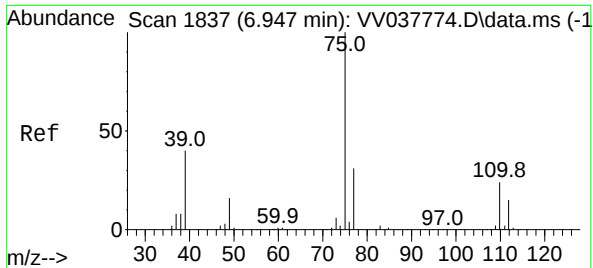

#39
cis-1,3-Dichloropropene
Concen: 1.009 ug/L
RT: 6.908 min Scan# 11
Delta R.T. -0.038 min
Lab File: VV037780.D
Acq: 09 Oct 2024 15:06

Instrument :
MSVOA_V
ClientSampleId :

Tgt Ion: 75 Resp: 7029
Ion Ratio Lower Upper
75 100
77 54.2 21.8 40.4#

