

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037784.D
 Acq On : 09 Oct 2024 16:32
 Operator : SY/MD
 Sample : P4349-12
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 10 03:14:03 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 10 03:11:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	608897	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.779	117	611807	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	267965	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.281	65	205918	38.524	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	77.040%		
7) Chloroethane-d5	1.532	69	173547	41.829	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.660%		
11) 1,1-Dichloroethene-d2	2.059	65	95382	42.712	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	85.420%		
21) 2-Butanone-d5	3.799	46	164950	86.641	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	86.640%		
24) Chloroform-d	4.243	84	423023	44.484	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.960%		
26) 1,2-Dichloroethane-d4	4.937	65	256674	46.113	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.220%		
32) Benzene-d6	4.953	84	829576	43.332	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	86.660%		
36) 1,2-Dichloropropane-d6	5.985	67	270698	44.404	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	88.800%		
41) Toluene-d8	7.236	98	727708	41.919	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	83.840%		
43) trans-1,3-Dichloroprop...	7.551	79	112972	39.892	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	79.780%		
47) 2-Hexanone-d5	8.024	63	101233	78.641	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.640%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	302311	42.679	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	85.360%		
66) 1,2-Dichlorobenzene-d4	11.554	152	280636	49.700	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	99.400%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.178	75	31242	8.194	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037784.D
Acq On : 09 Oct 2024 16:32
Operator : SY/MD
Sample : P4349-12
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 10 03:14:03 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 03:11:31 2024
Response via : Initial Calibration

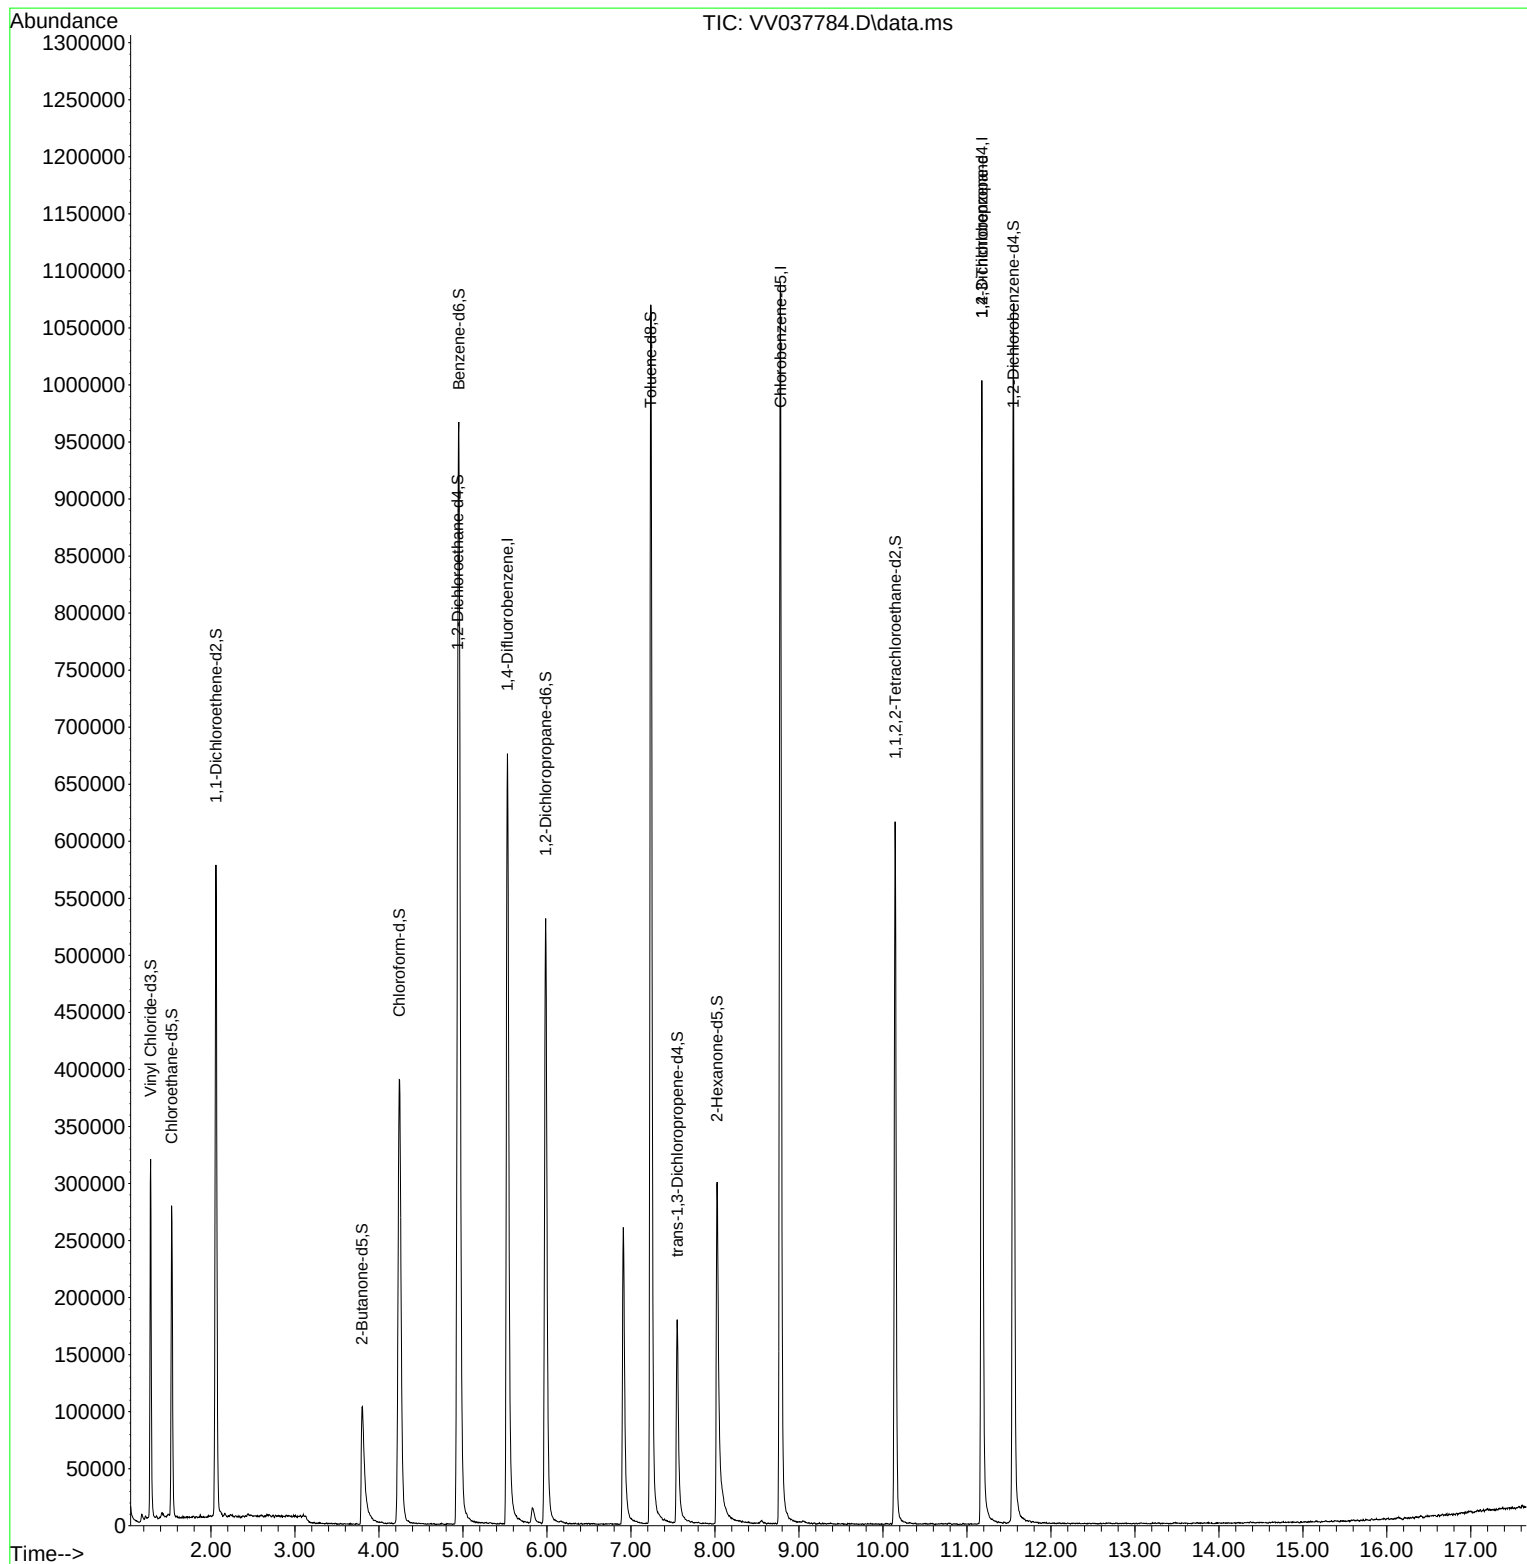

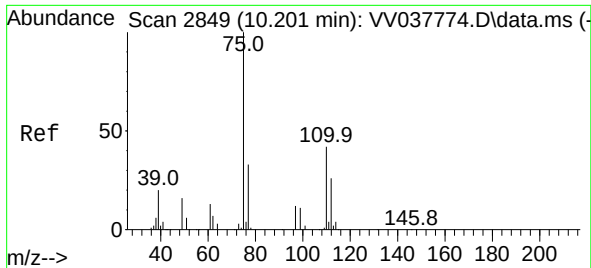

#61
 1,2,3-Trichloropropane
 Concen: 8.194 ug/L
 RT: 11.178 min Scan# 31
 Delta R.T. 0.977 min
 Lab File: VV037784.D
 Acq: 09 Oct 2024 16:32

Instrument :
 MSVOA_V
 ClientSampleId :

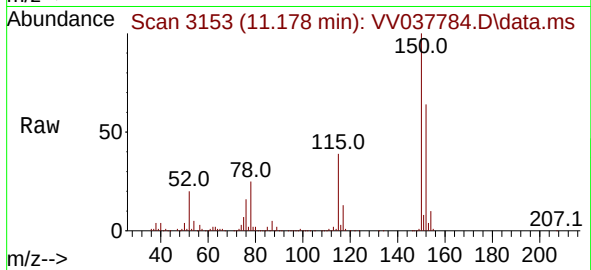

Tgt Ion: 75 Resp: 31242
 Ion Ratio Lower Upper
 75 100
 77 31.0 25.4 38.0
 110 3.1 31.7 47.5#

