

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037785.D
 Acq On : 09 Oct 2024 16:54
 Operator : SY/MD
 Sample : P4349-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 10 03:14:15 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 10 03:11:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	591240	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	589484	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	263253	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	208504	40.173	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	80.340%		
7) Chloroethane-d5	1.532	69	176240	43.747	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	87.500%		
11) 1,1-Dichloroethene-d2	2.056	65	95197	43.902	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	87.800%		
21) 2-Butanone-d5	3.799	46	164116	88.777	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	88.780%		
24) Chloroform-d	4.243	84	427955	46.346	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.700%		
26) 1,2-Dichloroethane-d4	4.937	65	259245	47.965	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.940%		
32) Benzene-d6	4.953	84	837217	45.387	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.780%		
36) 1,2-Dichloropropane-d6	5.982	67	271716	46.259	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	92.520%		
41) Toluene-d8	7.236	98	734981	43.941	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.880%		
43) trans-1,3-Dichloroprop...	7.548	79	109594	40.165	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.320%		
47) 2-Hexanone-d5	8.024	63	103654	83.571	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	83.570%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	306583	44.921	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	89.840%		
66) 1,2-Dichlorobenzene-d4	11.555	152	282062	50.847	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.700%		
Target Compounds				Qvalue		
61) 1,2,3-Trichloropropane	11.178	75	30555	8.157	ug/L #	66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037785.D
Acq On : 09 Oct 2024 16:54
Operator : SY/MD
Sample : P4349-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 10 03:14:15 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 03:11:31 2024
Response via : Initial Calibration

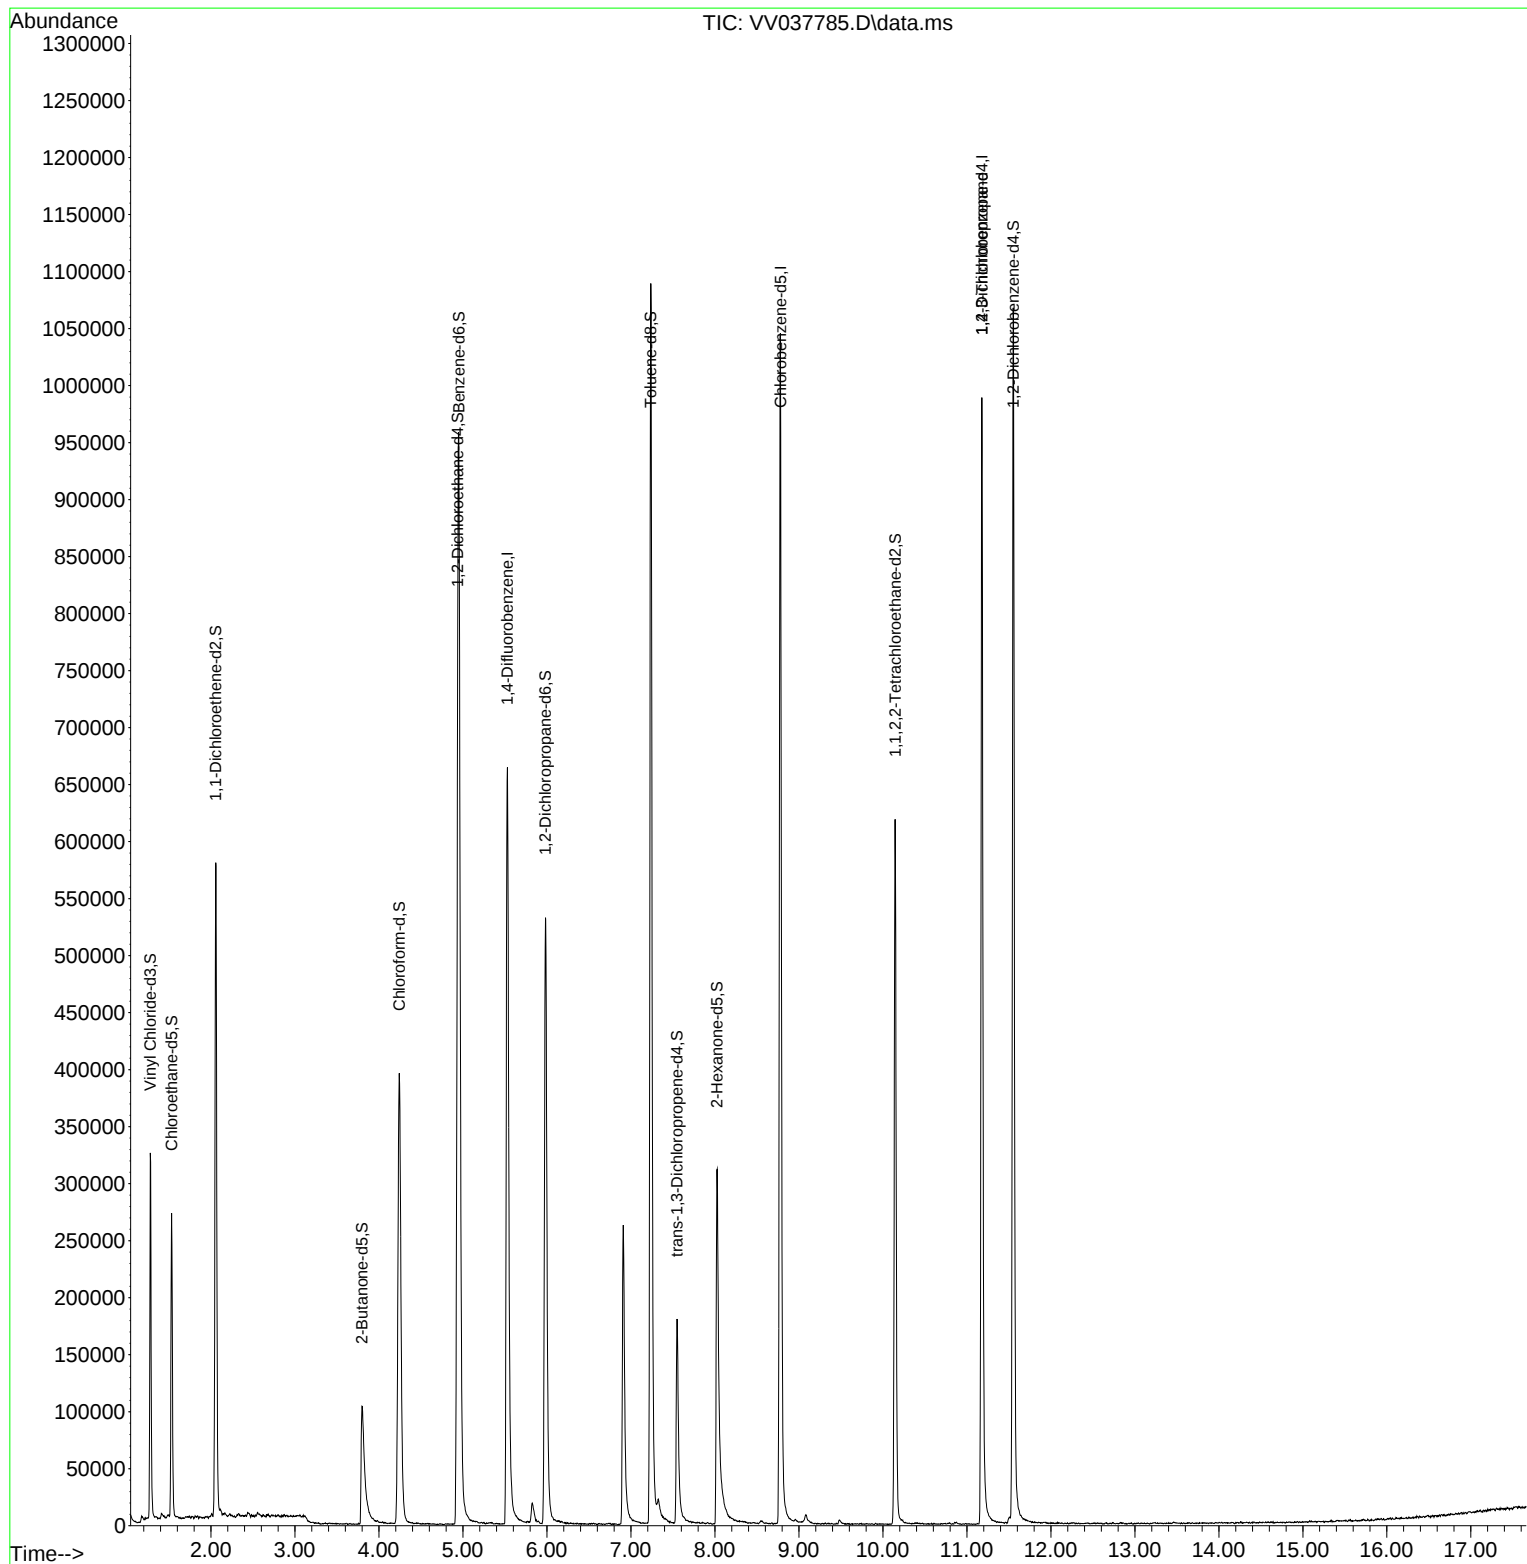

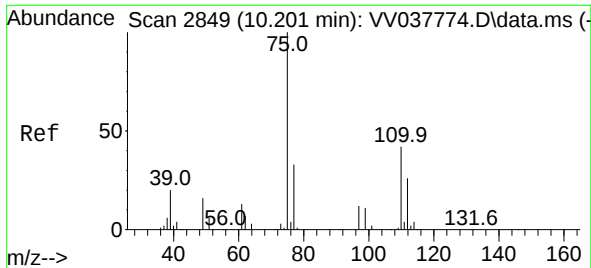

#61
 1,2,3-Trichloropropane
 Concen: 8.157 ug/L
 RT: 11.178 min Scan# 3153
 Delta R.T. 0.978 min
 Lab File: VV037785.D
 Acq: 09 Oct 2024 16:54

Instrument :
 MSVOA_V
 ClientSampleId :

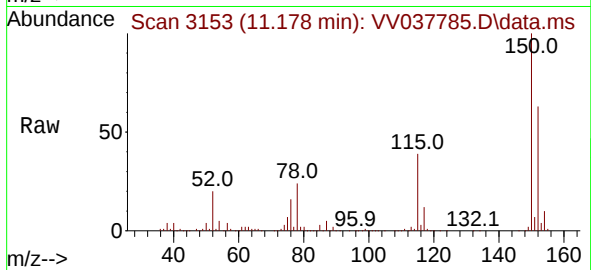

Tgt Ion: 75	Resp:	30555
Ion Ratio	Lower	Upper
75	100	
77	33.1	25.4 38.0
110	2.7	31.7 47.5#

