

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037787.D
 Acq On : 09 Oct 2024 17:37
 Operator : SY/MD
 Sample : P4349-15
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 10 03:14:38 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Thu Oct 10 03:11:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	600452	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	594636	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	265472	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	208667	39.588	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	79.180%		
7) Chloroethane-d5	1.532	69	176801	43.213	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	86.420%		
11) 1,1-Dichloroethene-d2	2.056	65	95169	43.216	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	86.440%		
21) 2-Butanone-d5	3.799	46	157354	83.813	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	83.810%		
24) Chloroform-d	4.243	84	426339	45.463	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	90.920%		
26) 1,2-Dichloroethane-d4	4.937	65	260588	47.474	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.940%		
32) Benzene-d6	4.950	84	833776	44.809	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	89.620%		
36) 1,2-Dichloropropane-d6	5.982	67	269177	45.430	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	90.860%		
41) Toluene-d8	7.236	98	735269	43.578	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.160%		
43) trans-1,3-Dichloroprop...	7.551	79	113656	41.293	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.580%		
47) 2-Hexanone-d5	8.024	63	98042	78.362	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	78.360%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	301857	43.845	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	87.700%		
66) 1,2-Dichlorobenzene-d4	11.554	152	284875	50.925	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	101.840%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.056	101	3001	0.701	ug/L	# 23


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037787.D
Acq On : 09 Oct 2024 17:37
Operator : SY/MD
Sample : P4349-15
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :


Quant Time: Oct 10 03:14:38 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Thu Oct 10 03:11:31 2024
Response via : Initial Calibration

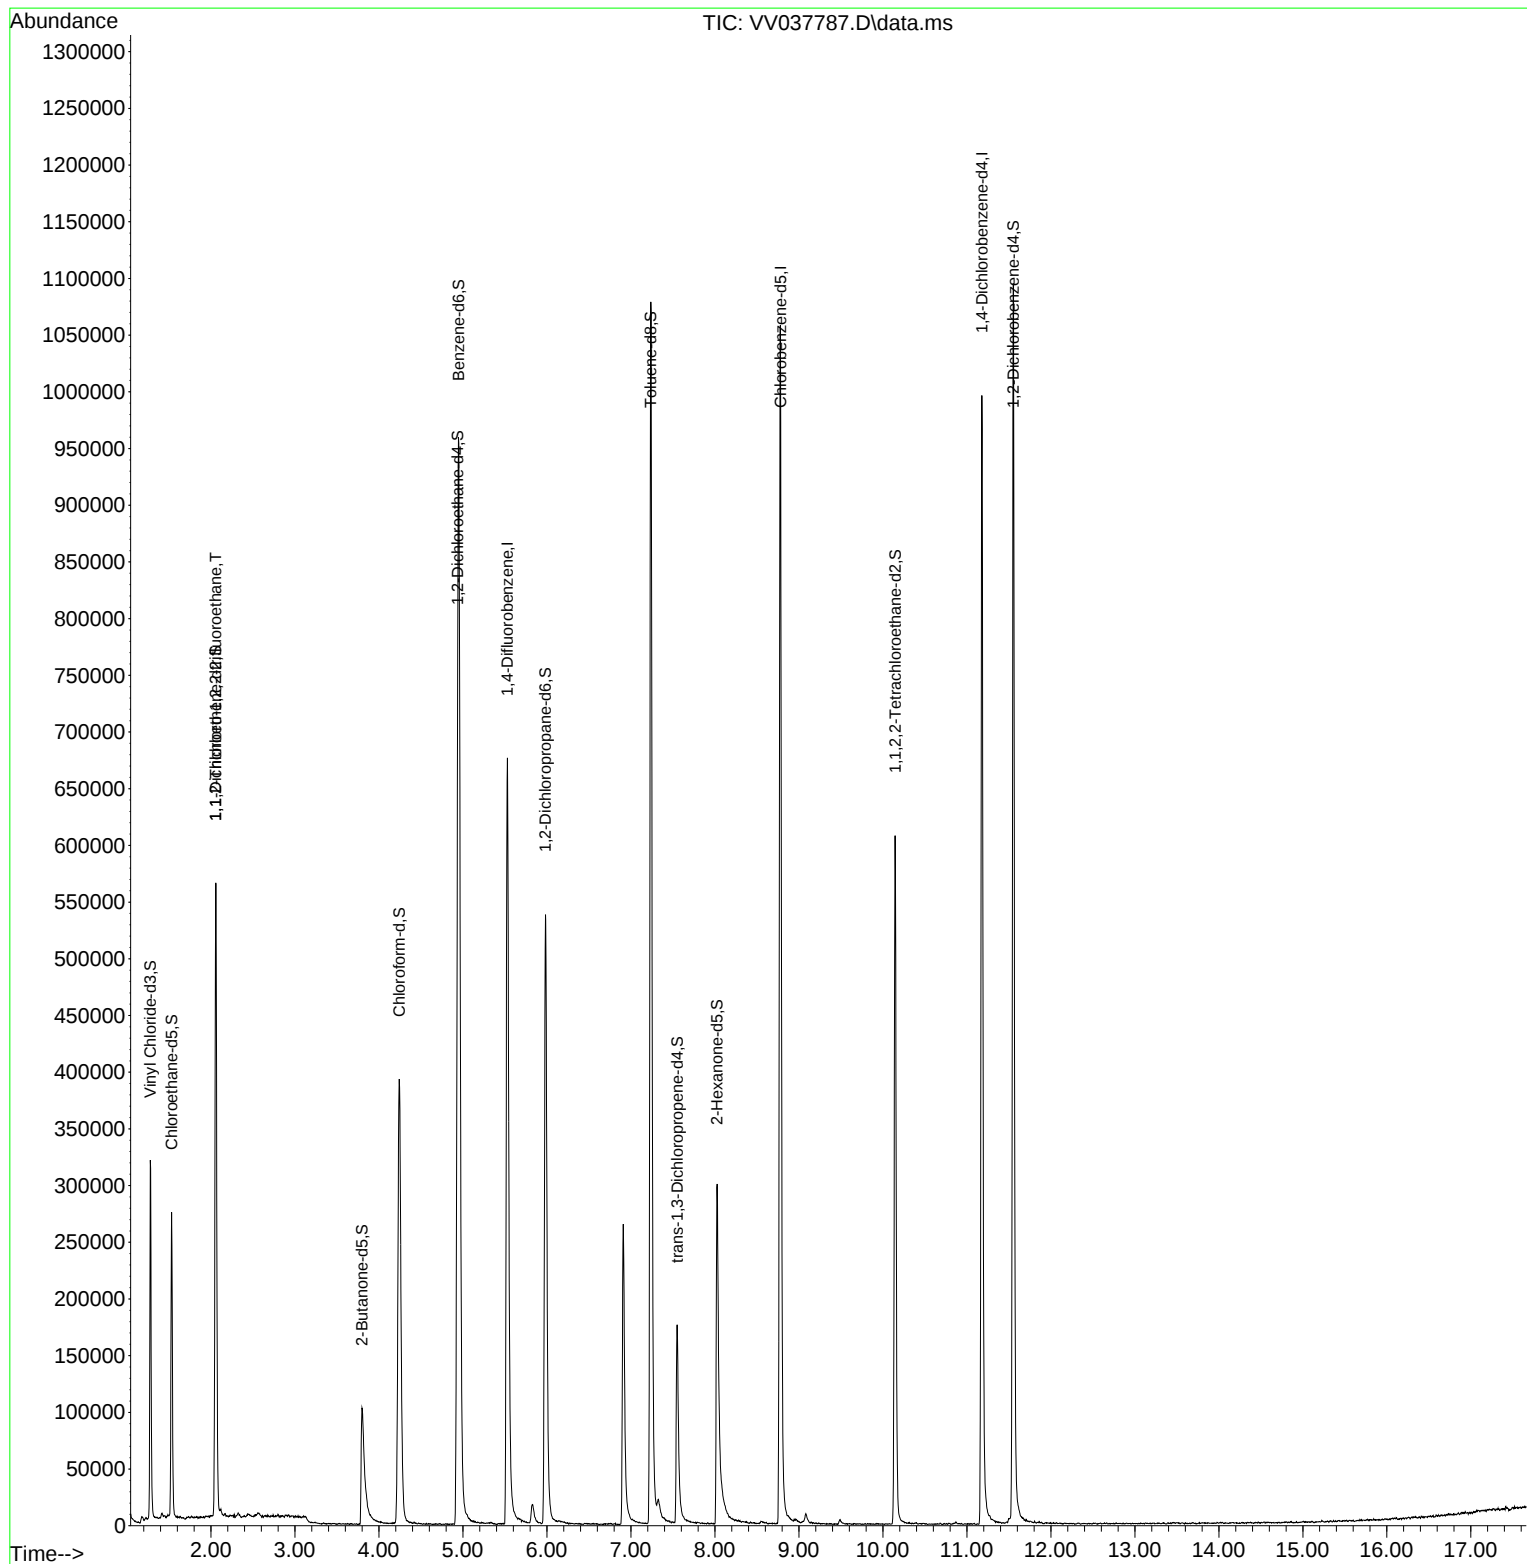

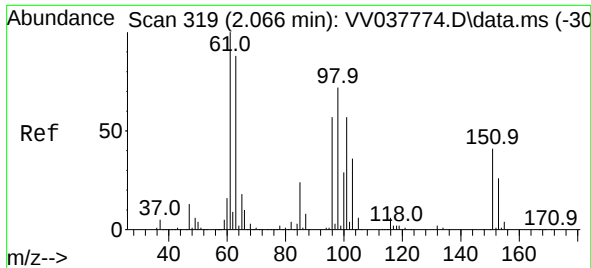

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.701 ug/L
 RT: 2.056 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV037787.D
 Acq: 09 Oct 2024 17:37

Instrument :
 MSVOA_V
 ClientSampleId :

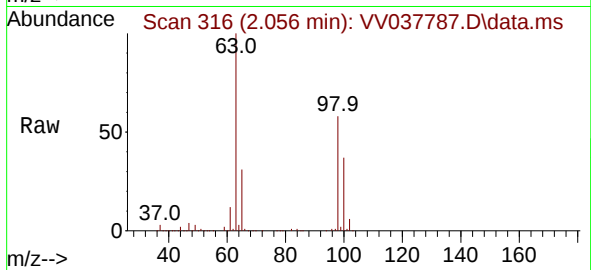

Tgt Ion:101 Resp: 3001
 Ion Ratio Lower Upper
 101 100
 85 4.4 34.6 52.0#
 151 0.0 57.5 86.3#

