

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037776.D
 Acq On : 09 Oct 2024 10:04
 Operator : SY/MD
 Sample : VV1009WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037776.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	38	42	51	rBV3	4199	7035	0.28%	0.039%
2	1.217	52	55	59	rBV5	2844	2714	0.11%	0.015%
3	1.281	67	75	92	rBV	319759	341791	13.52%	1.909%
4	1.532	145	153	170	rVB	286549	341687	13.52%	1.908%
5	2.060	306	317	335	rBV	580939	853626	33.77%	4.768%
6	3.301	700	703	707	rVB4	826	686	0.03%	0.004%
7	3.342	714	716	720	rBV4	1124	926	0.04%	0.005%
8	3.439	742	746	748	rBV2	742	490	0.02%	0.003%
9	3.490	759	762	767	rBV3	486	583	0.02%	0.003%
10	3.645	804	810	814	rBV4	705	705	0.03%	0.004%
11	3.799	847	858	895	rBV	115941	346777	13.72%	1.937%
12	4.243	979	996	1028	rBV	411645	1062745	42.05%	5.936%
13	4.494	1071	1074	1076	rBV2	763	455	0.02%	0.003%
14	4.522	1081	1083	1089	rVB3	1044	762	0.03%	0.004%
15	4.677	1125	1131	1135	rBV6	1017	1031	0.04%	0.006%
16	4.703	1135	1139	1142	rBV3	879	645	0.03%	0.004%
17	4.818	1171	1175	1178	rBV3	679	556	0.02%	0.003%
18	4.947	1200	1215	1250	rBV2	997645	2527481	100.00%	14.117%
19	5.249	1305	1309	1310	rBV4	989	590	0.02%	0.003%
20	5.313	1327	1329	1332	rBV2	908	438	0.02%	0.002%
21	5.333	1332	1335	1339	rBV4	1299	1012	0.04%	0.006%
22	5.452	1369	1372	1376	rVB7	841	639	0.03%	0.004%
23	5.529	1384	1396	1425	rBV	648934	1350457	53.43%	7.543%
24	5.831	1477	1490	1511	rVB3	16508	39178	1.55%	0.219%
25	5.982	1525	1537	1570	rBV	567636	1165944	46.13%	6.512%
26	6.301	1629	1636	1637	rBV4	583	603	0.02%	0.003%
27	6.326	1642	1644	1648	rBV4	759	577	0.02%	0.003%
28	6.429	1673	1676	1679	rBV3	1440	1049	0.04%	0.006%
29	6.471	1686	1689	1692	rBV4	658	439	0.02%	0.002%
30	6.760	1776	1779	1782	rBV3	605	503	0.02%	0.003%
31	6.866	1808	1812	1814	rBV3	718	468	0.02%	0.003%
32	6.908	1814	1825	1856	rBV	280697	541886	21.44%	3.027%
33	7.236	1916	1927	1962	rBV	1086795	1948729	77.10%	10.884%
34	7.548	2013	2024	2050	rBV	188204	359614	14.23%	2.009%
35	7.825	2105	2110	2112	rBV3	680	455	0.02%	0.003%
36	7.879	2125	2127	2129	rVB2	1058	447	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037776.D
 Acq On : 09 Oct 2024 10:04
 Operator : SY/MD
 Sample : VV1009WBL01
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.908	2129	2136	2139	rBV5	1673	1683	0.07%	0.009%
38	7.995	2159	2163	2164	rBV2	1301	921	0.04%	0.005%
39	8.024	2164	2172	2212	rVV2	330225	739107	29.24%	4.128%
40	8.400	2287	2289	2293	rVB4	914	471	0.02%	0.003%
41	8.516	2322	2325	2327	rBV3	807	488	0.02%	0.003%
42	8.551	2331	2336	2342	rBV6	1970	2793	0.11%	0.016%
43	8.625	2355	2359	2362	rBV6	615	494	0.02%	0.003%
44	8.670	2369	2373	2376	rBV4	895	697	0.03%	0.004%
45	8.712	2382	2386	2389	rBV3	679	523	0.02%	0.003%
46	8.776	2395	2406	2432	rBV	1031536	1720252	68.06%	9.608%
47	9.043	2487	2489	2492	rBV4	1057	784	0.03%	0.004%
48	9.101	2504	2507	2511	rBV5	1229	860	0.03%	0.005%
49	9.169	2524	2528	2532	rBV6	788	537	0.02%	0.003%
50	9.204	2532	2539	2541	rBV5	948	1023	0.04%	0.006%
51	9.230	2545	2547	2551	rVB4	913	555	0.02%	0.003%
52	9.320	2572	2575	2578	rVB3	872	517	0.02%	0.003%
53	9.339	2578	2581	2585	rBV4	674	636	0.03%	0.004%
54	9.390	2594	2597	2601	rVB4	995	884	0.03%	0.005%
55	9.423	2601	2607	2609	rBV2	726	677	0.03%	0.004%
56	9.452	2613	2616	2620	rBV3	607	479	0.02%	0.003%
57	9.503	2629	2632	2634	rVV2	1052	503	0.02%	0.003%
58	9.545	2642	2645	2647	rBV3	695	470	0.02%	0.003%
59	9.641	2671	2675	2676	rBV	689	480	0.02%	0.003%
60	9.747	2704	2708	2710	rBV2	762	649	0.03%	0.004%
61	9.863	2741	2744	2747	rBV4	814	762	0.03%	0.004%
62	9.985	2778	2782	2786	rVV4	776	562	0.02%	0.003%
63	10.101	2814	2818	2819	rBV3	707	439	0.02%	0.002%
64	10.146	2819	2832	2858	rBV	666704	1075025	42.53%	6.004%
65	10.477	2930	2935	2937	rBV4	652	650	0.03%	0.004%
66	10.593	2968	2971	2976	rVB4	950	586	0.02%	0.003%
67	10.683	2992	2999	3001	rBV4	583	707	0.03%	0.004%
68	10.734	3011	3015	3017	rBV3	858	707	0.03%	0.004%
69	10.789	3027	3032	3035	rBV4	1755	1542	0.06%	0.009%
70	10.869	3053	3057	3061	rBV3	832	728	0.03%	0.004%
71	10.943	3078	3080	3085	rVB3	654	475	0.02%	0.003%
72	10.976	3085	3090	3094	rBV3	580	502	0.02%	0.003%
73	11.123	3133	3136	3138	rBV3	1830	1277	0.05%	0.007%
74	11.178	3142	3153	3189	rBV	978677	1585946	62.75%	8.858%
75	11.551	3257	3269	3302	rBV	1130723	1817226	71.90%	10.150%
76	11.750	3327	3331	3333	rBV3	758	573	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037776.D
Acq On : 09 Oct 2024 10:04
Operator : SY/MD
Sample : VV1009WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis

77	11.985	3401	3404	3410	rVB6	783	710	0.03%	0.004%
78	12.310	3502	3505	3511	rBV4	761	471	0.02%	0.003%
79	12.368	3522	3523	3528	rVB4	699	480	0.02%	0.003%
80	12.394	3528	3531	3533	rBV4	665	506	0.02%	0.003%
81	12.432	3537	3543	3546	rBV5	640	555	0.02%	0.003%
82	12.586	3586	3591	3593	rBV5	1800	1845	0.07%	0.010%
83	12.686	3619	3622	3624	rBV2	949	577	0.02%	0.003%
84	12.744	3638	3640	3645	rBV3	548	462	0.02%	0.003%
85	12.889	3680	3685	3688	rBV3	895	665	0.03%	0.004%
86	12.911	3688	3692	3695	rVV3	1229	807	0.03%	0.005%
87	13.017	3723	3725	3729	rBV4	627	430	0.02%	0.002%
88	13.056	3735	3737	3743	rBV3	615	556	0.02%	0.003%
89	13.332	3820	3823	3827	rBV3	654	505	0.02%	0.003%
90	13.455	3850	3861	3872	rBV5	5980	13190	0.52%	0.074%
91	13.567	3893	3896	3897	rBV3	747	440	0.02%	0.002%
92	13.683	3920	3932	3938	rBV3	4168	7704	0.30%	0.043%
93	14.072	4048	4053	4056	rBV4	941	832	0.03%	0.005%
94	14.111	4063	4065	4070	rVB3	949	742	0.03%	0.004%
95	14.310	4123	4127	4130	rBV4	1079	1014	0.04%	0.006%
96	14.525	4192	4194	4198	rBV3	879	568	0.02%	0.003%
97	15.117	4376	4378	4380	rBV3	1083	481	0.02%	0.003%
98	15.172	4393	4395	4398	rBV2	1074	659	0.03%	0.004%
99	15.294	4430	4433	4437	rBV5	1321	958	0.04%	0.005%
100	15.429	4473	4475	4477	rBV3	1200	682	0.03%	0.004%




Sum of corrected areas: 17903752

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037776.D
Acq On : 09 Oct 2024 10:04
Operator : SY/MD
Sample : VV1009WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

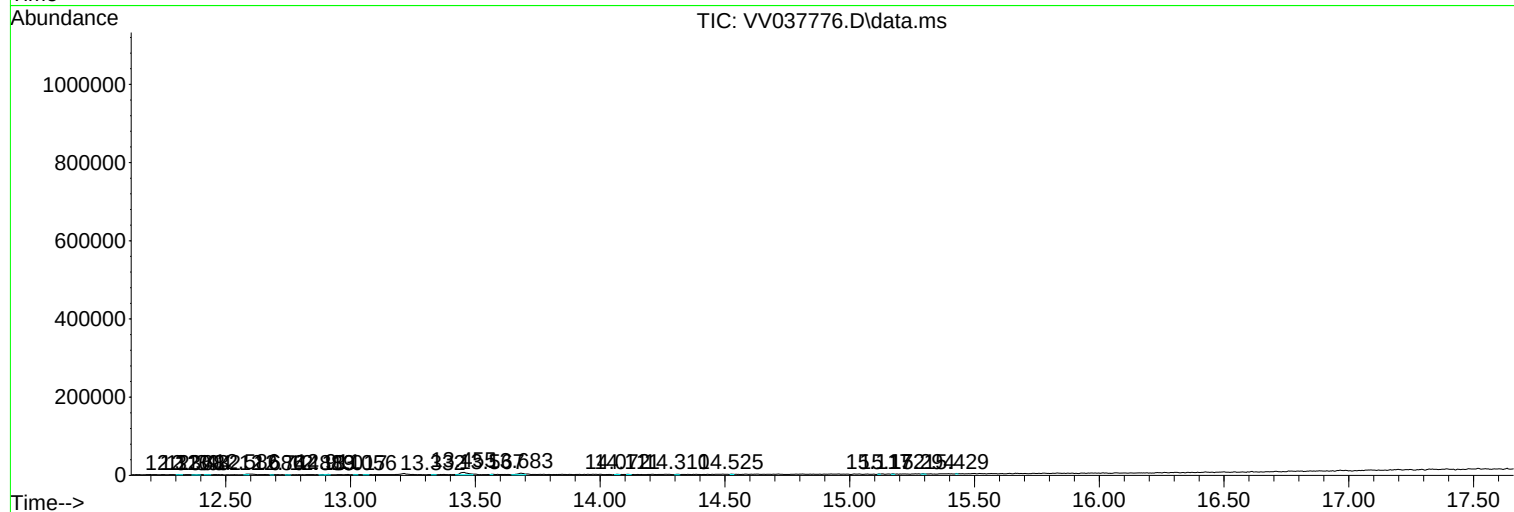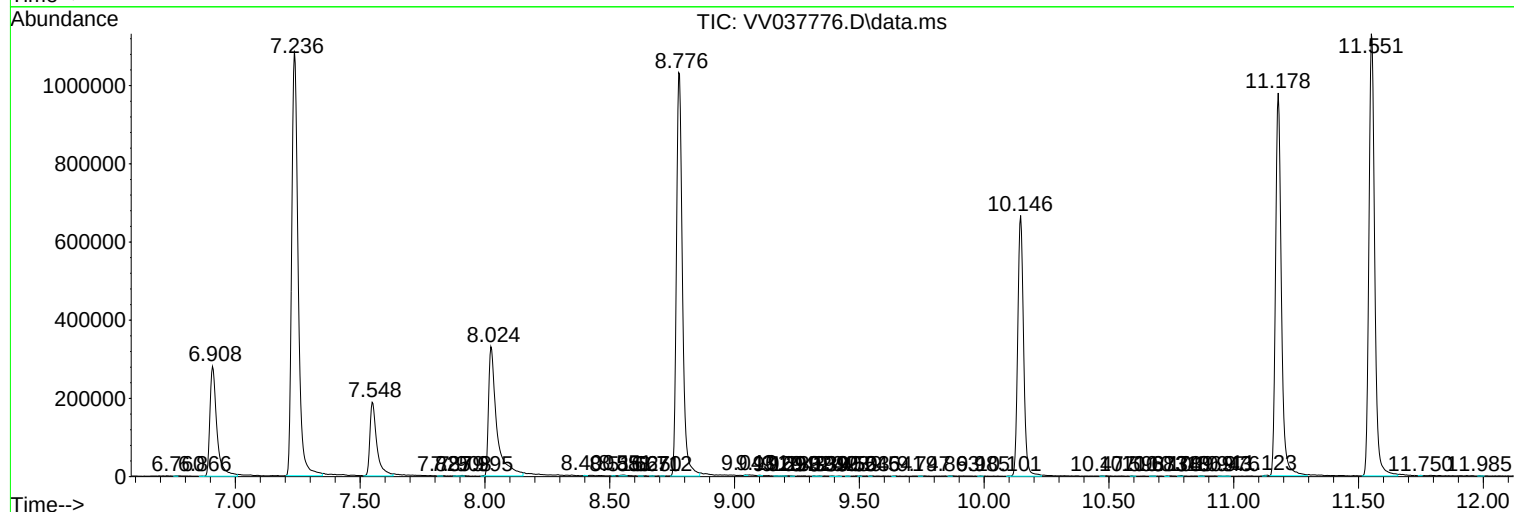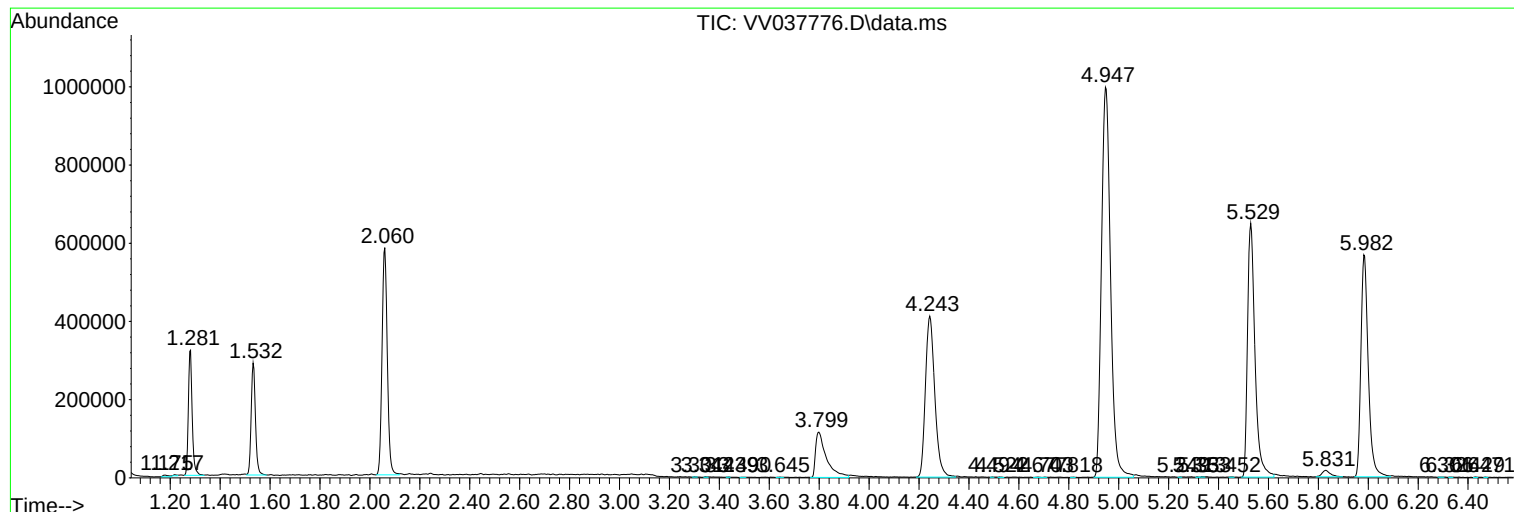

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037776.D
Acq On : 09 Oct 2024 10:04
Operator : SY/MD
Sample : VV1009WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037776.D
Acq On : 09 Oct 2024 10:04
Operator : SY/MD
Sample : VV1009WBL01
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK237

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------