

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037778.D
 Acq On : 09 Oct 2024 14:22
 Operator : SY/MD
 Sample : P4349-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037778.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	89	rVB	314147	339414	13.81%	1.953%
2	1.532	146	153	166	rVB	276213	323646	13.17%	1.863%
3	2.060	307	317	329	rBV	577825	834023	33.94%	4.800%
4	3.474	755	757	758	rBV	828	343	0.01%	0.002%
5	3.548	775	780	783	rVB5	694	683	0.03%	0.004%
6	3.568	783	786	789	rBV2	696	558	0.02%	0.003%
7	3.642	805	809	814	rVB3	654	653	0.03%	0.004%
8	3.661	814	815	818	rVB2	474	248	0.01%	0.001%
9	3.683	820	822	824	rBV	614	287	0.01%	0.002%
10	3.761	844	846	849	rBV2	543	340	0.01%	0.002%
11	3.799	849	858	903	rBV	98410	300428	12.22%	1.729%
12	4.162	966	971	974	rBV3	953	1013	0.04%	0.006%
13	4.243	981	996	1026	rBV	396217	996469	40.55%	5.735%
14	4.478	1066	1069	1075	rBV5	1051	1309	0.05%	0.008%
15	4.542	1087	1089	1091	rBV2	416	220	0.01%	0.001%
16	4.580	1099	1101	1103	rVB2	757	355	0.01%	0.002%
17	4.603	1103	1108	1112	rBV4	845	724	0.03%	0.004%
18	4.699	1136	1138	1139	rBV	312	90	0.00%	0.001%
19	4.760	1154	1157	1158	rBV	561	268	0.01%	0.002%
20	4.770	1158	1160	1162	rVB3	491	160	0.01%	0.001%
21	4.783	1162	1164	1167	rBV3	332	136	0.01%	0.001%
22	4.796	1167	1168	1171	rVV	347	184	0.01%	0.001%
23	4.870	1188	1191	1194	rBV4	663	519	0.02%	0.003%
24	4.896	1194	1199	1201	rBV3	630	473	0.02%	0.003%
25	4.950	1201	1216	1263	rBV2	982014	2457552	100.00%	14.144%
26	5.420	1358	1362	1364	rBV4	698	487	0.02%	0.003%
27	5.484	1381	1382	1383	rBV2	469	121	0.00%	0.001%
28	5.529	1385	1396	1430	rBV	666115	1387369	56.45%	7.985%
29	5.982	1525	1537	1571	rBV	539781	1117932	45.49%	6.434%
30	6.272	1621	1627	1631	rBV7	1230	1269	0.05%	0.007%
31	6.333	1642	1646	1647	rBV4	595	372	0.02%	0.002%
32	6.384	1659	1662	1663	rBV2	862	411	0.02%	0.002%
33	6.436	1676	1678	1680	rBV3	943	368	0.01%	0.002%
34	6.471	1686	1689	1694	rBV4	579	388	0.02%	0.002%
35	6.497	1694	1697	1699	rVB4	818	457	0.02%	0.003%
36	6.516	1699	1703	1708	rBV7	727	928	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037778.D
 Acq On : 09 Oct 2024 14:22
 Operator : SY/MD
 Sample : P4349-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.539	1708	1710	1713	rVB4	949	322	0.01%	0.002%
38	6.555	1713	1715	1719	rVB3	572	471	0.02%	0.003%
39	6.574	1719	1721	1724	rBV2	524	304	0.01%	0.002%
40	6.593	1725	1727	1730	rVB2	347	155	0.01%	0.001%
41	6.638	1733	1741	1746	rBV5	846	1109	0.05%	0.006%
42	6.661	1746	1748	1752	rVB3	461	239	0.01%	0.001%
43	6.683	1753	1755	1758	rVB	495	187	0.01%	0.001%
44	6.722	1764	1767	1768	rBV2	585	334	0.01%	0.002%
45	6.854	1805	1808	1811	rVB4	628	339	0.01%	0.002%
46	6.908	1811	1825	1854	rBV	266243	523968	21.32%	3.016%
47	7.236	1916	1927	1949	rBV	1099935	1936031	78.78%	11.143%
48	7.548	2016	2024	2055	rBV	180242	342689	13.94%	1.972%
49	7.905	2133	2135	2139	rVB4	1446	988	0.04%	0.006%
50	7.928	2139	2142	2144	rBV3	717	509	0.02%	0.003%
51	7.979	2155	2158	2160	rBV2	637	386	0.02%	0.002%
52	7.992	2160	2162	2164	rBV2	426	285	0.01%	0.002%
53	8.024	2164	2172	2210	rBV3	287029	664722	27.05%	3.826%
54	8.609	2349	2354	2355	rBV4	846	602	0.02%	0.003%
55	8.654	2364	2368	2370	rVB4	1421	1023	0.04%	0.006%
56	8.722	2385	2389	2390	rBV3	929	705	0.03%	0.004%
57	8.776	2396	2406	2441	rBV	1031536	1751061	71.25%	10.078%
58	9.304	2568	2570	2572	rBV3	433	182	0.01%	0.001%
59	9.416	2601	2605	2610	rVB3	582	556	0.02%	0.003%
60	9.487	2622	2627	2628	rBV2	2460	2186	0.09%	0.013%
61	9.545	2644	2645	2646	rBV	487	130	0.01%	0.001%
62	9.596	2657	2661	2665	rBV3	817	766	0.03%	0.004%
63	9.619	2665	2668	2670	rBV3	552	333	0.01%	0.002%
64	9.722	2694	2700	2701	rBV4	824	691	0.03%	0.004%
65	9.773	2709	2716	2721	rBV5	663	831	0.03%	0.005%
66	9.792	2721	2722	2726	rVB2	517	258	0.01%	0.001%
67	9.812	2726	2728	2729	rBV2	466	245	0.01%	0.001%
68	9.841	2735	2737	2740	rVB3	497	239	0.01%	0.001%
69	9.857	2740	2742	2744	rBV2	305	142	0.01%	0.001%
70	9.915	2758	2760	2765	rVB2	459	288	0.01%	0.002%
71	9.937	2765	2767	2769	rBV3	527	281	0.01%	0.002%
72	9.979	2778	2780	2781	rBV2	650	295	0.01%	0.002%
73	10.046	2799	2801	2803	rVB2	414	167	0.01%	0.001%
74	10.059	2803	2805	2806	rBV	552	245	0.01%	0.001%
75	10.108	2817	2820	2821	rBV2	559	322	0.01%	0.002%
76	10.146	2821	2832	2852	rBV	600374	958962	39.02%	5.519%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037778.D
 Acq On : 09 Oct 2024 14:22
 Operator : SY/MD
 Sample : P4349-06
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.365	2898	2900	2905	rBV2	1000	712	0.03%	0.004%
78	10.590	2965	2970	2971	rBV2	502	377	0.02%	0.002%
79	10.683	2997	2999	3004	rVB3	919	725	0.03%	0.004%
80	10.709	3004	3007	3009	rBV2	778	537	0.02%	0.003%
81	10.789	3027	3032	3036	rVB5	1344	1264	0.05%	0.007%
82	10.818	3036	3041	3044	rBV5	1008	702	0.03%	0.004%
83	10.863	3049	3055	3060	rBV5	1230	1746	0.07%	0.010%
84	10.905	3066	3068	3072	rBV5	499	368	0.01%	0.002%
85	10.944	3077	3080	3082	rBV2	385	205	0.01%	0.001%
86	11.056	3113	3115	3116	rBV	339	116	0.00%	0.001%
87	11.082	3121	3123	3127	rBV2	581	507	0.02%	0.003%
88	11.111	3127	3132	3133	rBV2	664	521	0.02%	0.003%
89	11.178	3142	3153	3177	rBV	982887	1575667	64.12%	9.069%
90	11.484	3240	3248	3258	rBV2	24699	53906	2.19%	0.310%
91	11.551	3260	3269	3298	rVB	1073813	1766415	71.88%	10.166%
92	12.834	3665	3668	3671	rVB3	807	547	0.02%	0.003%
93	12.976	3707	3712	3713	rBV3	821	652	0.03%	0.004%
94	13.210	3783	3785	3792	rVB3	1436	1286	0.05%	0.007%
95	13.271	3801	3804	3809	rBV5	1123	1345	0.05%	0.008%
96	13.387	3836	3840	3843	rBV4	776	770	0.03%	0.004%
97	13.445	3855	3858	3859	rBV3	939	535	0.02%	0.003%
98	13.519	3879	3881	3882	rBV2	1069	497	0.02%	0.003%
99	14.017	4034	4036	4043	rVB6	1074	847	0.03%	0.005%
100	14.120	4064	4068	4071	rBV3	1009	986	0.04%	0.006%




Sum of corrected areas: 17374978

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037778.D
Acq On : 09 Oct 2024 14:22
Operator : SY/MD
Sample : P4349-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

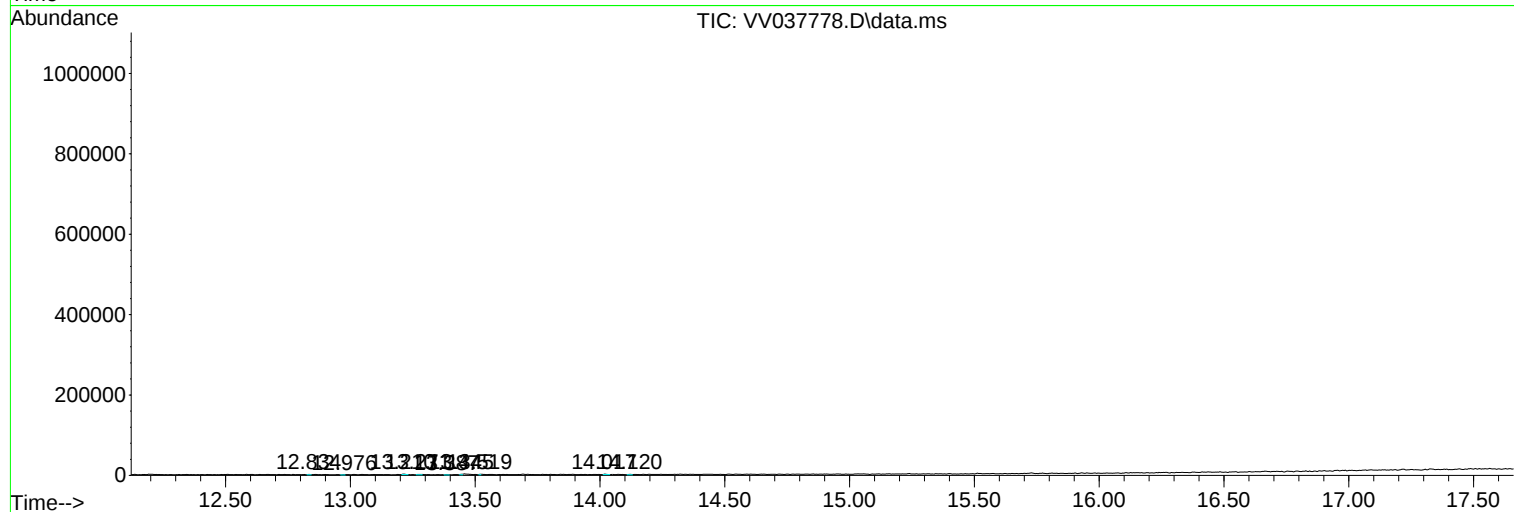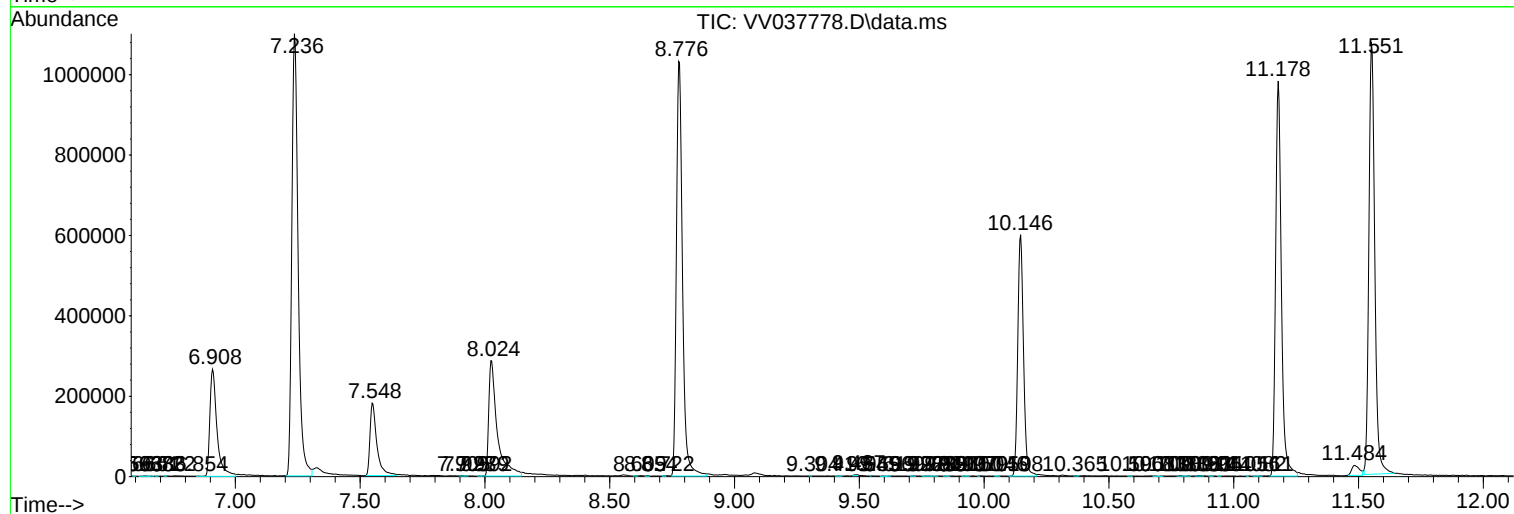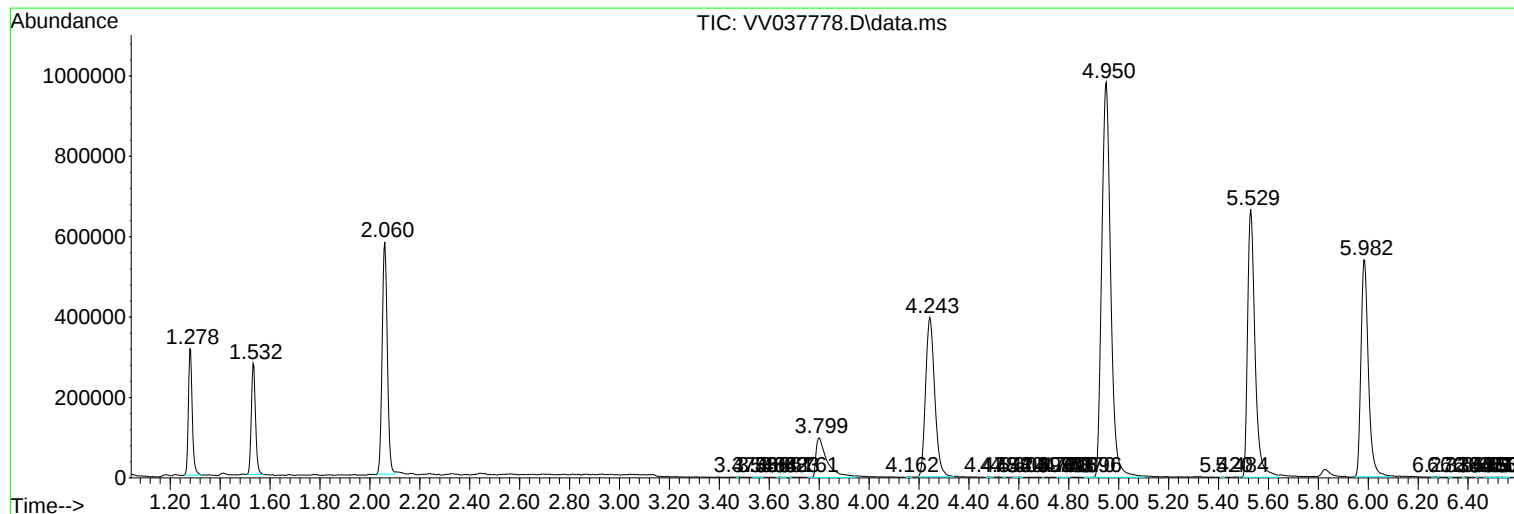

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037778.D
Acq On : 09 Oct 2024 14:22
Operator : SY/MD
Sample : P4349-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037778.D
Acq On : 09 Oct 2024 14:22
Operator : SY/MD
Sample : P4349-06
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------