

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037779.D
 Acq On : 09 Oct 2024 14:44
 Operator : SY/MD
 Sample : P4349-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037779.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	50	rBV2	4584	8284	0.34%	0.047%
2	1.281	67	75	92	rBV	325472	346664	14.04%	1.962%
3	1.532	145	153	169	rVB	274726	326729	13.23%	1.849%
4	2.059	306	317	330	rBV	585565	842524	34.11%	4.769%
5	3.468	752	755	758	rVB3	903	510	0.02%	0.003%
6	3.487	758	761	763	rBV3	678	438	0.02%	0.002%
7	3.564	782	785	790	rBV4	592	471	0.02%	0.003%
8	3.606	795	798	802	rVB2	904	543	0.02%	0.003%
9	3.641	802	809	813	rBV4	592	673	0.03%	0.004%
10	3.667	813	817	821	rVB4	695	683	0.03%	0.004%
11	3.735	835	838	843	rVB3	498	435	0.02%	0.002%
12	3.799	849	858	889	rBV	99279	293982	11.90%	1.664%
13	4.005	920	922	925	rVB2	1069	498	0.02%	0.003%
14	4.079	941	945	948	rBV4	765	684	0.03%	0.004%
15	4.243	978	996	1027	rBV	401539	1013361	41.03%	5.736%
16	4.429	1049	1054	1056	rBV4	739	596	0.02%	0.003%
17	4.442	1056	1058	1061	rVB3	774	499	0.02%	0.003%
18	4.696	1133	1137	1140	rBV4	684	732	0.03%	0.004%
19	4.783	1161	1164	1166	rBV	597	452	0.02%	0.003%
20	4.947	1200	1215	1256	rBV2	975353	2469727	100.00%	13.980%
21	5.297	1320	1324	1326	rBV3	716	527	0.02%	0.003%
22	5.432	1363	1366	1371	rVB5	1041	1016	0.04%	0.006%
23	5.529	1385	1396	1428	rBV	682986	1432187	57.99%	8.107%
24	5.770	1468	1471	1473	rBV4	1293	742	0.03%	0.004%
25	5.825	1479	1488	1504	rBV5	17874	41645	1.69%	0.236%
26	5.940	1520	1524	1525	rBV3	1150	748	0.03%	0.004%
27	5.982	1525	1537	1575	rVV	539570	1134993	45.96%	6.424%
28	6.239	1615	1617	1620	rVB3	988	542	0.02%	0.003%
29	6.272	1624	1627	1629	rBV2	672	534	0.02%	0.003%
30	6.349	1648	1651	1654	rVB4	874	702	0.03%	0.004%
31	6.381	1654	1661	1664	rBV5	987	930	0.04%	0.005%
32	6.410	1667	1670	1673	rVB2	675	449	0.02%	0.003%
33	6.464	1684	1687	1691	rBV5	802	642	0.03%	0.004%
34	6.644	1739	1743	1746	rBV3	573	540	0.02%	0.003%
35	6.680	1751	1754	1757	rBV3	729	459	0.02%	0.003%
36	6.786	1785	1787	1791	rVB3	839	432	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037779.D
 Acq On : 09 Oct 2024 14:44
 Operator : SY/MD
 Sample : P4349-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOA7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.847	1798	1806	1810	rBV7	860	1006	0.04%	0.006%
38	6.908	1815	1825	1857	rBV	267515	527154	21.34%	2.984%
39	7.101	1882	1885	1890	rVB6	1061	1097	0.04%	0.006%
40	7.236	1912	1927	1950	rBV	1104881	1939460	78.53%	10.978%
41	7.551	2015	2025	2054	rBV	183771	350426	14.19%	1.984%
42	7.728	2078	2080	2083	rBV4	1023	521	0.02%	0.003%
43	7.841	2113	2115	2117	rBV3	742	522	0.02%	0.003%
44	7.886	2126	2129	2132	rBV3	525	439	0.02%	0.002%
45	7.950	2144	2149	2152	rVB5	872	737	0.03%	0.004%
46	8.027	2158	2173	2213	rBV2	292845	689860	27.93%	3.905%
47	8.345	2270	2272	2275	rBV4	1013	549	0.02%	0.003%
48	8.374	2278	2281	2285	rBV7	1153	840	0.03%	0.005%
49	8.548	2331	2335	2337	rBV4	1094	975	0.04%	0.006%
50	8.599	2348	2351	2355	rVB3	1050	625	0.03%	0.004%
51	8.628	2358	2360	2364	rVV3	911	690	0.03%	0.004%
52	8.705	2381	2384	2386	rBV	806	547	0.02%	0.003%
53	8.734	2390	2393	2395	rBV3	709	508	0.02%	0.003%
54	8.779	2396	2407	2436	rBV	1083601	1797317	72.77%	10.174%
55	9.214	2538	2542	2544	rBV4	1146	943	0.04%	0.005%
56	9.275	2558	2561	2562	rBV3	849	460	0.02%	0.003%
57	9.487	2616	2627	2634	rBV8	4123	7277	0.29%	0.041%
58	9.558	2643	2649	2652	rBV4	1027	866	0.04%	0.005%
59	9.664	2676	2682	2685	rBV2	566	662	0.03%	0.004%
60	9.696	2691	2692	2700	rVB4	734	687	0.03%	0.004%
61	9.821	2726	2731	2737	rVB5	765	658	0.03%	0.004%
62	9.931	2761	2765	2770	rVB3	696	605	0.02%	0.003%
63	10.014	2789	2791	2798	rVB5	913	606	0.02%	0.003%
64	10.066	2803	2807	2810	rBV3	639	634	0.03%	0.004%
65	10.146	2820	2832	2857	rBV	608546	972242	39.37%	5.503%
66	10.323	2883	2887	2891	rBV4	671	495	0.02%	0.003%
67	10.394	2905	2909	2911	rBV3	1442	1062	0.04%	0.006%
68	10.590	2965	2970	2972	rBV3	825	670	0.03%	0.004%
69	10.757	3019	3022	3027	rVB3	620	523	0.02%	0.003%
70	10.779	3027	3029	3034	rBV5	1079	829	0.03%	0.005%
71	11.088	3121	3125	3128	rVV3	859	588	0.02%	0.003%
72	11.178	3141	3153	3190	rBV	1014715	1641880	66.48%	9.294%
73	11.451	3234	3238	3239	rBV4	858	534	0.02%	0.003%
74	11.500	3244	3253	3258	rVV4	8381	14980	0.61%	0.085%
75	11.554	3259	3270	3301	rVB	1094663	1763563	71.41%	9.982%
76	11.808	3348	3349	3353	rVB3	1005	470	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037779.D
 Acq On : 09 Oct 2024 14:44
 Operator : SY/MD
 Sample : P4349-07
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	11.902	3376	3378	3382	rVB6	715	428	0.02%	0.002%
78	12.130	3445	3449	3450	rBV2	663	429	0.02%	0.002%
79	12.178	3461	3464	3467	rVB5	1368	787	0.03%	0.004%
80	12.201	3467	3471	3473	rBV3	1068	999	0.04%	0.006%
81	12.223	3476	3478	3483	rVV3	720	596	0.02%	0.003%
82	12.291	3497	3499	3502	rVB2	882	441	0.02%	0.002%
83	12.445	3544	3547	3550	rVB3	969	621	0.03%	0.004%
84	12.467	3550	3554	3557	rBV3	811	573	0.02%	0.003%
85	12.525	3569	3572	3575	rBV2	832	462	0.02%	0.003%
86	12.590	3586	3592	3599	rBV7	1644	2216	0.09%	0.013%
87	12.770	3645	3648	3652	rVB4	706	519	0.02%	0.003%
88	12.930	3693	3698	3701	rVB5	580	492	0.02%	0.003%
89	12.956	3703	3706	3709	rBV4	816	563	0.02%	0.003%
90	12.975	3709	3712	3716	rVB3	751	444	0.02%	0.003%
91	13.059	3735	3738	3742	rBV3	545	482	0.02%	0.003%
92	13.342	3822	3826	3830	rBV5	676	681	0.03%	0.004%
93	13.458	3858	3862	3866	rBV5	1274	1437	0.06%	0.008%
94	13.728	3943	3946	3947	rBV2	879	519	0.02%	0.003%
95	13.892	3994	3997	3999	rBV3	659	465	0.02%	0.003%
96	14.130	4067	4071	4076	rBV5	1111	1122	0.05%	0.006%
97	14.332	4130	4134	4135	rBV2	670	434	0.02%	0.002%
98	14.544	4197	4200	4204	rBV6	1079	842	0.03%	0.005%
99	14.869	4299	4301	4303	rBV2	872	455	0.02%	0.003%
100	15.355	4449	4452	4453	rBV3	1011	561	0.02%	0.003%




Sum of corrected areas: 17666648

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037779.D
Acq On : 09 Oct 2024 14:44
Operator : SY/MD
Sample : P4349-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

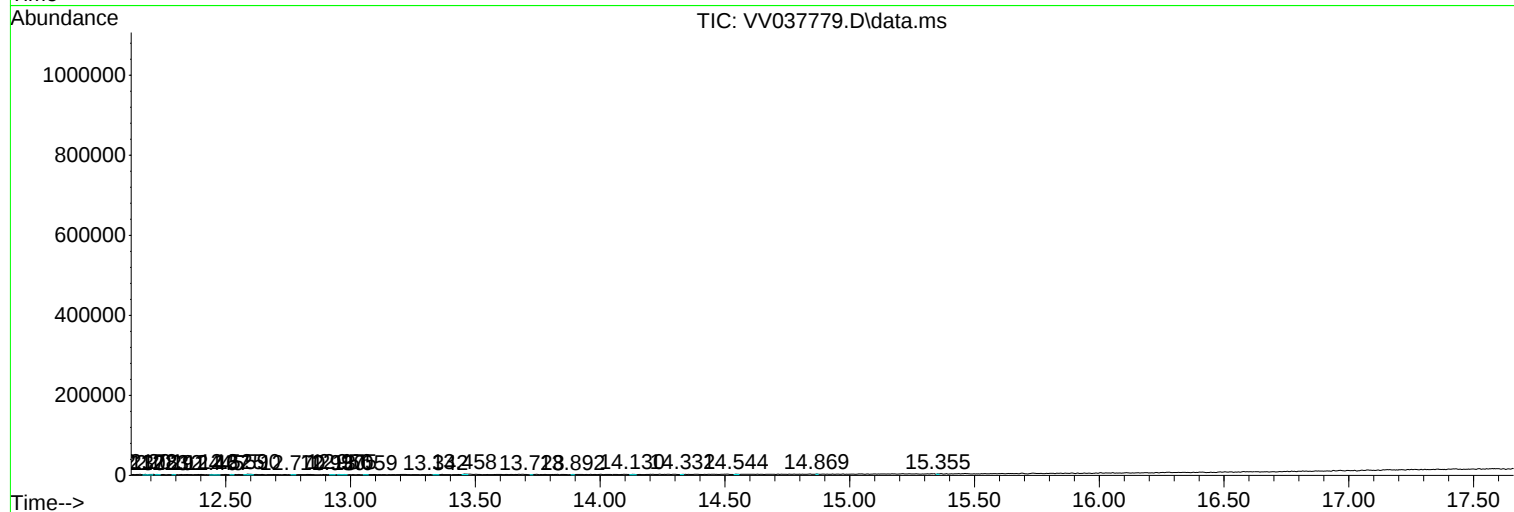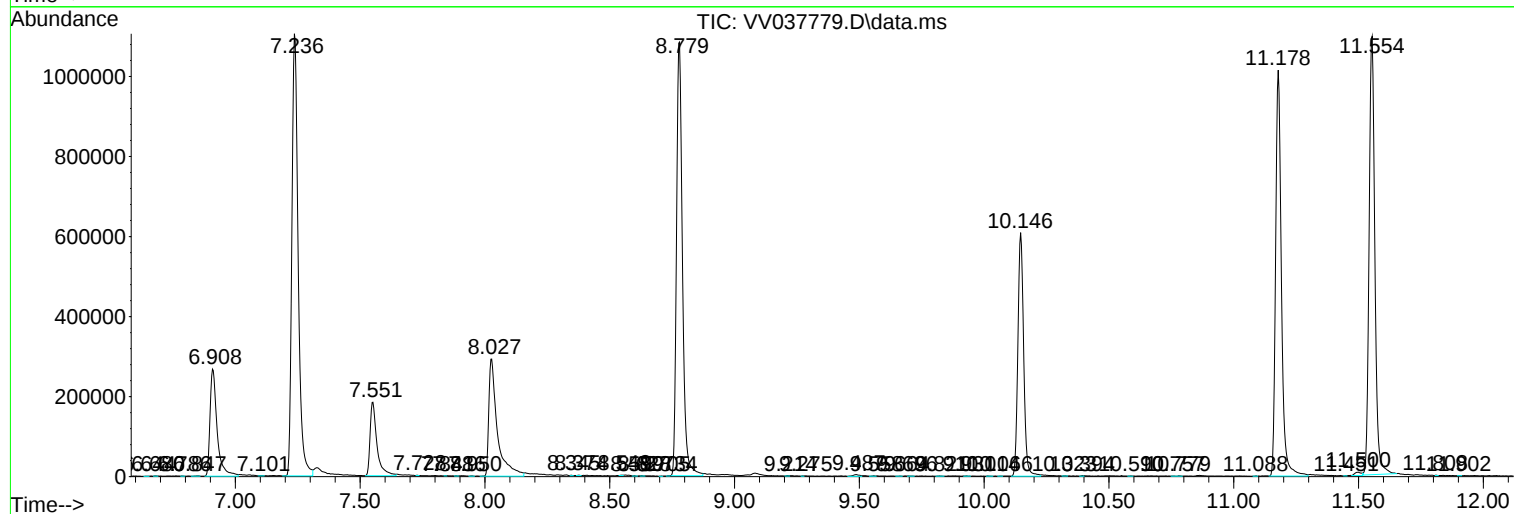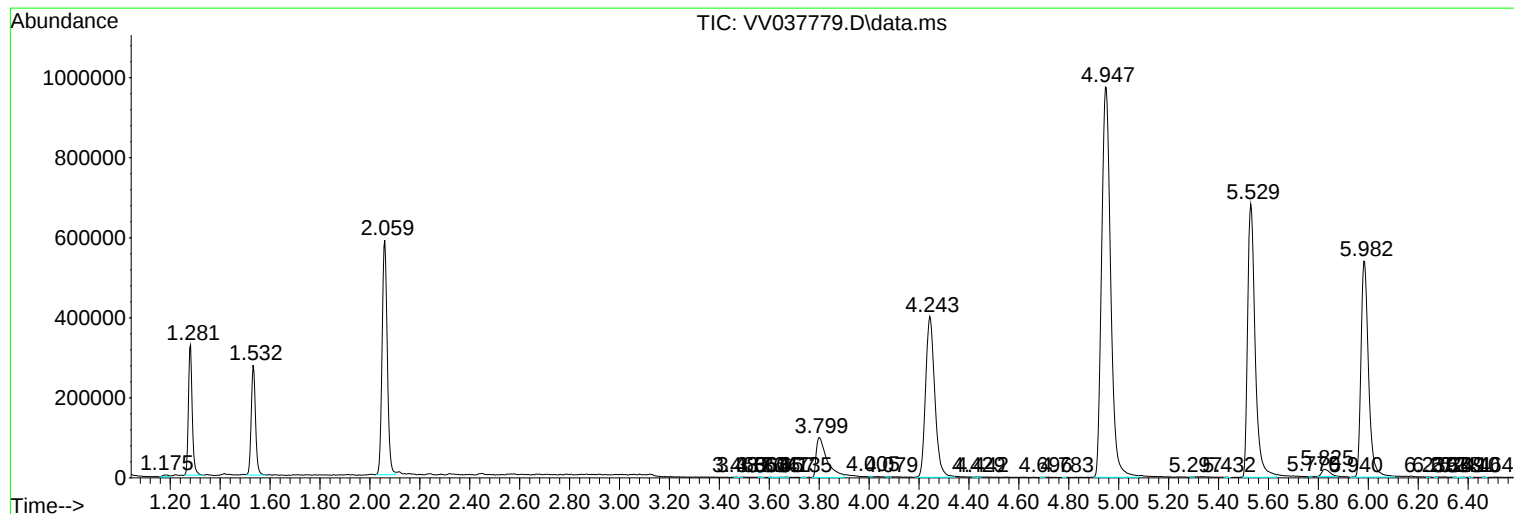

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037779.D
Acq On : 09 Oct 2024 14:44
Operator : SY/MD
Sample : P4349-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037779.D
Acq On : 09 Oct 2024 14:44
Operator : SY/MD
Sample : P4349-07
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------