

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037783.D
 Acq On : 09 Oct 2024 16:11
 Operator : SY/MD
 Sample : P4349-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

Signal : TIC: VV037783.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.175	36	42	52	rBV	7952	16192	0.65%	0.092%
2	1.282	68	75	92	rVB	333835	344820	13.94%	1.953%
3	1.355	93	98	104	rVB3	3771	4540	0.18%	0.026%
4	1.532	145	153	174	rVB	281413	327949	13.26%	1.857%
5	2.060	307	317	331	rBV	576298	823508	33.30%	4.664%
6	3.249	685	687	691	rVB2	1204	642	0.03%	0.004%
7	3.275	691	695	697	rBV3	750	497	0.02%	0.003%
8	3.384	727	729	733	rBV3	811	459	0.02%	0.003%
9	3.622	798	803	806	rBV2	608	591	0.02%	0.003%
10	3.799	850	858	886	rBV	106626	297461	12.03%	1.685%
11	4.243	978	996	1024	rBV	401512	1016083	41.08%	5.754%
12	4.494	1071	1074	1078	rBV4	915	637	0.03%	0.004%
13	4.526	1081	1084	1089	rVB4	870	615	0.02%	0.003%
14	4.593	1101	1105	1108	rBV4	816	696	0.03%	0.004%
15	4.609	1108	1110	1113	rVV2	885	533	0.02%	0.003%
16	4.658	1118	1125	1128	rBV4	845	865	0.03%	0.005%
17	4.683	1132	1133	1140	rVB3	665	540	0.02%	0.003%
18	4.844	1179	1183	1188	rBV5	585	684	0.03%	0.004%
19	4.950	1197	1216	1252	rBV2	979178	2473264	100.00%	14.006%
20	5.426	1361	1364	1371	rVB4	689	665	0.03%	0.004%
21	5.465	1371	1376	1378	rBV5	765	677	0.03%	0.004%
22	5.529	1385	1396	1428	rBV	693406	1422237	57.50%	8.054%
23	5.831	1480	1490	1506	rVV5	14190	31796	1.29%	0.180%
24	5.889	1506	1508	1511	rVB4	1200	698	0.03%	0.004%
25	5.931	1518	1521	1525	rBV4	1019	594	0.02%	0.003%
26	5.982	1525	1537	1565	rBV	540906	1119574	45.27%	6.340%
27	6.307	1635	1638	1643	rVB6	877	598	0.02%	0.003%
28	6.413	1668	1671	1673	rBV3	659	449	0.02%	0.003%
29	6.487	1691	1694	1699	rVB4	679	518	0.02%	0.003%
30	6.532	1705	1708	1712	rVB5	615	514	0.02%	0.003%
31	6.645	1739	1743	1746	rVB4	825	766	0.03%	0.004%
32	6.757	1775	1778	1780	rBV	1115	711	0.03%	0.004%
33	6.799	1787	1791	1797	rVB5	1072	952	0.04%	0.005%
34	6.908	1815	1825	1852	rBV	268082	521164	21.07%	2.951%
35	7.146	1895	1899	1904	rBV7	868	899	0.04%	0.005%
36	7.236	1916	1927	1961	rBV	1099563	1956029	79.09%	11.077%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037783.D
 Acq On : 09 Oct 2024 16:11
 Operator : SY/MD
 Sample : P4349-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.548	2015	2024	2051	rBV	184702	348005	14.07%	1.971%
38	7.895	2129	2132	2136	rVB4	1276	816	0.03%	0.005%
39	7.956	2146	2151	2153	rBV4	1034	889	0.04%	0.005%
40	8.024	2161	2172	2218	rBV2	316589	718446	29.05%	4.069%
41	8.336	2266	2269	2271	rBV3	1040	686	0.03%	0.004%
42	8.397	2285	2288	2291	rBV3	710	596	0.02%	0.003%
43	8.535	2328	2331	2332	rBV	1113	578	0.02%	0.003%
44	8.641	2360	2364	2370	rBV7	1118	1050	0.04%	0.006%
45	8.706	2381	2384	2388	rBV4	699	559	0.02%	0.003%
46	8.780	2396	2407	2432	rBV	1089022	1799988	72.78%	10.194%
47	9.130	2510	2516	2521	rBV7	784	1029	0.04%	0.006%
48	9.243	2547	2551	2557	rBV5	822	1022	0.04%	0.006%
49	9.497	2626	2630	2638	rVB5	1555	1643	0.07%	0.009%
50	9.545	2638	2645	2648	rBV5	1055	1304	0.05%	0.007%
51	9.645	2672	2676	2682	rVB3	658	720	0.03%	0.004%
52	9.770	2712	2715	2719	rBV4	852	718	0.03%	0.004%
53	9.828	2729	2733	2735	rBV4	895	476	0.02%	0.003%
54	9.966	2772	2776	2781	rVB5	807	779	0.03%	0.004%
55	10.146	2820	2832	2852	rBV	636417	1003153	40.56%	5.681%
56	10.333	2888	2890	2895	rVB3	953	645	0.03%	0.004%
57	10.439	2919	2923	2926	rVB4	645	483	0.02%	0.003%
58	10.461	2926	2930	2932	rBV2	604	525	0.02%	0.003%
59	10.606	2972	2975	2980	rBV2	864	945	0.04%	0.005%
60	10.667	2991	2994	2999	rBV4	792	782	0.03%	0.004%
61	10.738	3013	3016	3021	rVB3	809	549	0.02%	0.003%
62	10.780	3027	3029	3033	rVV3	834	626	0.03%	0.004%
63	10.876	3056	3059	3063	rVB4	912	609	0.02%	0.003%
64	10.953	3079	3083	3088	rBV3	468	488	0.02%	0.003%
65	11.017	3096	3103	3105	rBV4	695	673	0.03%	0.004%
66	11.136	3133	3140	3142	rBV4	922	865	0.03%	0.005%
67	11.178	3142	3153	3191	rBV	997677	1622286	65.59%	9.187%
68	11.394	3217	3220	3223	rBV4	1170	898	0.04%	0.005%
69	11.448	3234	3237	3240	rVB4	1066	589	0.02%	0.003%
70	11.509	3245	3256	3258	rBV7	5694	9066	0.37%	0.051%
71	11.554	3259	3270	3298	rVV	1081597	1744178	70.52%	9.877%
72	11.824	3352	3354	3357	rVB3	1184	740	0.03%	0.004%
73	11.850	3359	3362	3365	rVV5	1304	875	0.04%	0.005%
74	11.940	3387	3390	3392	rBV4	801	449	0.02%	0.003%
75	11.969	3392	3399	3401	rVV5	772	835	0.03%	0.005%
76	12.371	3518	3524	3525	rBV4	804	691	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037783.D
 Acq On : 09 Oct 2024 16:11
 Operator : SY/MD
 Sample : P4349-11
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAG4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.532	3570	3574	3576	rVB2	726	446	0.02%	0.003%
78	12.670	3615	3617	3622	rBV3	697	506	0.02%	0.003%
79	12.709	3626	3629	3633	rBV3	647	616	0.02%	0.003%
80	12.767	3643	3647	3652	rBV3	1175	1395	0.06%	0.008%
81	12.886	3681	3684	3689	rBV4	580	449	0.02%	0.003%
82	12.914	3689	3693	3696	rBV5	668	537	0.02%	0.003%
83	13.088	3743	3747	3749	rBV4	686	529	0.02%	0.003%
84	13.130	3756	3760	3767	rBV8	739	893	0.04%	0.005%
85	13.181	3774	3776	3781	rVB5	1117	826	0.03%	0.005%
86	13.223	3784	3789	3791	rBV4	618	483	0.02%	0.003%
87	13.397	3837	3843	3848	rBV4	690	859	0.03%	0.005%
88	13.426	3848	3852	3856	rBV3	977	869	0.04%	0.005%
89	13.477	3866	3868	3870	rBV2	748	442	0.02%	0.003%
90	13.558	3890	3893	3895	rBV3	873	641	0.03%	0.004%
91	13.631	3914	3916	3920	rVB2	923	458	0.02%	0.003%
92	13.686	3928	3933	3940	rBV8	1210	1594	0.06%	0.009%
93	14.049	4044	4046	4052	rBV5	620	523	0.02%	0.003%
94	14.387	4146	4151	4156	rBV4	907	1059	0.04%	0.006%
95	14.596	4212	4216	4221	rBV5	1592	1487	0.06%	0.008%
96	14.648	4228	4232	4233	rBV3	929	629	0.03%	0.004%
97	14.840	4290	4292	4297	rVB5	1046	609	0.02%	0.003%
98	14.985	4335	4337	4346	rVB6	1328	1289	0.05%	0.007%
99	15.027	4347	4350	4354	rVV4	959	699	0.03%	0.004%
100	15.561	4514	4516	4519	rBV3	1182	681	0.03%	0.004%




Sum of corrected areas: 17658190

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037783.D
Acq On : 09 Oct 2024 16:11
Operator : SY/MD
Sample : P4349-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

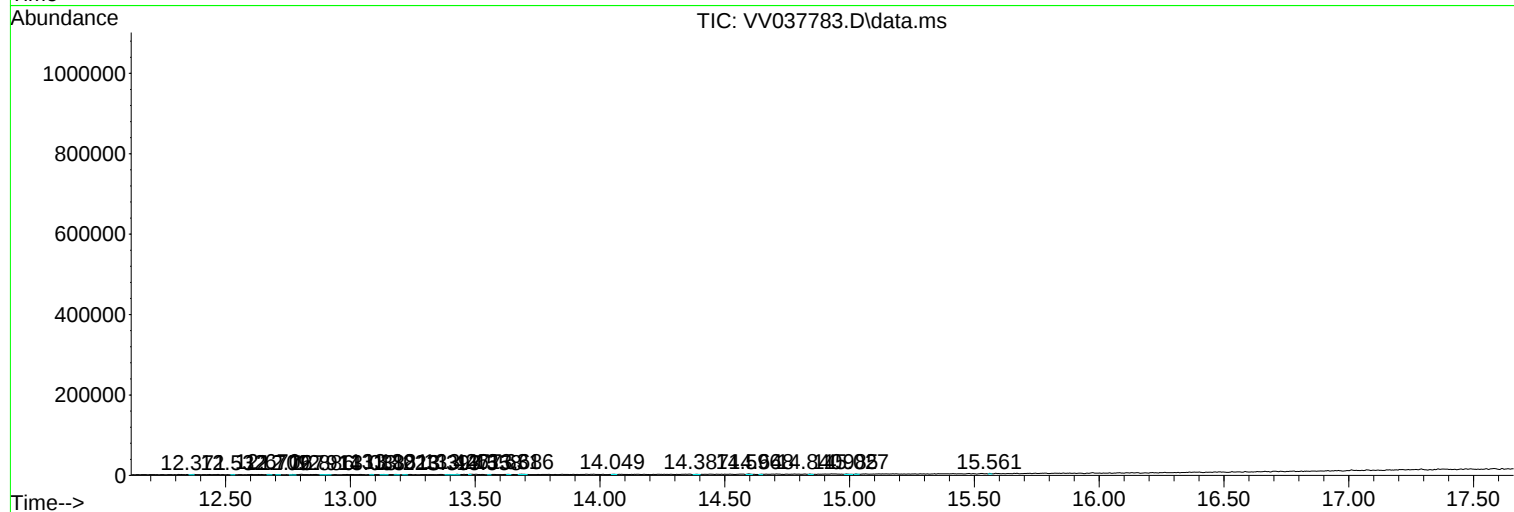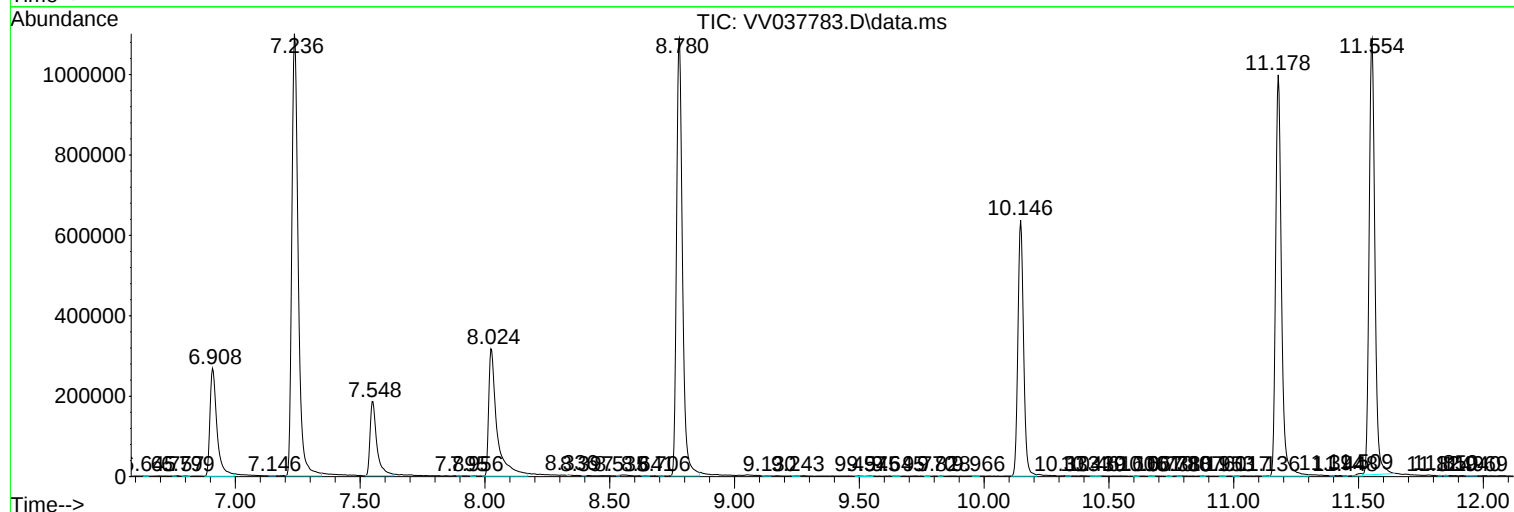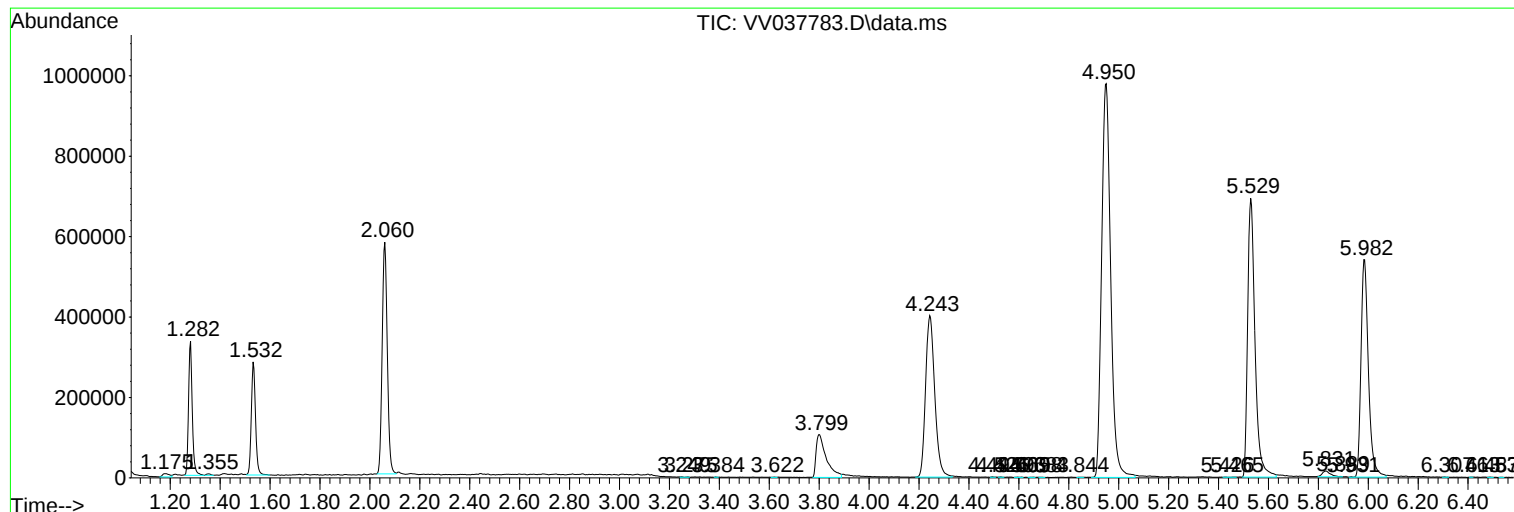

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037783.D
Acq On : 09 Oct 2024 16:11
Operator : SY/MD
Sample : P4349-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037783.D
Acq On : 09 Oct 2024 16:11
Operator : SY/MD
Sample : P4349-11
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAG4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------