

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037785.D
 Acq On : 09 Oct 2024 16:54
 Operator : SY/MD
 Sample : P4349-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037785.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.176	36	42	51	rBV	5689	10061	0.41%	0.058%
2	1.278	67	74	90	rBV	320269	339614	13.96%	1.955%
3	1.532	145	153	169	rVB	266475	319321	13.12%	1.838%
4	2.056	306	316	330	rBV	573332	825976	33.94%	4.755%
5	3.249	683	687	693	rBV5	739	572	0.02%	0.003%
6	3.397	729	733	734	rBV4	592	463	0.02%	0.003%
7	3.487	758	761	765	rBV3	830	519	0.02%	0.003%
8	3.545	775	779	785	rBV4	665	743	0.03%	0.004%
9	3.609	797	799	805	rVB4	932	804	0.03%	0.005%
10	3.655	808	813	819	rBV4	645	701	0.03%	0.004%
11	3.799	850	858	896	rBV2	103089	313197	12.87%	1.803%
12	4.076	942	944	947	rVB3	759	421	0.02%	0.002%
13	4.243	979	996	1029	rBV	394823	1006635	41.37%	5.795%
14	4.606	1106	1109	1112	rBV3	551	463	0.02%	0.003%
15	4.728	1141	1147	1148	rBV3	627	489	0.02%	0.003%
16	4.796	1164	1168	1170	rBV2	570	508	0.02%	0.003%
17	4.947	1201	1215	1259	rBV2	957721	2433519	100.00%	14.009%
18	5.281	1316	1319	1322	rBV3	963	718	0.03%	0.004%
19	5.307	1322	1327	1329	rVV3	652	560	0.02%	0.003%
20	5.529	1385	1396	1437	rBV	663263	1395126	57.33%	8.031%
21	5.825	1479	1488	1501	rBV3	16721	36343	1.49%	0.209%
22	5.982	1524	1537	1569	rBV	531498	1116201	45.87%	6.425%
23	6.227	1611	1613	1616	rVB4	1041	495	0.02%	0.003%
24	6.246	1616	1619	1623	rVB6	1242	953	0.04%	0.005%
25	6.278	1624	1629	1633	rBV7	925	995	0.04%	0.006%
26	6.359	1651	1654	1659	rBB6	1026	698	0.03%	0.004%
27	6.510	1699	1701	1705	rVB3	661	495	0.02%	0.003%
28	6.532	1705	1708	1710	rBV3	862	521	0.02%	0.003%
29	6.555	1712	1715	1719	rVB5	773	598	0.02%	0.003%
30	6.757	1776	1778	1781	rVB	1023	533	0.02%	0.003%
31	6.809	1790	1794	1796	rBV4	813	585	0.02%	0.003%
32	6.828	1797	1800	1805	rVB4	744	524	0.02%	0.003%
33	6.908	1815	1825	1850	rBV	262010	505238	20.76%	2.908%
34	7.236	1916	1927	1949	rBV	1087080	1907647	78.39%	10.982%
35	7.465	1996	1998	2002	rBV2	1195	685	0.03%	0.004%
36	7.548	2014	2024	2047	rBV	179089	335369	13.78%	1.931%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037785.D
 Acq On : 09 Oct 2024 16:54
 Operator : SY/MD
 Sample : P4349-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	7.732	2079	2081	2082	rBV	853	421	0.02%	0.002%
38	7.947	2145	2148	2153	rVB4	815	702	0.03%	0.004%
39	7.986	2156	2160	2162	rBV3	535	439	0.02%	0.003%
40	8.027	2164	2173	2216	rBV2	310920	717069	29.47%	4.128%
41	8.407	2287	2291	2292	rBV3	652	461	0.02%	0.003%
42	8.548	2326	2335	2337	rBV6	2502	3078	0.13%	0.018%
43	8.677	2369	2375	2380	rVB6	1277	1522	0.06%	0.009%
44	8.709	2382	2385	2387	rBV3	714	485	0.02%	0.003%
45	8.780	2395	2407	2439	rBV	1044000	1757641	72.23%	10.118%
46	9.034	2484	2486	2489	rBV4	765	465	0.02%	0.003%
47	9.082	2496	2501	2510	rVB6	5194	7743	0.32%	0.045%
48	9.278	2558	2562	2564	rBV4	923	800	0.03%	0.005%
49	9.313	2569	2573	2577	rVV5	1085	838	0.03%	0.005%
50	9.391	2594	2597	2603	rVB4	935	792	0.03%	0.005%
51	9.445	2611	2614	2616	rBV4	934	520	0.02%	0.003%
52	9.481	2620	2625	2633	rBV5	3342	5848	0.24%	0.034%
53	9.632	2666	2672	2674	rBV4	742	701	0.03%	0.004%
54	9.696	2688	2692	2697	rVB6	548	492	0.02%	0.003%
55	9.911	2754	2759	2761	rBV2	1047	870	0.04%	0.005%
56	10.082	2808	2812	2817	rBV3	645	626	0.03%	0.004%
57	10.146	2818	2832	2854	rBV	618166	988034	40.60%	5.688%
58	10.381	2902	2905	2908	rVV4	1189	890	0.04%	0.005%
59	10.400	2908	2911	2913	rVV4	1007	715	0.03%	0.004%
60	10.413	2913	2915	2918	rVV4	944	532	0.02%	0.003%
61	10.532	2948	2952	2956	rBV2	509	434	0.02%	0.002%
62	10.577	2960	2966	2968	rBV3	993	663	0.03%	0.004%
63	10.789	3029	3032	3041	rVB5	1308	1514	0.06%	0.009%
64	10.854	3049	3052	3056	rBV4	1643	1561	0.06%	0.009%
65	10.953	3079	3083	3088	rBV3	642	743	0.03%	0.004%
66	11.124	3130	3136	3140	rBV5	781	838	0.03%	0.005%
67	11.178	3142	3153	3189	rBV	987965	1567463	64.41%	9.023%
68	11.458	3236	3240	3244	rBV6	1194	1265	0.05%	0.007%
69	11.506	3246	3255	3258	rBV6	5466	8505	0.35%	0.049%
70	11.551	3259	3269	3296	rVV	1062185	1717731	70.59%	9.888%
71	11.886	3370	3373	3376	rBV3	686	511	0.02%	0.003%
72	12.030	3416	3418	3423	rVB3	758	501	0.02%	0.003%
73	12.082	3432	3434	3438	rBV4	1281	702	0.03%	0.004%
74	12.101	3438	3440	3444	rVV3	678	492	0.02%	0.003%
75	12.329	3509	3511	3516	rVB3	814	541	0.02%	0.003%
76	12.551	3577	3580	3585	rBV2	719	518	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037785.D
 Acq On : 09 Oct 2024 16:54
 Operator : SY/MD
 Sample : P4349-13
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAJ0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	12.651	3605	3611	3613	rBV3	1014	985	0.04%	0.006%
78	12.664	3613	3615	3620	rVB3	1341	912	0.04%	0.005%
79	12.706	3626	3628	3632	rVB2	685	439	0.02%	0.003%
80	12.731	3632	3636	3637	rBV3	1032	572	0.02%	0.003%
81	12.892	3683	3686	3691	rVB3	781	537	0.02%	0.003%
82	12.927	3691	3697	3699	rBV5	898	826	0.03%	0.005%
83	12.956	3704	3706	3711	rVB3	1134	713	0.03%	0.004%
84	13.185	3774	3777	3779	rBV2	975	570	0.02%	0.003%
85	13.271	3801	3804	3808	rVB4	836	521	0.02%	0.003%
86	13.551	3888	3891	3896	rVB5	880	797	0.03%	0.005%
87	13.583	3896	3901	3904	rBV4	908	849	0.03%	0.005%
88	13.648	3919	3921	3926	rVB2	843	628	0.03%	0.004%
89	13.686	3929	3933	3938	rVB4	816	725	0.03%	0.004%
90	13.741	3947	3950	3955	rVB2	694	664	0.03%	0.004%
91	13.860	3984	3987	3989	rBV3	603	429	0.02%	0.002%
92	13.956	4014	4017	4020	rBV2	838	662	0.03%	0.004%
93	14.114	4063	4066	4070	rBV3	690	605	0.02%	0.003%
94	14.204	4089	4094	4095	rBV3	1104	822	0.03%	0.005%
95	14.259	4109	4111	4118	rVB4	1729	1388	0.06%	0.008%
96	14.365	4141	4144	4148	rVB3	922	570	0.02%	0.003%
97	14.644	4228	4231	4234	rVB4	1438	929	0.04%	0.005%
98	14.763	4265	4268	4272	rBV4	830	727	0.03%	0.004%
99	14.956	4326	4328	4333	rBV4	828	755	0.03%	0.004%
100	15.541	4508	4510	4513	rBV4	1240	876	0.04%	0.005%




Sum of corrected areas: 17371457

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037785.D
Acq On : 09 Oct 2024 16:54
Operator : SY/MD
Sample : P4349-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

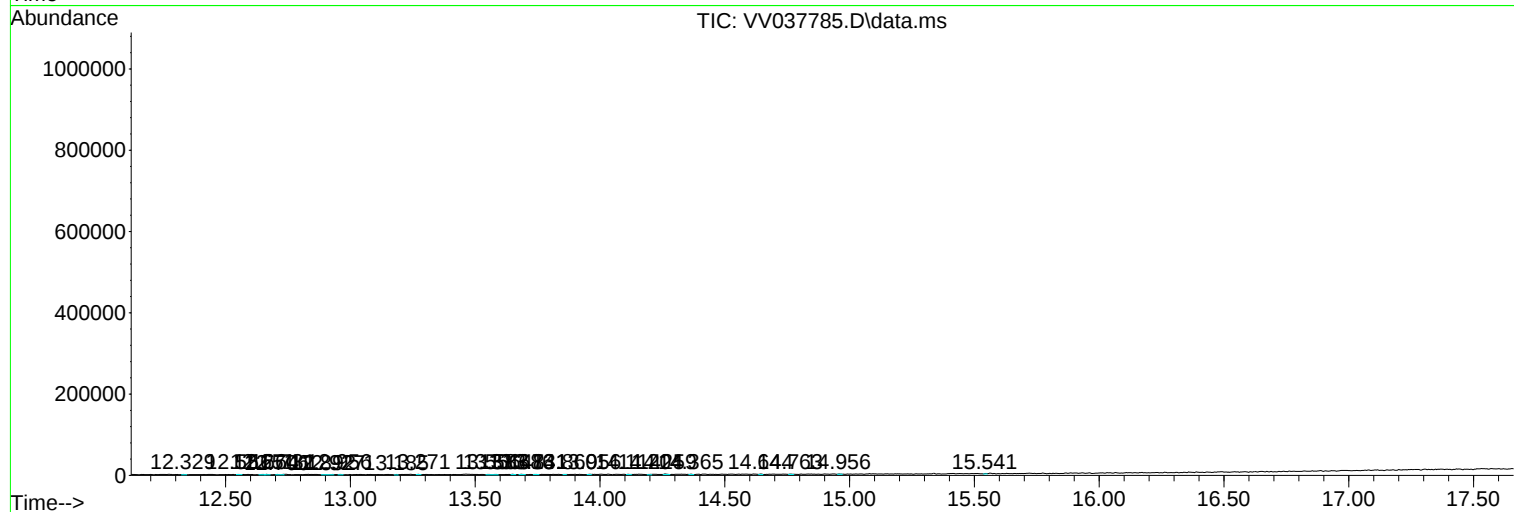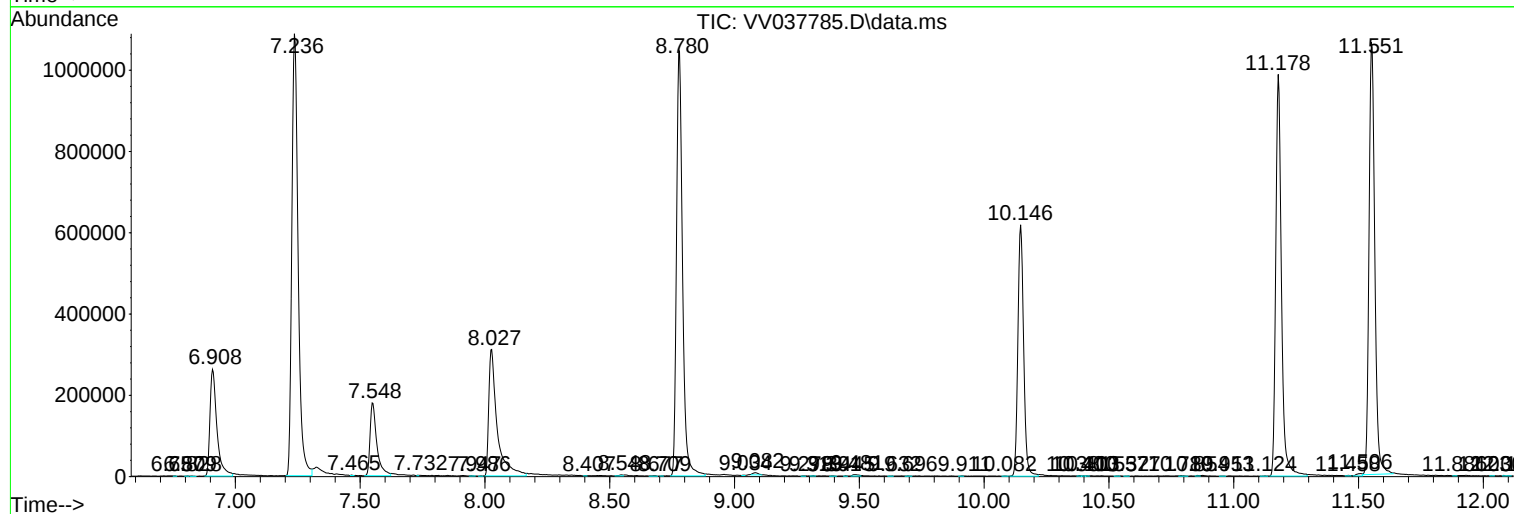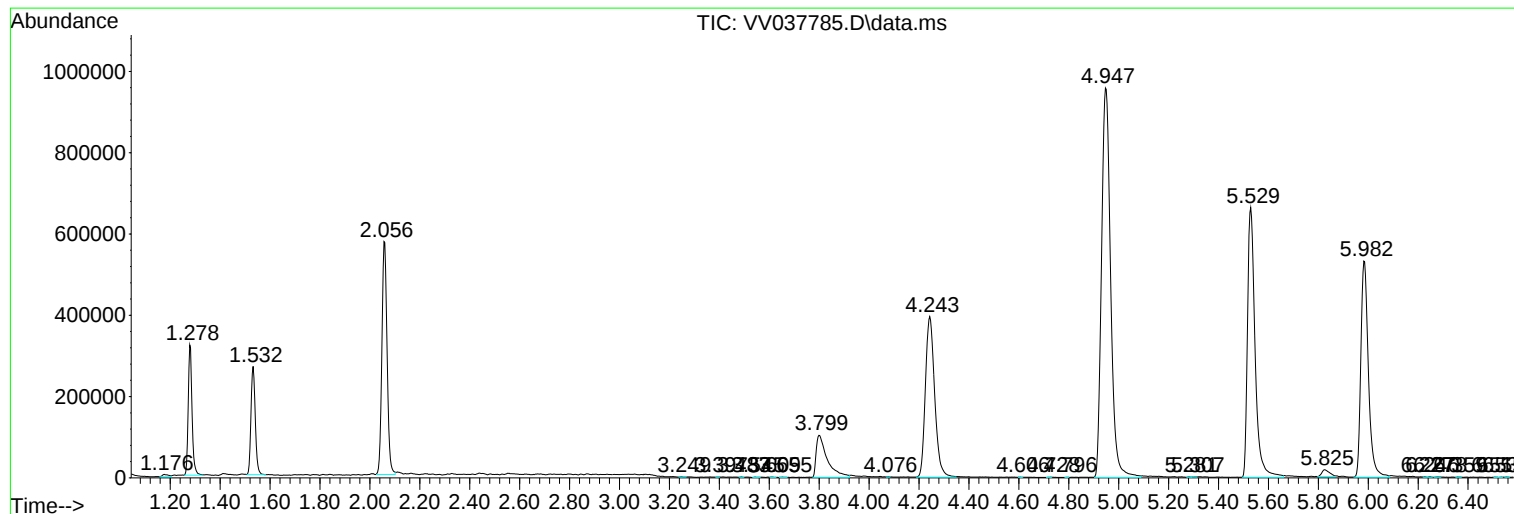

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037785.D
Acq On : 09 Oct 2024 16:54
Operator : SY/MD
Sample : P4349-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037785.D
Acq On : 09 Oct 2024 16:54
Operator : SY/MD
Sample : P4349-13
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAJ0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc