

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037786.D
 Acq On : 09 Oct 2024 17:15
 Operator : SY/MD
 Sample : P4349-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M

Title : VOC Analysis

Signal : TIC: VV037786.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.278	68	74	91	rVB	311562	330083	13.67%	1.918%
2	1.532	146	153	168	rVB	266921	315608	13.07%	1.834%
3	2.059	307	317	332	rBV	561032	812376	33.65%	4.721%
4	3.387	728	730	732	rBV2	636	310	0.01%	0.002%
5	3.535	774	776	779	rBV3	493	309	0.01%	0.002%
6	3.593	792	794	796	rBV	640	270	0.01%	0.002%
7	3.606	796	798	800	rVB	407	120	0.00%	0.001%
8	3.690	822	824	827	rBV	422	228	0.01%	0.001%
9	3.709	828	830	832	rVB2	564	210	0.01%	0.001%
10	3.728	832	836	838	rBV2	664	412	0.02%	0.002%
11	3.799	850	858	888	rBV	102335	291422	12.07%	1.694%
12	4.182	975	977	978	rBV2	1144	565	0.02%	0.003%
13	4.243	982	996	1028	rVB	390070	990116	41.02%	5.754%
14	4.564	1093	1096	1097	rBV2	571	350	0.01%	0.002%
15	4.603	1104	1108	1114	rVB4	1102	1218	0.05%	0.007%
16	4.632	1114	1117	1120	rBV2	1122	753	0.03%	0.004%
17	4.654	1122	1124	1128	rVB3	800	506	0.02%	0.003%
18	4.677	1129	1131	1134	rVV3	545	288	0.01%	0.002%
19	4.696	1135	1137	1140	rVB3	583	308	0.01%	0.002%
20	4.712	1140	1142	1145	rBV2	367	172	0.01%	0.001%
21	4.802	1166	1170	1173	rBV3	753	735	0.03%	0.004%
22	4.850	1183	1185	1186	rBV3	605	276	0.01%	0.002%
23	4.883	1191	1195	1198	rBV4	413	294	0.01%	0.002%
24	4.950	1200	1216	1250	rBV2	963926	2413941	100.00%	14.028%
25	5.288	1317	1321	1324	rBV4	972	745	0.03%	0.004%
26	5.458	1372	1374	1375	rBV2	499	208	0.01%	0.001%
27	5.468	1375	1377	1378	rBV2	534	241	0.01%	0.001%
28	5.529	1385	1396	1431	rBV	674763	1401230	58.05%	8.143%
29	5.985	1525	1538	1564	rBV	530922	1099150	45.53%	6.387%
30	6.239	1616	1617	1621	rVB2	1148	638	0.03%	0.004%
31	6.387	1661	1663	1666	rBV2	416	330	0.01%	0.002%
32	6.426	1672	1675	1676	rBV	392	271	0.01%	0.002%
33	6.471	1685	1689	1691	rVB3	743	491	0.02%	0.003%
34	6.490	1691	1695	1700	rBV4	949	811	0.03%	0.005%
35	6.513	1700	1702	1703	rBV	423	149	0.01%	0.001%
36	6.522	1703	1705	1709	rVB3	846	544	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037786.D
 Acq On : 09 Oct 2024 17:15
 Operator : SY/MD
 Sample : P4349-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

37	6.564	1714	1718	1720	rBV3	417	291	0.01%	0.002%
38	6.583	1722	1724	1725	rBV2	548	239	0.01%	0.001%
39	6.641	1739	1742	1746	rBV3	1278	965	0.04%	0.006%
40	6.738	1768	1772	1774	rBV4	691	455	0.02%	0.003%
41	6.783	1784	1786	1792	rVB4	737	743	0.03%	0.004%
42	6.818	1792	1797	1798	rBV4	784	563	0.02%	0.003%
43	6.834	1800	1802	1805	rVB2	630	252	0.01%	0.001%
44	6.850	1805	1807	1811	rBV3	459	296	0.01%	0.002%
45	6.908	1815	1825	1858	rBV	256838	506753	20.99%	2.945%
46	7.162	1900	1904	1907	rBV5	1021	847	0.04%	0.005%
47	7.236	1916	1927	1958	rBV	1084056	1907095	79.00%	11.083%
48	7.548	2016	2024	2065	rBV	172422	342439	14.19%	1.990%
49	7.905	2132	2135	2137	rBV3	1043	688	0.03%	0.004%
50	7.940	2144	2146	2151	rBV3	416	231	0.01%	0.001%
51	7.979	2157	2158	2159	rBV	478	145	0.01%	0.001%
52	8.027	2164	2173	2216	rBV2	310851	706363	29.26%	4.105%
53	8.686	2376	2378	2382	rBV4	505	434	0.02%	0.003%
54	8.779	2396	2407	2445	rBV	1078887	1796781	74.43%	10.442%
55	9.242	2547	2551	2553	rBV3	591	507	0.02%	0.003%
56	9.352	2584	2585	2588	rBV2	470	320	0.01%	0.002%
57	9.464	2619	2620	2621	rBV2	325	108	0.00%	0.001%
58	9.474	2621	2623	2625	rVV	415	180	0.01%	0.001%
59	9.493	2626	2629	2630	rBV2	456	218	0.01%	0.001%
60	9.644	2673	2676	2679	rVB2	797	491	0.02%	0.003%
61	9.673	2679	2685	2687	rBV5	851	787	0.03%	0.005%
62	9.706	2692	2695	2696	rBV2	606	325	0.01%	0.002%
63	9.747	2704	2708	2711	rBV2	225	187	0.01%	0.001%
64	9.779	2715	2718	2719	rBV	307	179	0.01%	0.001%
65	9.850	2734	2740	2742	rBV4	562	531	0.02%	0.003%
66	9.886	2749	2751	2755	rVB3	583	373	0.02%	0.002%
67	9.902	2755	2756	2757	rBV	409	123	0.01%	0.001%
68	9.940	2764	2768	2770	rBV4	820	529	0.02%	0.003%
69	9.995	2781	2785	2787	rBV2	577	396	0.02%	0.002%
70	10.027	2793	2795	2799	rBV2	869	447	0.02%	0.003%
71	10.053	2801	2803	2804	rBV	383	123	0.01%	0.001%
72	10.078	2809	2811	2813	rBV	601	337	0.01%	0.002%
73	10.146	2820	2832	2853	rBV	618040	987804	40.92%	5.740%
74	10.416	2914	2916	2918	rBV2	815	358	0.01%	0.002%
75	10.432	2919	2921	2923	rVV2	432	111	0.00%	0.001%
76	10.480	2934	2936	2937	rBV	357	165	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
 Data File : VV037786.D
 Acq On : 09 Oct 2024 17:15
 Operator : SY/MD
 Sample : P4349-14
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 EOAH0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Title : VOC Analysis

77	10.522	2947	2949	2951	rBV3	347	184	0.01%	0.001%
78	10.564	2957	2962	2967	rBV4	924	1062	0.04%	0.006%
79	10.641	2984	2986	2987	rBV4	432	184	0.01%	0.001%
80	10.702	3000	3005	3009	rBV4	636	594	0.02%	0.003%
81	10.738	3014	3016	3019	rVB	606	278	0.01%	0.002%
82	10.760	3020	3023	3026	rBV3	575	435	0.02%	0.003%
83	10.844	3044	3049	3050	rBV3	626	422	0.02%	0.002%
84	10.853	3050	3052	3053	rBV	427	160	0.01%	0.001%
85	10.898	3064	3066	3067	rBV	277	89	0.00%	0.001%
86	10.921	3071	3073	3074	rBV	216	95	0.00%	0.001%
87	10.931	3074	3076	3078	rBV2	278	153	0.01%	0.001%
88	11.088	3121	3125	3128	rBV3	545	353	0.01%	0.002%
89	11.104	3128	3130	3132	rBV2	591	308	0.01%	0.002%
90	11.130	3136	3138	3141	rBV	675	491	0.02%	0.003%
91	11.178	3143	3153	3178	rBV	976906	1576344	65.30%	9.161%
92	11.554	3259	3270	3305	rVB	1058714	1697071	70.30%	9.862%
93	12.059	3423	3427	3430	rBV4	1167	1025	0.04%	0.006%
94	12.316	3505	3507	3509	rBV3	610	268	0.01%	0.002%
95	12.365	3519	3522	3523	rBV2	487	219	0.01%	0.001%
96	12.371	3523	3524	3525	rBV	857	191	0.01%	0.001%
97	12.493	3559	3562	3563	rBV	463	288	0.01%	0.002%
98	12.754	3640	3643	3646	rBV3	908	719	0.03%	0.004%
99	13.004	3718	3721	3724	rVB3	764	477	0.02%	0.003%
100	13.667	3924	3927	3929	rBV3	1000	614	0.03%	0.004%




Sum of corrected areas: 17207881

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037786.D
Acq On : 09 Oct 2024 17:15
Operator : SY/MD
Sample : P4349-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

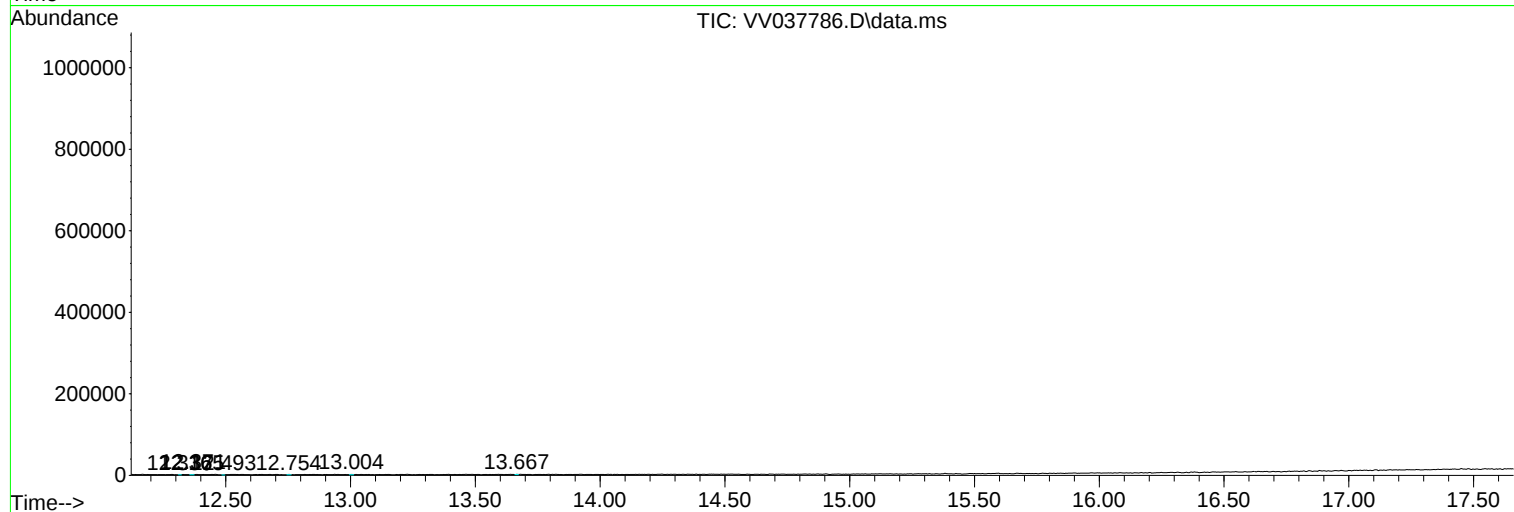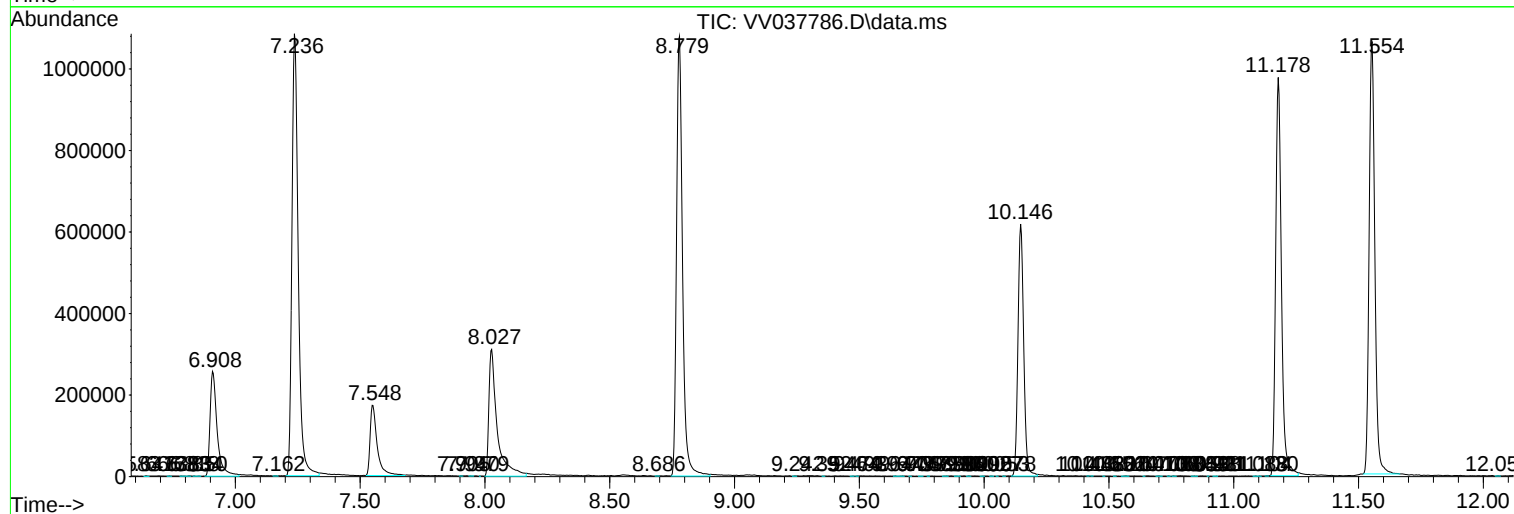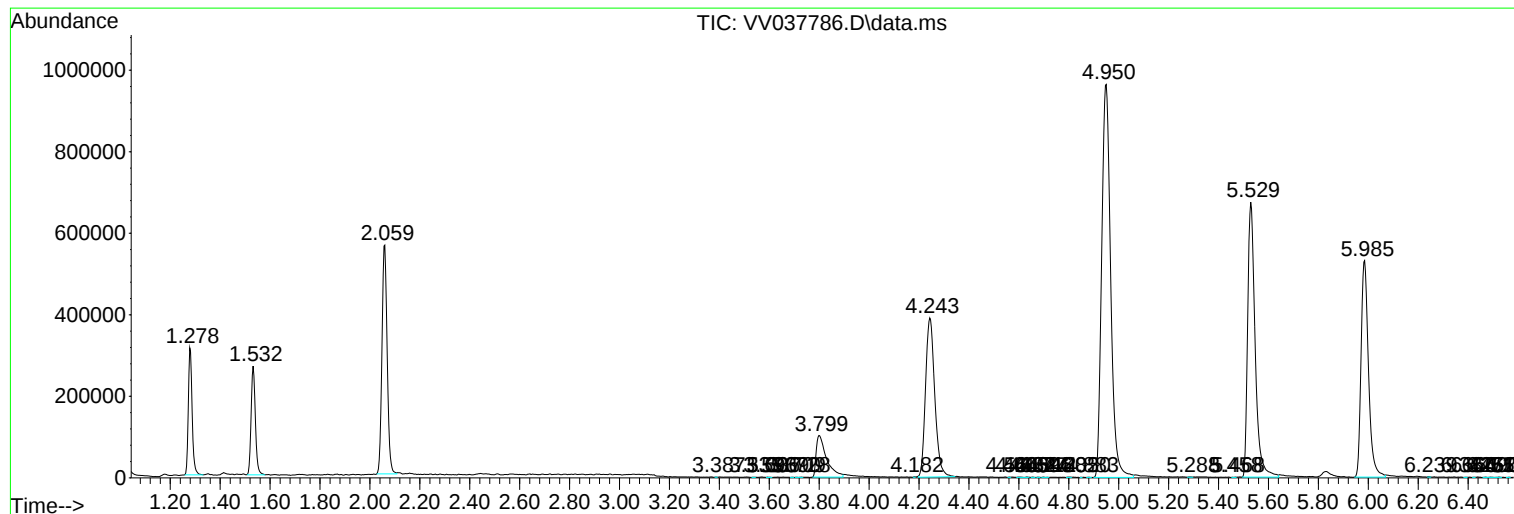

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037786.D
Acq On : 09 Oct 2024 17:15
Operator : SY/MD
Sample : P4349-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037786.D
Acq On : 09 Oct 2024 17:15
Operator : SY/MD
Sample : P4349-14
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
EOAH0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------