
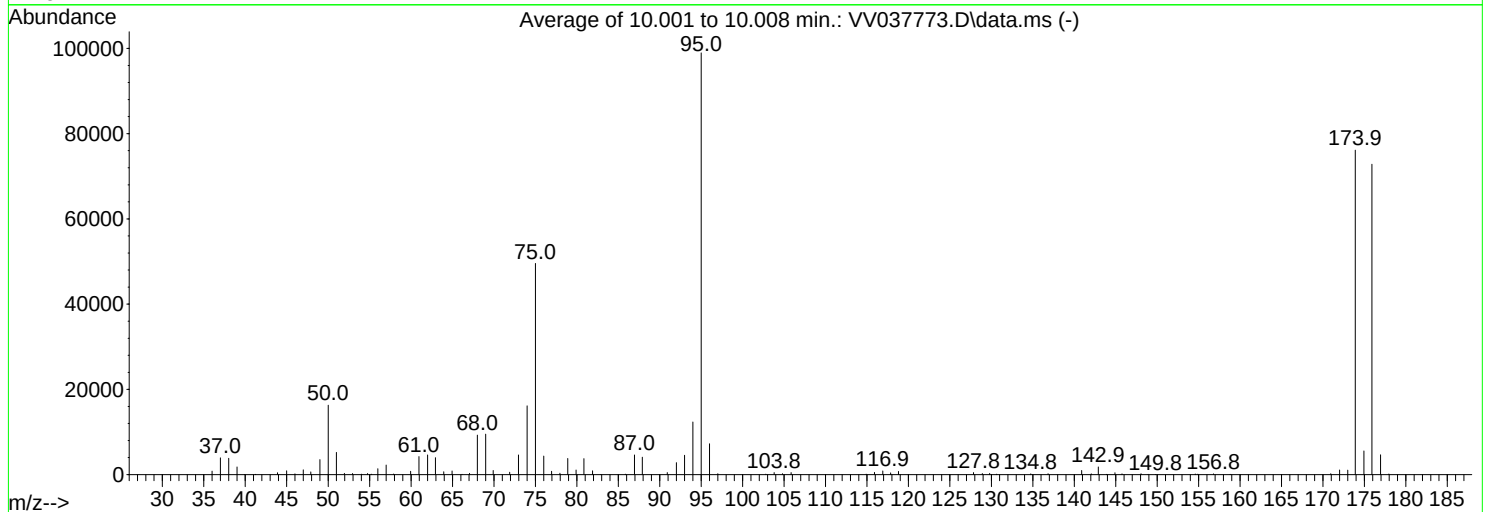


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV100924\
Data File : VV037773.D
Acq On : 09 Oct 2024 08:29
Operator : SY/MD
Sample : BFB390
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB390

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Title : VOC Analysis
Last Update : Thu Oct 10 03:11:31 2024

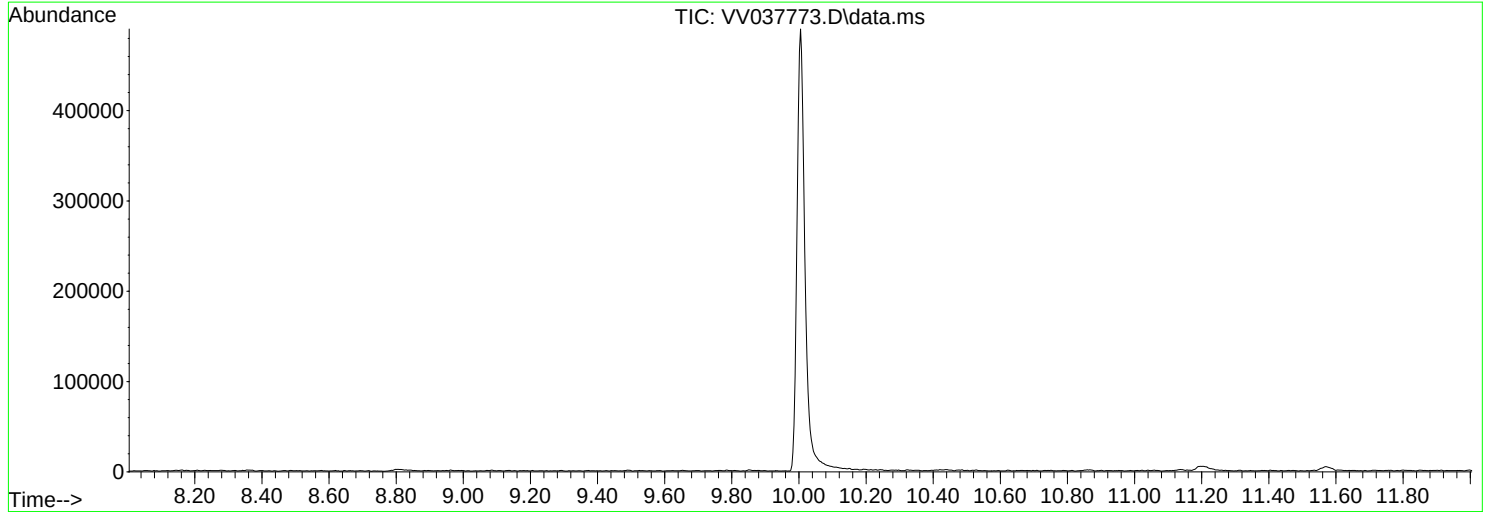

AutoFind: Scans 2787, 2788, 2789; Background Corrected with Scan 2777

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	16308	PASS
75	95	30	80	50.1	49544	PASS
95	95	100	100	100.0	98960	PASS
96	95	5	9	7.3	7265	PASS
173	174	0.00	2	1.4	1060	PASS
174	95	50	120	76.9	76149	PASS
175	174	5	9	7.3	5550	PASS
176	174	95	105	95.6	72824	PASS
177	176	5	10	6.4	4664	PASS

m/z	Abundance
39.80	315.0
43.80	620.0
59.80	122.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
36.00	847.0
37.00	4054.0
38.00	3864.0
39.00	1804.0
40.10	345.0
41.30	129.0
44.00	1080.0
45.00	883.0
46.00	254.0
47.00	1165.0
47.90	718.0
49.00	3412.0
50.00	16472.0
51.00	5645.0
51.90	270.0
53.00	298.0
54.00	129.0
54.80	270.0
56.00	1210.0
57.00	2435.0
57.90	112.0
60.10	741.0
60.90	4297.0
62.00	4828.0
63.00	3706.0
64.00	649.0
64.90	862.0
67.10	327.0
68.00	9236.0
69.00	9605.0
69.90	882.0
71.90	570.0
73.00	4599.0
74.00	15949.0
75.00	49024.0
76.00	4342.0
77.00	776.0
77.90	329.0
78.90	3701.0
79.90	1081.0
80.80	3702.0
81.90	896.0
82.90	120.0
85.80	121.0
87.00	4602.0
87.90	3981.0
90.90	442.0
92.00	2772.0
93.00	4371.0
94.00	11906.0
95.00	98552.0
96.00	7663.0
97.00	177.0
102.90	105.0
103.80	558.0
104.80	176.0
105.80	456.0
114.90	165.0
115.90	533.0
116.90	881.0
117.90	464.0
118.80	729.0
127.90	450.0
128.90	241.0
129.70	308.0
130.70	118.0
134.80	170.0
136.90	209.0
140.90	895.0
142.10	207.0
142.90	1659.0
143.90	142.0
145.00	385.0
145.80	184.0
148.00	188.0
154.60	205.0
155.00	155.0
156.90	158.0
158.80	134.0
170.90	240.0
172.00	1071.0
173.00	1011.0
173.90	72360.0
174.90	5506.0
175.90	70192.0
177.00	4620.0
177.90	164.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
36.00	870.0
37.00	4073.0
38.00	3985.0
39.00	1892.0
40.00	355.0
41.20	109.0
44.00	1122.0
45.00	930.0
46.00	201.0
47.00	1183.0
47.90	650.0
49.00	3623.0
50.00	16784.0
51.00	5437.0
51.90	301.0
53.00	275.0
54.00	145.0
54.70	259.0
55.20	182.0
56.00	1481.0
57.00	2335.0
57.90	158.0
60.00	880.0
61.00	4330.0
62.00	4736.0
62.90	4130.0
64.00	735.0
65.00	863.0
66.20	106.0
67.10	328.0
68.00	9664.0
69.00	9867.0
69.90	1008.0
71.90	575.0
73.00	4795.0
74.00	16656.0
75.00	51536.0
76.00	4520.0
77.00	825.0
77.90	365.0
78.90	3880.0
79.90	1149.0
80.90	3825.0
81.90	933.0
85.80	132.0
86.90	4817.0
87.90	4167.0
90.90	517.0
92.00	2949.0
93.00	4684.0
94.00	12919.0
95.00	102336.0
96.00	7567.0
97.00	241.0
102.80	119.0
103.80	496.0
104.80	215.0
105.80	486.0
114.90	128.0
115.90	574.0
116.90	913.0
117.80	460.0
118.80	780.0
127.80	513.0
128.90	289.0
129.80	329.0
130.60	132.0
134.80	188.0
136.90	235.0
140.90	1030.0
142.00	167.0
142.90	1905.0
143.90	110.0
144.90	438.0
145.70	219.0
148.10	227.0
148.90	107.0
149.80	106.0
154.60	208.0
156.80	185.0
158.80	139.0
170.90	246.0
172.00	1114.0
173.00	1090.0
173.90	78896.0
175.00	5786.0
175.90	75280.0
176.90	4763.0
178.00	152.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390

m/z	Abundance
36.00	794.0
37.00	3685.0
38.00	3671.0
39.00	1770.0
39.90	366.0
44.00	1068.0
45.00	875.0
45.90	116.0
47.00	1048.0
47.90	572.0
49.00	3536.0
50.00	15667.0
51.00	4623.0
52.00	356.0
52.90	238.0
54.10	122.0
54.70	244.0
55.20	155.0
56.00	1486.0
57.00	2022.0
57.90	149.0
59.90	1065.0
61.00	4121.0
62.00	4242.0
62.90	4122.0
63.90	694.0
65.00	838.0
66.10	147.0
67.00	309.0
68.00	8900.0
69.00	9020.0
69.90	990.0
71.90	559.0
72.90	4464.0
74.00	15794.0
75.00	48072.0
76.00	4173.0
76.90	725.0
78.00	384.0
78.90	3837.0
79.90	1098.0
80.90	3704.0
81.90	870.0
85.90	139.0
86.90	4402.0
87.90	4110.0
90.90	520.0
92.00	2751.0
93.00	4553.0
94.00	12201.0
95.00	95992.0
96.00	6564.0
97.00	262.0
102.70	105.0
103.80	425.0
104.80	232.0
105.90	486.0
115.90	523.0
116.90	813.0
117.80	324.0
118.80	773.0
127.80	522.0
128.90	244.0
129.90	326.0
130.60	125.0
134.70	163.0
136.80	217.0
140.90	1007.0
142.00	145.0
142.90	1904.0
144.80	517.0
145.70	200.0
148.00	253.0
148.90	116.0
154.80	194.0
156.70	193.0
171.00	221.0
172.00	1079.0
173.00	1080.0
173.90	77192.0
175.00	5357.0
175.90	73000.0
176.90	4610.0
178.00	158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB390