

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
 Data File : VV037795.D
 Acq On : 10 Oct 2024 11:29
 Operator : SY/MD
 Sample : P4360-03
 Misc : 5mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Oct 11 05:12:09 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
 Quant Title : VOC Analysis
 QLast Update : Fri Oct 11 05:10:27 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.529	114	585692	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.780	117	581747	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.178	152	262422	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.278	65	195115	37.949	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	75.900%		
7) Chloroethane-d5	1.532	69	167230	41.903	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	83.800%		
11) 1,1-Dichloroethene-d2	2.056	65	89825	41.817	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.640%		
21) 2-Butanone-d5	3.799	46	155173	84.735	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	84.730%		
24) Chloroform-d	4.243	84	404585	44.230	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	88.460%		
26) 1,2-Dichloroethane-d4	4.937	65	248998	46.506	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.020%		
32) Benzene-d6	4.953	84	798906	43.886	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	87.780%		
36) 1,2-Dichloropropane-d6	5.982	67	252733	43.599	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	87.200%		
41) Toluene-d8	7.236	98	703464	42.616	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	85.240%		
43) trans-1,3-Dichloroprop...	7.551	79	108539	40.307	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	80.620%		
47) 2-Hexanone-d5	8.024	63	92043	75.197	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	75.200%		
56) 1,1,2,2-Tetrachloroeth...	10.146	84	284670	42.265	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	84.540%		
66) 1,2-Dichlorobenzene-d4	11.551	152	269742	48.780	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	97.560%		
Target Compounds						
					Qvalue	
13) Acetone	2.114	43	107381	59.815	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV101024\
Data File : VV037795.D
Acq On : 10 Oct 2024 11:29
Operator : SY/MD
Sample : P4360-03
Misc : 5mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Oct 11 05:12:09 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092624WMA.M
Quant Title : VOC Analysis
QLast Update : Fri Oct 11 05:10:27 2024
Response via : Initial Calibration

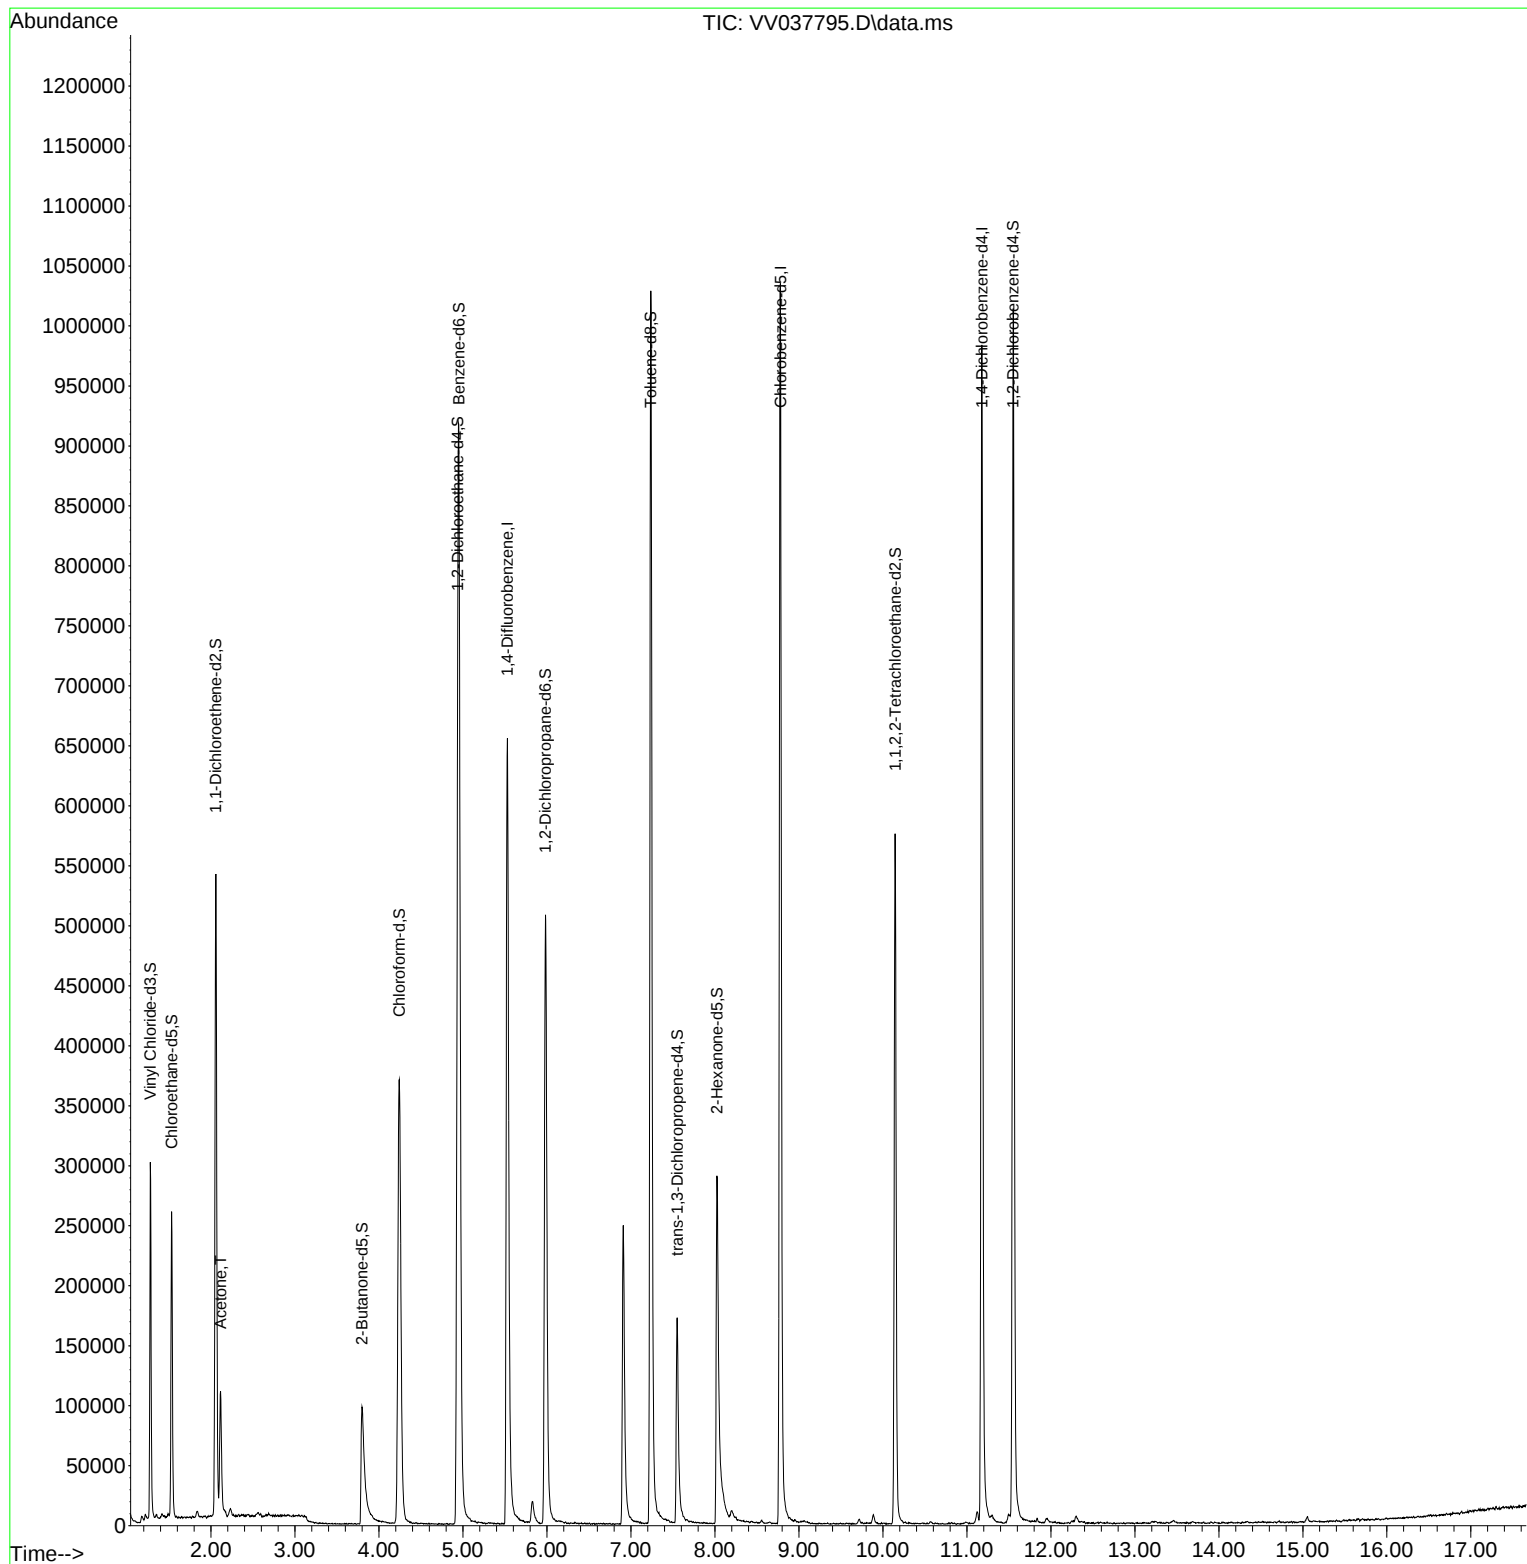

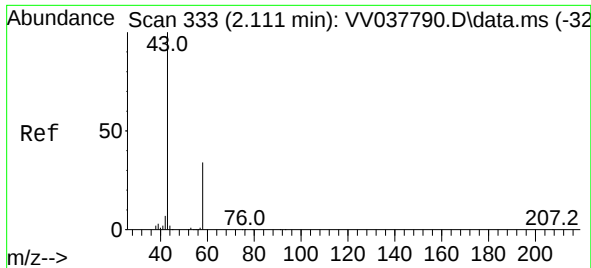

#13

Acetone

Concen: 59.815 ug/L

RT: 2.114 min Scan# 34

Delta R.T. 0.003 min


Lab File: VV037795.D

Acq: 10 Oct 2024 11:29

Instrument :

MSVOA_V

ClientSampleId :

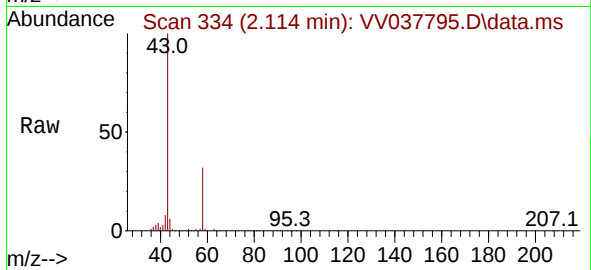

Tgt Ion: 43 Resp: 107381

Ion Ratio Lower Upper

43 100

58 31.8 0.0 66.6

